


(EN) Ameda Platinum® Breast Pump Instructions
English. page 3

(CA) Mode d'emploi du Tire-lait Ameda Platinum
Français. page 11

**(ES) Instrucciones de la Bomba de extracción
Ameda Platinum**
Español página 17

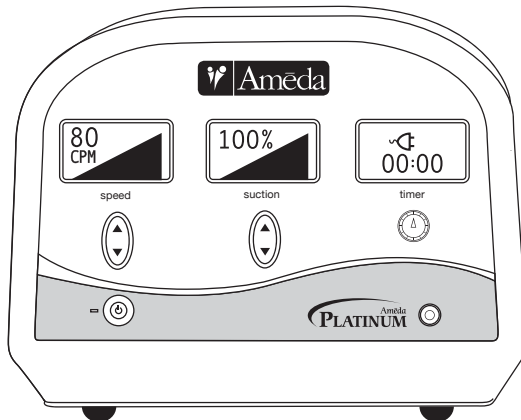

CONTENTS

Important Safeguards	3	Cleaning	7
Intended Use	3	<i>Ameda Platinum Breast Pump</i>	7
Ameda Platinum Breast Pump Diagram	4	<i>For At-Home/End-Users</i>	7
Ameda Platinum Breast Pump Trolley	5	<i>For Hospitals/Rental Stations</i>	7
Set Up and Assembly	6	Troubleshooting	7
<i>Ameda® HygieniKit® Milk Collection System</i>	6	Maintenance	7
<i>Before Every Use</i>	6	Technical Information	7
<i>Single and Dual Pumping</i>	6	Icon Glossary	10
Controls and Displays	6	Product Disposal	10
<i>Using “Up/Down” Buttons</i>	6	Warranty Information	10
<i>Operating the Pump</i>	6		
<i>Setting Suction</i>	6		
<i>Setting Speed</i>	6		
<i>Using Timer</i>	7		
<i>Turning Pump Function Off</i>	7		
<i>Removing Ameda HygieniKit Milk</i>			
<i>Collection System from Breast(s)</i>	7		

IMPORTANT SAFEGUARDS

When using electrical products, especially if children are present, the following basic safety precautions should always be maintained.

READ ALL INSTRUCTIONS BEFORE USING

Danger: To reduce the risk of electrocution:

- Always unplug electrical devices immediately after use.
- Do not use while bathing, showering or swimming.
- Do not place or store where product can fall or be pulled into bathtub, sink or pool.
- Do not place or drop product into water or other liquid.
- Do not reach for electrical product that has fallen into water. Unplug from wall outlet immediately.

Warning: To reduce the risk of burns, electrocution, fire, or injury to persons:

- Never leave product unattended when plugged into electrical outlet.
- Close supervision is necessary when product is used near children or invalids.
- Use product only for intended use as described in this manual.
- Do not use attachments or other milk collection kits other than those recommended by manufacturer.
- Never operate if product has damaged cord or plug, is not working properly, or has been dropped, damaged, or becomes wet.
- Keep cord and all attachments away from heated surfaces.
- Never use while sleeping or drowsy.
- Do not use outdoors with cord.
- Do not operate where aerosol spray products are being used or oxygen is being administered.

Caution: To reduce the risk of fire or chemical burn:

- Do not disassemble or heat above 100°C (212°F).

SAVE THESE INSTRUCTIONS

Intended Use


The Ameda Platinum Breast Pump is intended to facilitate the expression and collection of breast milk from a lactating woman for the purpose of feeding the collected milk to a child.

EN Pump Diagrams


CA Diagrammes du tire-lait

ES Diagramas de extracción


Front View
Vue avant
Vista frontal

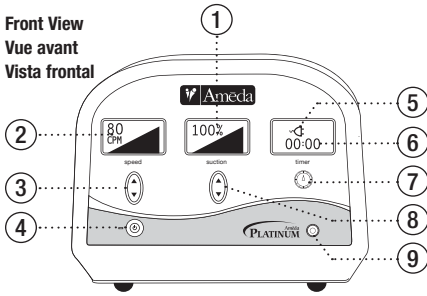

Top View
Vue supérieure
Vista superior

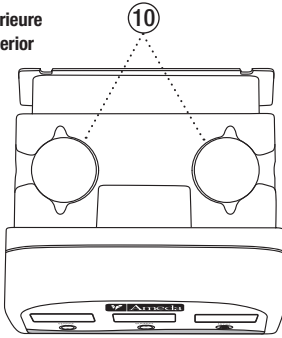


Rear View
Vue arrière
Vista trasera

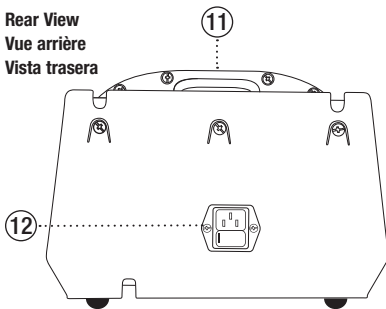

1. Suction Display (Maximum Shown in Percentage)
Affichage de l'aspiration (Maximum illustré en pourcentage)
Pantalla de succión (Se muestra el máximo en porcentaje)
2. Speed Display (Maximum Cycles per minute shown)
Affichage de la vitesse (Maximum des cycles par minute illustré)
Pantalla de velocidad (Se muestran los ciclos máximos por minuto)
3. Speed Control
Contrôle de la vitesse
Control de velocidad
4. Power Button (Turn Pump ON/OFF)
Bouton "Power" (Met le tire-lait en marche/arrêt)
Botón de energía (encender/apagar la bomba [ON/OFF])
5. AC Power Indicator
Indicateur de l'alimentation CA
Indicador de CA
6. Timer Display
Affichage de la minuterie
Pantalla del reloj programador
7. Timer Reset Button
Bouton de réinitialisation de la minuterie
Botón de reinicio del reloj programador
8. Suction Control
Contrôle de l'aspiration
Control de succión
9. Tubing Adapter Port
Pièce d'adaptateur de tube
Puerto del adaptador del tubo
10. Milk Bottle/Breast Flange Holders
Supports de manchon de sein/bouteille de lait
Sujetadores para biberones/embudo
11. Handle
Poignée
Mango
12. AC Power Inlet
Prise d'alimentation secteur
Entrada de CA

Bottom View
Vue du bas
Vista inferior

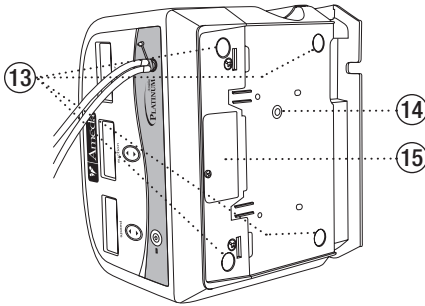

(EN) Attaching the Ameda Platinum Breast Pump to Trolley (if applicable)

Trolley


Trolley is available as an accessory item.

- Attach pump to trolley prior to plugging cord into wall outlet.
- Align front of the Ameda Platinum Breast Pump with wording, "Front of Ameda Platinum Pump and Elite™ Pump" found on top of trolley mounting plate.
- Lower pump onto plate, inserting pump's four feet into holes, one in each corner of trolley mounting plate.
- Locate mounting hole with wording, "Ameda Platinum and Elite Pump Mounting" found on underside of trolley mounting plate.
- Use mounting screw for the Ameda Platinum Breast Pump supplied with trolley to secure pump to trolley base.

Trolley Plate Top View (optional accessory)

Vue supérieure de la plaque de chariot
 (accessoire en option)

Vista superior de la placa de la base (accesorio opcional)

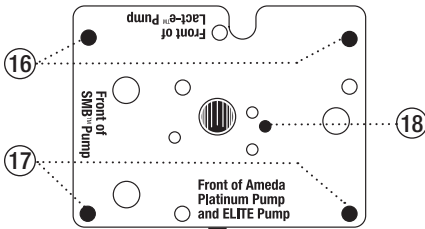

FRONT OF AMEDA PLATINUM PUMP

AVANT DU TIRE-LAIT AMEDA PLATINUM

PARTE DELANTERA DE LA BOMBA AMEDA PLATINUM

- 13. Pump Feet**
 Pied du tire-lait
 Patas de la bomba
- 14. Trolley Mounting Hole**
 Trou de montage du chariot
 Orificio de montaje de la base
- 15. Service Port Door**
 Porte de port de service
 Puerta del puerto de servicio
- 16. Pump Rear Foot Location**
 Emplacement du pied arrière du tire-lait
 Ubicación de las patas traseras de la bomba
- 17. Pump Front Foot Location**
 Emplacement du pied avant du tire-lait
 Ubicación de las patas delanteras de la bomba
- 18. Pump Mounting Hole**
 Trou de montage du tire-lait
 Orificio de montaje de la bomba

Set Up and Assembly

Ameda HygieniKit Milk Collection System

Before Every Use




Always wash hands well with soap and water before handling the Ameda Platinum Breast Pump and Ameda HygieniKit Milk Collection System.

IMPORTANT NOTE: ONLY USE THE AMEDA HYGIENIKIT MILK COLLECTION SYSTEM ON AMEDA ELECTRIC BREAST PUMPS.


Prior to starting pump, assemble and connect the Ameda HygieniKit Milk Collection System, per included instructions. If the Ameda HygieniKit Milk Collection System is sterile, use as is. If not sterile, see the Ameda HygieniKit Milk Collection System cleaning instructions.

Ameda Platinum Breast Pump



Pump

- Attach Ameda supplied grounded power cord to AC power inlet on rear of pump.
- Connect grounded plug to wall outlet.

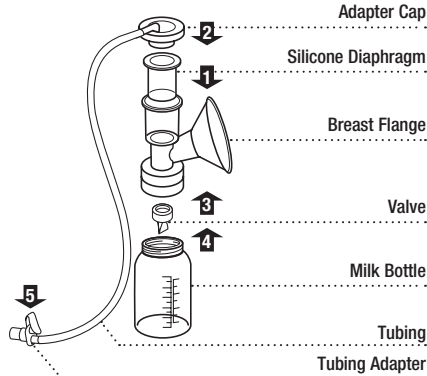


The Ameda HygieniKit Milk Collection System can be used to single or dual pump.




To single pump:

Remove one tube and close tubing adapter.



To dual pump:

Both tubes should be attached to tubing adapter.




- Insert tubing adapter into tubing adapter port.

Controls and Displays


Before starting pump, please note how the controls work.

- Press and **release** controls to increase/decrease settings by increments of 1.
- Press and **hold** controls to increase/decrease settings by increments of 10.





Operating the Pump

- When pump is plugged in, a light will appear next to the Power button.
- Press the Power button. The displays light up. Pump is now ON.
- Pump starts at lowest suction setting (1% or approximately 30 mmHg/4.0 kPa) and maximum speed (80 cpm).



Setting Suction


- Pump starts at lowest suction setting (1% or approximately 30 mmHg/4.0 kPa).
- Center nipple(s) in breast flange(s) and fill breast flange(s) with the breast(s) to create an air seal.
- Press to increase suction until reaching maximum comfort level.
- If discomfort is felt in nipple(s) or breast(s), decrease suction. If discomfort is felt at all suction settings, turn pump off, insert a finger between breast(s) and breast flange(s) to break suction, remove breast flange(s) from breast(s). Discontinue pumping and contact a healthcare provider.



Setting Speed


- Pump starts at fastest speed (80 cpm).
- When milk flows (let-down), press to a slower speed to help drain the breast faster.
- When milk flow slows, press to 60-80 cpm to help start another let-down.
- Repeat as milk flow changes to pump more milk.

NOTE: If "Check Kit" appears in suction window, see Troubleshooting section, on page 7.



Using Timer

- Timer starts when pump is on. Timer displays pumping duration in minutes : seconds.
- Timer can be reset by pressing Timer Reset button.
- Timer and pump automatically turn OFF after 60 minutes.



Turning Pump OFF

- When finished pumping, press and hold Power button to turn pump and timer functions OFF.

Removing Ameda HygieniKit Milk Collection System from Breast(s)

- After pump is OFF, if necessary, insert a finger between breast(s) and breast flanges(s) to break suction.
- Remove breast flanges(s) from breast(s).

Cleaning the Ameda Platinum Breast Pump

For At-Home/End-Users

After each pumping, wipe the Ameda Platinum Breast Pump with clean, damp cloth.

For Hospitals/Rental Stations

Clean between users. Wearing disposable gloves, wipe the Ameda Platinum Breast Pump with damp disposable cloth using hospital approved antibacterial cleaner, such as CaviCide™.

Troubleshooting

Pump does not turn ON

- Ensure proper power cord connection to pump.
- Ensure grounded plug connection to electrical outlet.
- Ensure outlet has power.

Unable to adjust speed

- Ensure pump function is ON.
- Ensure "Check Kit" is not shown in suction display window.

Unable to adjust suction

- Ensure pump function is ON.
- Ensure "Check Kit" is not shown in suction display window.

Low or no suction

- Ensure "Check Kit" is not shown in suction display window.
- Check breast flange for adequate seal against breast.
- Check that the Ameda HygieniKit Milk Collection System is properly assembled.
- Check that adapter cap is firmly snapped onto top of breast flange.
- Ensure silicone diaphragm is in place inside top of breast flange.
- Ensure tubing adapter is properly fitted into tubing adapter port on pump.
- Inspect valve for stretching or tears. If seen, replace valve.
- Ensure valve is pushed firmly into place in lower portion of breast flange.
- Ensure one side of tubing adapter is closed when single pumping.

"Check Kit" error message appears

- Ensure tubing adapter is properly fitted into tubing adapter port on pump.
- Ensure one side of tubing adapter is closed when single pumping.
- Check that adapter cap is firmly snapped onto top of breast flange.
- Ensure silicone diaphragm is in place inside top of breast flange.
- Check tubing and silicone diaphragm to ensure that parts are free of defects.
- Check tubing is firmly attached to adapter cap.

"Service Required" error message appears

- Call your local distributor. For listing of distributors worldwide, visit www.ameda.com.

The Ameda Platinum Breast Pump should be serviced only by Ameda, Inc. or authorized Service Centers approved by Ameda, Inc.

Maintenance

It is recommended the Ameda Platinum Breast Pump be inspected at least once every year to include the following:

- Visually check pump housing for cracks, breakage, or damage and ensure Pump Feet are present.
- Visually check for power cord damage.
- Check for proper operation of controls and buttons.
- Check there are no missing screws.
- Check cover is present on Service Port Door.
- Check Tubing Adapter Port is free from obstruction.

Quick Functional Check

The following checks/tests should be performed prior to use by a new user:

- Visual checks for power cord damage.
- Check for abnormal noise.
- Check for proper operation of controls and buttons.

Service Port

- Do not open Service Port Door on bottom of the Pump.
- Do not connect any equipment to the service port when operating the pump.
- Service port is to be accessed only by authorized Service Centers approved by Ameda, Inc.

Replacing Detachable Power Cord:

- Power cord is detachable from power inlet.
- If power cord condition is in doubt, only replace with Ameda supplied 3-conductor cord equipped with protective ground conductor.

Technical Information

Protection Class 1, Type B

Power Supply:

Operating Input Voltage 100 VAC to 240 VAC

Operating Frequency 50/60Hz

Input Power 80VA

Fuse Rating Quick Acting (F), 2.5A, 250V, 5 x 20mm

Power Cord: Use only Ameda supplied power cord

For North America, use Ameda 24502059

Minimum Voltage Rating: 125V

Minimum Current Rating: 10A

Plug Type: IEC 60320 C13 (Hospital Grade)

Maximum Length: 10 feet (3.05m)

Cord Type: 3x18AWG, rated VW-1, 105C

Jacket Type: SJT or SJTW

Certification: UL Listed (ELBZ)

Operation:

ISO 10079-1, Intermittent Suction, Medium Vacuum

Suction: Shown in percentage of full scale suction 1%-100%; (approximately 30 mmHg to 250 mmHg/4.0 kPa to 33.3 kPa)

Speed: 30 to 80 cycles per minute (cpm)

Operational Conditions: Pump

Temperature +53°F (+12°C) to +93°F (+34°C)
 Relative Humidity 20% to 70%
 Atmospheric Pressure 0.82atm (83.1 kPa) to 1.05atm (106.4kPa)

Transport and Storage Conditions: Pump

Temperature -10°F (-23°C) to +130°F (+54°C)
 Relative Humidity 20% to 90%
 Atmospheric Pressure 0.82atm (83.1 kPa) to 1.05atm (106.4kPa)

Weight: Approximately 9.75 lbs. (approximately 4.42 kg)

Dimensions: Length 9.75 in. (24.7 cm)/Width 10.5 in. (26.7 cm)/Height 8.0 in. (20.3 cm)

Standards:

E325189 MEDICAL EQUIPMENT
 WITH RESPECT TO ELECTRIC SHOCK,
 FIRE AND MECHANICAL HAZARDS ONLY
 IN ACCORDANCE WITH
 IEC60601-1: 1988 + A1:1991 + A2:1995,
 IEC60601-1-2, CAN/CSA C22.2 No. 601.1-M90

MEDICAL ELECTRICAL EQUIPMENT needs special precautions regarding EMC and needs to be installed and put into service according to the EMC provided in these Instructions for use.

Portable and mobile RF communications equipment can affect MEDICAL ELECTRICAL EQUIPMENT.

Warning: The use of ACCESSORIES, transducers and cables other than those specified, with the exception of transducers and cabled sold by the MANUFACTURER of the

Ameda Platinum Breast Pump as replacement parts for internal components, may result in increased EMISSIONS or decreased IMMUNITY of the Ameda Platinum Breast Pump.

Warning: The Ameda Platinum Breast Pump should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the Ameda Platinum Breast Pump should be observed to verify normal operation in the configuration in which it will be used.


Guidance and manufacturer's declaration – electromagnetic emissions		
The Ameda Platinum Breast Pump is intended for use in the electromagnetic environment specified below.		The customer or the user of the Ameda Platinum Breast Pump should assure that it is used in such an environment.
Emissions test	Compliance	Electromagnetic environment – guidance
RF emissions CISPR 11	Group 1	The Ameda Platinum Breast Pump uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The Ameda Platinum Breast Pump is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations/flicker emissions IEC 61000-3-3	Complies	

Guidance and manufacturer's declaration – electromagnetic immunity			
The Ameda Platinum Breast Pump is intended for use in the electromagnetic environment specified below.		The customer or the user of the Ameda Platinum Breast Pump should assure that it is used in such an environment.	
IMMUNITY test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Electrostatic discharge (ESD) IEC 61000-4-2	± 6 kV contact ± 8 kV air	± 6 kV contact ± 8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	± 2 kV for power supply lines/± 1 kV for input/output lines	± 2 kV for power supply lines/± 1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	± 1 kV line(s) to line(s) ± 2 kV line(s) to earth	± 1 kV line(s) to line(s) ± 2 kV line(s) to earth	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<5% U _T (>95% dip in U _T) for 0,5 cycle 40% U _T (60% dip in U _T) for 5 cycles 70% U _T (30% dip in U _T) for 25 cycles <5% U _T (>95% dip in U _T) for 5 s	<5% U _T (>95% dip in U _T) for 0,5 cycle 40% U _T (60% dip in U _T) for 5 cycles 70% U _T (30% dip in U _T) for 25 cycles <5% U _T (>95% dip in U _T) for 5 s	Mains power quality should be that of a typical commercial or hospital environment. If the user of the Ameda Platinum Breast Pump requires continued operation during power mains interruptions, it is recommended that the Ameda Platinum Breast Pump be powered from an uninterruptible power supply.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE: U _T is the a.c. mains voltage prior to application of the test level.			

Guidance and manufacturer's declaration – electromagnetic immunity

The Ameda Platinum Breast Pump is intended for use in the electromagnetic environment specified below. The

customer or the user of the Ameda Platinum Breast Pump should assure that it is used in such an environment.

IMMUNITY test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Conducted RF IEC 61000-4-6 Radiated RF IEC 61000-4-3	3 Vrms 150 kHz to 80 MHz 3 V/m 80 MHz to 2,5 GHz	3 Vrms 3 V/m	<p>Portable and mobile RF communications equipment should be used no closer to any part of the Ameda Platinum Breast Pump, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p>Recommended separation distance $d = 1,2\sqrt{P}$</p> <p>$d = 1,2\sqrt{P}$ 80 MHz to 800 MHz $d = 2,3\sqrt{P}$ 800 MHz to 2,5 GHz</p> <p>Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,^a should be less than the compliance level in each frequency range.^b</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> 

NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

^a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic

site survey should be considered. If the measured field strength in the location in which the Ameda Platinum Breast Pump is used exceeds the applicable RF compliance level above, the Ameda Platinum Breast Pump should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the Ameda Platinum Breast Pump.

^b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

Recommended separation distances between portable and mobile RF communications equipment and the Ameda Platinum Breast Pump

The Ameda Platinum Breast Pump is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the Ameda Platinum Breast Pump can help prevent electromagnetic interference by maintaining a minimum

distance between portable and mobile RF communications equipment (transmitters) and the Ameda Platinum Breast Pump as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter m		
	150 kHz to 80 MHz $d = 1,2\sqrt{P}$	80 MHz to 800 MHz $d = 1,2\sqrt{P}$	800 MHz to 2,5 GHz $d = 2,3\sqrt{P}$
0,01	0,12	0,12	0,23
0,1	0,38	0,38	0,73
1	1,2	1,2	2,3
10	3,8	3,8	7,3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.



Icon Glossary

Type B Applied Part



Connected to Wall Outlet



% of Full Scale Suction 1% -100%; (approximately 30mmHg to 250mmHg/4.0kPa to 33.3kPa)



Cycles Per Minute (30-80 cpm)



Timer Display



Consult Instructions For Use



Fuse

IPX1

Liquid ingress classification



E325189 MEDICAL EQUIPMENT WITH RESPECT TO ELECTRIC SHOCK, FIRE AND MECHANICAL HAZARDS ONLY IN ACCORDANCE WITH IEC60601-1: 1988 + A1:1991 + A2:1995, IEC60601-1-2, CAN/CSA C22.2 No. 601.1-M90



Fragile




Protect from sunlight



Keep Dry



Transport/Storage



Operation

CE 0086



EMERGO EUROPE

Molenstraat 15
2513 BH, The Hague
The Netherlands
Phone: +31.70.345.8570
Fax: +31.70.346.7299



Ameda, Inc.
485 Half Day Road
Buffalo Grove, IL 60089
USA

Product Disposal

This product contains electrical and electronic equipment.



1. The internal components of this product may contain hazardous materials. Dispose of this product according to local or regional waste administration systems and regulations.

2. Do not dispose of as unsorted municipal waste.

3. For further information regarding the environmental performance of this product please visit our website www.ameda.com.

Limited Warranty

The Ameda Platinum Electric Breast Pump ("Product") is warranted to the original user--whether institutional or individual ("First User")--only.

From the date of First User's purchase of this Product, Ameda, Inc. ("Ameda") warrants the Product to the First User against defects in material or workmanship for three years on the pump mechanism. Ameda's sole obligation under this limited warranty shall be to repair or replace, at Ameda's option, any Product that is determined to be defective by Ameda and determined to be covered by this express limited warranty. Repair or replacement under this limited warranty is the sole and exclusive remedy of the First User. Proof of purchase in the form of a receipted invoice or bill of sale evidencing that the Product is within the warranty period must be presented to obtain warranty service. This limited warranty is extended by Ameda ONLY to the First User and is not assignable or transferable. For warranty service contact Ameda at 1.866.99.AMEDA(263332).

EXCEPT TO THE EXTENT PROHIBITED BY APPLICABLE LAW, ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE ON THE PRODUCT IS HEREBY DISCLAIMED. AMEDA SHALL NOT BE LIABLE FOR ANY INCIDENTAL, CONSEQUENTIAL, SPECIAL OR PUNITIVE DAMAGES OF ANY KIND FOR BREACH OF THE EXPRESS LIMITED WARRANTY ON THE PRODUCT OR ANY WARRANTY IMPLIED BY OPERATION OF LAW, OTHER THAN THE EXPRESS LIMITED WARRANTY SET FORTH ABOVE, THERE ARE NO OTHER WARRANTIES THAT ACCOMPANY THIS PRODUCT AND ANY ORAL, WRITTEN OR ANY OTHER EXPRESS REPRESENTATION OF ANY KIND IS HEREBY DISCLAIMED.

Non-Applicability of Warranty

The above warranty shall not apply to consumable materials and attachment to the Product. These include:

- (i) the power cord; and
- (ii) the Ameda HygieniKit Milk Collection System (sold separately).

In addition to any other limitations on the warranty discussed above, the warranty shall expire and be of no force or effect upon the occurrence of any of the following:

- (i) the cause of damage to the Product is due to improper handling or use
- (ii) the Product is not properly maintained by the First User, as determined by Ameda
- (iii) non-Ameda approved accessories or spare parts are used with the Product, as determined by Ameda
- (iv) the Product is repaired by a non-approved Ameda service provider.

If any of the above occurs, Ameda shall not be responsible for damage to the Product, parts thereof or injuries arising therefrom, either directly or indirectly. The warranty set forth above replaces all prior warranties with respect to the purchased Product, whether in writing or otherwise.

Outside the United States: Call your local distributor or location where you purchased the Product. For a listing of distributors in your country, please visit www.ameda.com.

CE 0086



EMERGO EUROPE

Molenstraat 15
2513 BH, The Hague
The Netherlands
Phone: +31.70.345.8570
Fax: +31.70.346.7299



Ameda, Inc.
485 Half Day Road
Buffalo Grove, IL 60089
USA



MOM INSPIRED. HOSPITAL TRUSTED.

Distributed in USA by:

Ameda, Inc.

485 Half Day Road
Buffalo Grove, IL 60089
1.866.99.AMEDA (26332)

Distributed in Canada by:

Distribué au Canada par:

Mothers Choice Products Ltd.

2133-11871 Horseshoe Way
Richmond, BC V7A 5H5
1.800.604.6225

Distributed in Australia by:

Advantage Health Care

34 Percy Street
Mordialloc VIC 3195
61 (3) 9580 9288

Distribution in other countries:

For product information or feedback, visit

www.ameda.com

Ameda, Ameda Platinum, Elite, SMB,
Lact-e, HygieniKit and associated logos
are trademarks of Ameda, Inc.

Any other trademarks, brand or images appearing herein
are property of their respective owners and are used
herein with expressed or implied permission.

©2013 Ameda, Inc.

25708696-0813