

# ARTROMOT®-K3



## **Service Manual** (New Generation)

Starting from Serial number 3000

## Table of contents

1. History	2
2. Purpose	2
3. General	2
4. Packing and unpacking	4
5. Block diagram of electronic parts	4
6. Bill of material for service parts	5
7. How to perform the repair	9
8. Explosion drawing part 1	10
9. Explosion drawing part 2	11
10. Checklist for Function- and Safetytest	12

## 1. Historie History

Revision	Date	Name	Change
1	17.09.2001	M. Nunnenmacher	Initial Release
2	19.09.2001	M. Nunnenmacher	Pos. 4.8 new partnumber 0.0013.104
3	15.10.2001	M. Nunnenmacher	Pos. 1.9, 1.15, 1.16 new partnumber
4	6.11.2001	M. Nunnenmacher	Update reference run, new packaging
5	15.01.2002	M. Nunnenmacher	Update Pos. 3.13, 3.45, 4.3, 4.5, Safetytest
6	06.02.2002	M. Nunnenmacher	Update Pos. 3.12 Labeled casting
7	27.03.2002	M. Nunnenmacher	Update Pos. 1.1 part-number power cord
8	21.10.2002	S. Herr	Update for all electronic parts, explosion drawings and reference run
9	02.06.2003	S. Herr	Update Pos. 2.10 explosion drawing
10	05.04.2004	S. Herr	Update Pos.1.6, function test

## 2. Purpose

This service manual is to perform some repairs on ARTROMOT®-K3 products. Repair and maintenance work may only be carried out by authorised persons, as otherwise all warranty services and liabilities shall be void. It is not allowed to utilize any other spare part which is not mentioned in chapter 6.

## 3. General

### 3.1 Electronic and cable

- Electronic devices as hand-held programming unit, motor electronics and spiral cable are not interchangeable with ARTROMOT®-K3 serial number < 3000.
- Make sure that the characteristic values of your power supply correspond to the voltage and frequency data indicated on the power adapter.
- Error possibilities, showed by the Hand-held programming unit:

#### DEVICE NEEDS

REFERENCE RUN: The reference run was interrupted or the electronics were replaced.  
-> Perform a reference run. See chapter 7.4

POTENTIOMETER: Potentiometer shows incorrect value  
-> Check plug connection, replace potentiometer if persistent

POTENTIOM. CABLE: Spiral cable for knee case defective  
-> Replace spiral cable for knee case (Pos. 5.9), check plug connection

MOTOR DRIVER: Motor electronics defective  
-> Replace motor electronics (see chapter 7.3) if persistent

OVER CURRENT: Motor power to high  
-> Replace motor electronics (see chapter 7.3) if persistent

UNWANTED BUSY: Motor control unit is not answering  
-> Hand-held programming unit, motor electronics or spiral cable of the hand-held programming unit defective

CPM MEMORY RAM: Memory fault in the motor control unit  
-> Replace motor electronics (see chapter 7.3) if persistent

CPM MEMORY ROM: Memory fault in the motor control unit  
-> Replace motor electronics (see chapter 7.3) if persistent

**COMMUNICATION:** Communication problem between hand-held programming unit and the motor control unit  
-> Hand-held programming unit, motor electronics or spiral cable of the hand-held programming unit defective

**CPM-DEVICE ERROR:** General mistake in the motor control unit  
-> Replace motor electronics (see chapter 7.3) if persistent

**MOT. EN. TIMEOUT:** Motor can not be activated  
-> Check motor electronics and plug connection for motor. Replace motor electronics (see chapter 7.3) and spiral cable of the hand-held programming unit if persistent

**INVALID PARAMET.:** Motor control unit received a wrong parameter  
-> Hand-held programming unit, motor electronics or spiral cable of the hand-held programming unit defective

**STOP RELEASE ERR:** Stop line can not be released  
-> Remove hand-held programming unit or spiral cable (see chapter 7.2) if persistent

**UNEXP. MOT. STOP:** Motor stopped unexpectedly  
-> Motor electronics or connecting line to motor defective

**MOTOR DISABLED:** Motor is disconnected  
-> Motor electronics or connecting line to motor defective

**MOTOR ERROR:** Motor is not turning  
-> Check motor cable and motor. Replace motor electronics (see chapter 7.3) if persistent

**RTC INIT ERROR:** Hand-held programming unit defective  
-> Replace hand-held programming unit (see chapter 7.2) if persistent

**RTC COM ERROR:** Communication problem with hand-held programming unit  
-> Replace hand-held programming unit (see chapter 7.2) if persistent

**RTC ERROR:** Hand-held programming unit defective  
-> Replace hand-held programming unit (see chapter 7.2) if persistent

**RANGE EXCEEDED:** Potentiometer shows a value out of range  
-> Replace Potentiometer and/ or spiral cable

**UNKNOWN CPM ERR.:** Unknown error in the motor control unit  
-> Replace motor electronics (see chapter 7.3) if persistent

**UNDEFINED ERROR:** Undefined error  
-> Hand-held programming unit, motor electronics or spiral cable of the hand-held programming unit defective

**CPM 24V SUPPLY:** 24V supply in motor control out of range  
-> Check power supply. Replace motor electronics (see chapter 7.3) if persistent

**CPM 3.3V SUPPLY:** 3.3V supply in motor control out of range  
-> Replace motor electronics(see chapter 7.3) if persistent

**HS 24V SUPPLY:** 24V supply in hand-held programming out of range  
-> Replace hand-held programming unit or spiral cable if persistent

**HS 5V SUPPLY:** 5V supply in hand-held programming unit out of range  
-> Replace hand-held programming unit if persistent

**HS 3.3V SUPPLY:** 3.3V supply in hand-held programming unit out of range  
-> Replace hand-held programming unit if persistent

### 3.2 Mechanics

■ The Threaded spindle is not interchangeable with ARTROMOT®-K3 serial number < 3000.

■ Do not loosen the knurled handles completely for any adjustment. For operation or transport, make sure that the knurled handles are tight.

### 3.3 Others



■ Do not clean the casing or the support with grease or oil.

■ Do not utilize any solvent for cleaning the ARTROMOT®-K3.


#### 4. Packing and unpacking

Preparations for transport the ARTROMOT®-K3 has to be done.

- The first step is to move the device in a position of EXTENSION = 10 degrees.
- Remove the power adapter and put this part in a separate pad.
- Loosen the 2 knurled handles (Pos. 6.2), pull out the ankle joint (Pos. 4.x) and put the ankle joint just the other way round.
- Protect the hand-held programming unit against vibration and damage and put the hand-held programming unit in a separate pad.
- Make sure, that all of the knurled handles are tight.
- For transportation, use the original packaging.

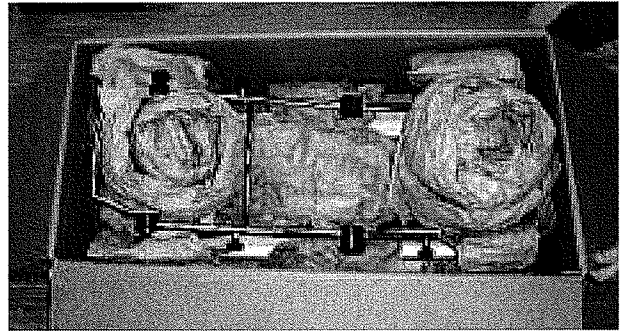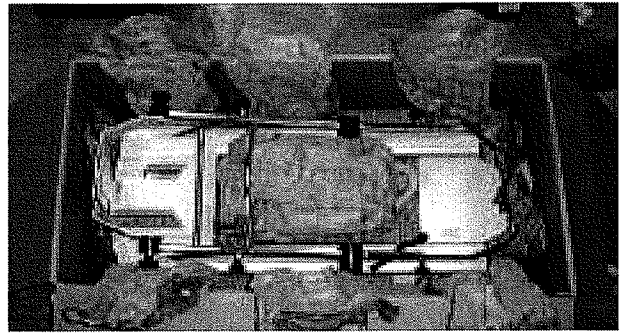

#### 5. Block diagram of electronic parts

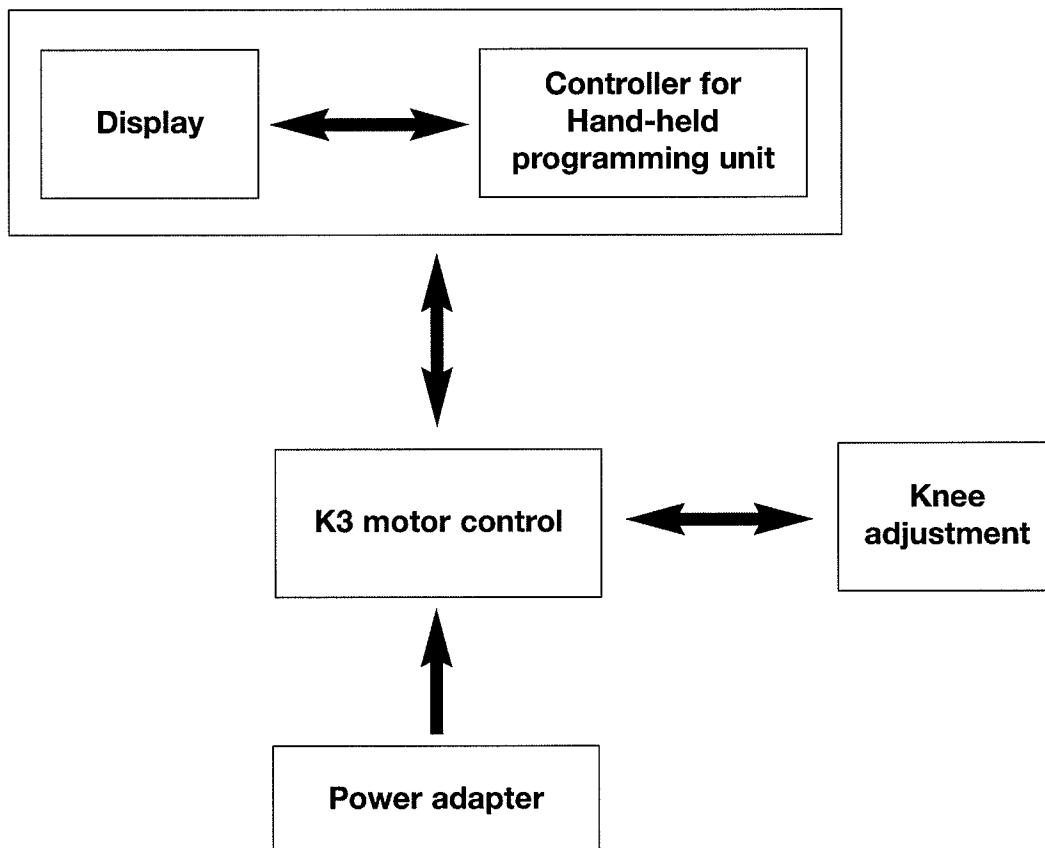

## 6. Bill of material for service parts

Position	Description	Order-Number
<b>1.0</b>	<b>Electronics</b>	
1.1	Power adapter 115V / 230V	0.0031.107W
	Power cord USA - version to 0.0031.107W	0.0032.011
	Power cord EU - version to 0.0031.107W	0.0034.118
1.2	Hand-held programming unit	0.0032.113
1.4	Rubber mat	2.0031.195
1.5	Sheet metal cover	2.0032.136
1.6	Motor electronics	2.0032.900RevB
1.7	Fantype lock washer	DIN6798AD3,2vz
1.8	Screw thread slab	962.903
1.9	Screw	LIKOM4x8A2
1.11	Hexagonal nut	DIN934M3vz
1.13	Cloth white	0.0010.144
1.14	Sticker	2.0013.362
1.15	Phillips screw	9B2.013
1.16	Cover top black	9B2.013
1.17	Spiral cable	2.0032.137
1.18	Holding clip	0.0031.004
1.19	Countersunk screw	DIN7991M3x10sw
1.20	Flat connector	0.0013.125
1.21	Washer	DIN125D3,2vz
1.22	Wire-Set Motor	2.0032.139
1.23	Pan head screw	DIN912M3x6A2
1.24	Washer	2.0013.317
<b>2.0</b>	<b>Exterior underframe</b>	
2.1	Right profile	2.0032.107
2.2	Left profile	2.0032.106
2.3	Right rubber mat	2.0032.116
2.4	Left rubber mat	2.0032.115
2.5	Lip	2.0031.193
2.6	Interior slit	2.0032.113
2.7	Interior slit	2.0032.128
2.8	Right cover	2.0032.105
2.9	Left cover	2.0032.104
2.10	Shaft bearing	2.0031.112
2.11	DU collar	0.0031.110

2.12	Interior slit	2.0031.197
2.14	Exterior slit	2.0032.114
2.15	Exterior slit	2.0032.114
2.16	Bottom plate	2.0032.108
2.17	Attachment plate femur bow	2.0032.101
2.18	Attachment plate femur bow	2.0032.100
2.19	Thread plate M6	962.901
2.20	Pan head screw	DIN912M6x8A2
2.21	Pan head screw	DIN7984M5x25A2
2.22	Countersunk screw	DIN7991M4x8A2
2.23	Cylinder pin	DIN6325D5x10
2.24	Shell nut	0.0032.122
2.25	Countersunk screw	DIN7991M6x10A2
2.26	Sping wire	0.0031.300
2.27	Band white	2.0020.163
2.28	Cloth black	0.0032.110
2.29	Implementation spout	0.0031.145

### **3.0 Drive technology**

3.1	Motor including transmission	0.0031.100
3.2	Right slide	2.0031.108
3.3	Left slide	2.0031.109
3.4	Threaded spindle	2.0032.138
3.5	Rubber ring	2.0031.176
3.7	Rubber plate	2.0028.170
3.8	Motor plate	2.0031.156
3.9	Spline shaft drive	2.0031.181
3.10	Toothed belt	0.0031.130
3.11	Toothed lock washer drive	2.0031.180
3.12	Labeled Casing	2.0032.032
3.13	Bearing plate left	2.0031.165
3.14	Rubber plate	2.0031.102
3.15	Sheet metal	2.0031.115
3.17	Ball bearing	910.008
3.18	Rubber ring	2.0031.105
3.19	Rubber disk	2.0031.104
3.20	Joint plate	2.0031.113
3.22	Covering plate	0.0028.105
3.23	Ring	0.0028.106
3.24	Split rivet	0.0031.136
3.25	Wire-Set power supply	2.0032.140
3.26	Retaining ring	DIN471A8x0,8
3.27	Rubber buffer	0.0031.109

3.28	Spacer sleeve	0.0031.104
3.29	Pin	2.0031.188
3.30	Countersunk screw	DIN7991M5x20vz
3.31	Screw thread pin	DIN916M4x4sw
3.32	Screw thread pin	DIN914M4x4sw
3.33	Countersunk screw	DIN7991M4x10vz
3.34	Hexagonal nut	DIN934M5vz
3.35	Pan head crew	DIN912M5x6vz
3.36	Countersunk screw	DIN7991M5x25A2
3.37	Countersunk screw	DIN7991M5x55vz
3.38	Countersunk screw	DIN7991M5x16vz
3.39	Bearing plate right	2.0031.103
3.50	Countersunk screw	DIN7991M4x16vz
3.51	Pan head screw	DIN912M4x12vz
3.53	Spindle nut	2.0032.141

#### **4.0 Ankle joint**

4.1	Ankle joint bowl	2.0031.120
4.2	Base plate	2.0031.170
4.3	Knurled handle	GN534-40-M6-10sw
4.4	Washer	DIN9021D6,4vz
4.5	Washer	0.0031.111
4.6	Washer	0.0031.142
4.7	Screw rosette	0.0031.137
4.8	Spacer sleeve	0.0013.104
4.9	Sleeve nut	2.0031.178
4.10	Fastening band	0.0031.144
4.11	Rigid pipe	2.0031.117
4.12	Knurled handle	2.0031.031
4.13	Washer	DIN7349D6,4vz
4.14	Hinge box	2.0031.119
4.15	Washer	2.0031.118
4.16	Countersunk screw	DIN7991M5x8A2
4.17	Cylinder pin	DIN7D4x20A2
4.18	Nut	0.0031.108
4.19	Nut	0.0031.105

#### **5.0 Knee case**

5.1	Knee case	2.0032.125
5.2	Retaining ring	DIN471A10x1
5.3	Bearing shell	2.0032.122

5.4	Washer	2.0032.123
5.5	Shim	DIN988D10x16x0,1
5.6	Knee case	2.0032.119
5.7	Knee case (Poti)	2.0032.121
5.8	Knee electronics	0.0031.121
5.9	Spiral cable for knee case	0.0031.122
5.10	Lid potentiometer	2.0031.189
5.11	Shaft	2.0032.120
5.12	Countersunk screw	DIN7991M4x12A2
5.13	Countersunk screw	DIN7991M4x20A2
5.15	Screw thread pin	DIN913M4x8sw
5.16	Washer	2.0013.231
5.17	Shim	DIN988D10x16x0,3

## 6.0 Femur bow

6.1	Femur bow	2.0032.001
6.2	Knurled handle	GN534-32-M6-10
6.3	Right pipe thigh	2.0032.004
6.4	Left pipe thigh	2.0032.006
6.5	Stop bow femur adjustment	2.0032.127
6.6	Support	2.0032.005
6.7	Washer	DIN125D2,2A2
6.8	Washer	DIN125D3,2A2
6.9	Hexagonal nut	DIN934M2A2
6.10	Pin	DIN1481D3x16A2
6.11	Sticker precaution	0.0031.146
6.12	Sticker precaution	0.0031.147

## Patient kits

No illustration	Patient kit fleece	2.0032.155
No illustration	Patient kit cool-quilt	2.0032.155B



## 7. How to perform the repair

### 7.1 How to remove the casing (Pos. 3.12)


- Move the ARTROMOT®-K3 in a position of approximately 110 degrees.
- Turn the power OFF at the ARTROMOT®-K3 and remove the power adapter.
- Hit the 4 pins of the split rivet (Pos. 3.24) inwards.
- Remove the 2 covering plates (Pos. 3.22)
- Loosen the 2 countersunk screws (Pos. 3.50) and remove the casing.
- Remove the 4 pins of the split rivet, which are inside the casing.
- If you have exchanged any of the printed circuit boards including the knee electronics and the hand held programming unit or any parts of the drive technology (Pos. 3.x), you have to perform a reference run. See chapter 7.4
- Finally, a function- and safetytest has to be performed.

### 7.2 How to exchange the hand-held programming unit (Pos. 1.2)

- Remove the casing. See chapter 7.1
- Pull out the connector of the hand held programming unit.  
**Attention:** Use your ESD (Electro Static Discharge)-equipment.
- Put in the connector of the new hand held programming unit.
- Rebuild the casing.
- Perform a reference run. See chapter 7.4
- Finally, a function- and safetytest has to be performed.

### 7.3 How to exchange the motor electronics (Pos. 1.6)

- Remove the casing. See chapter 7.1
- Pull out the required cables at the printed circuit board (Pos. 1.6)  
**Attention:** Use your ESD (Electro Static Discharge)-equipment.

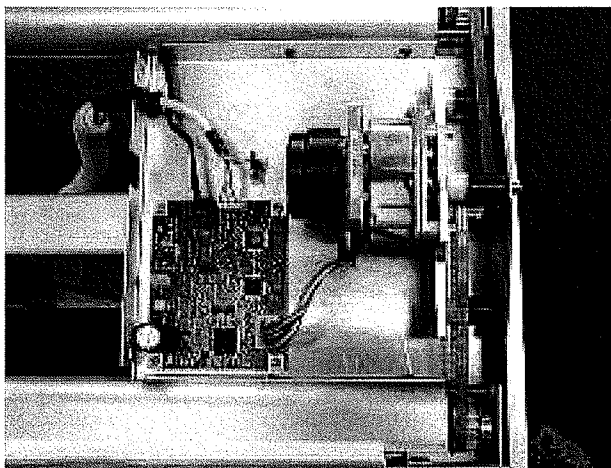

- Exchange the defect printed circuit board.
- Put in the cables at the same position. (Pay attention to the code)

- Rebuild the casing.
- Perform a reference run. See chapter 7.4
- Finally, a function- and safetytest has to be performed.

### 7.4 How to perform a reference run.

- Adjust a maximum femur length (red Point), a minimum lower leg length and the middle position of the foot rotation.
- Under special functions select the operation REFERENCE RUN by using „+“ and „-“. Press „SET“ for five seconds.

The display shows: REFERENCE RUN (flashing for 5 sec.)  
FOR SERVICE ONLY

Then the display shows: REFERENCE RUN  
ENTER KEY

- To start the reference run press „+“ and „-“ at the same time. While the reference run is in progress the display shows: PERFORMING R-RUN  
PLEASE WAIT
- The reference run starts automatically and will take up to 10 minutes. The ARTROMOT®-K3 will reach both points of the mechanical stud (first minimum at EXTENSION afterwards maximum at FLEXION).  
Now the ARTROMOT®-K3 moves between 0 to 110 degrees or parts of this range with different speed and will stop at a position of 0 degrees. After the ARTROMOT®-K3 stops the display will show: REFERENCE RUN  
SUCCESSFUL

The ARTROMOT®-K3 is now ready for operation.  
Finally, a function- and safetytest has to be performed.


#### **Attention:**

If the reference run was interrupted the display shows:  
REFERENCE RUN  
INTERRUPTED (The ARTROMOT®-K3 stops)


If you try to start the ARTROMOT®-K3 the display will show:  
DEVICE NEEDS  
REFERENCE RUN (The ARTROMOT®-K3 is inoperable)

Performe a reference run.

## 8. Explosion drawing part 1

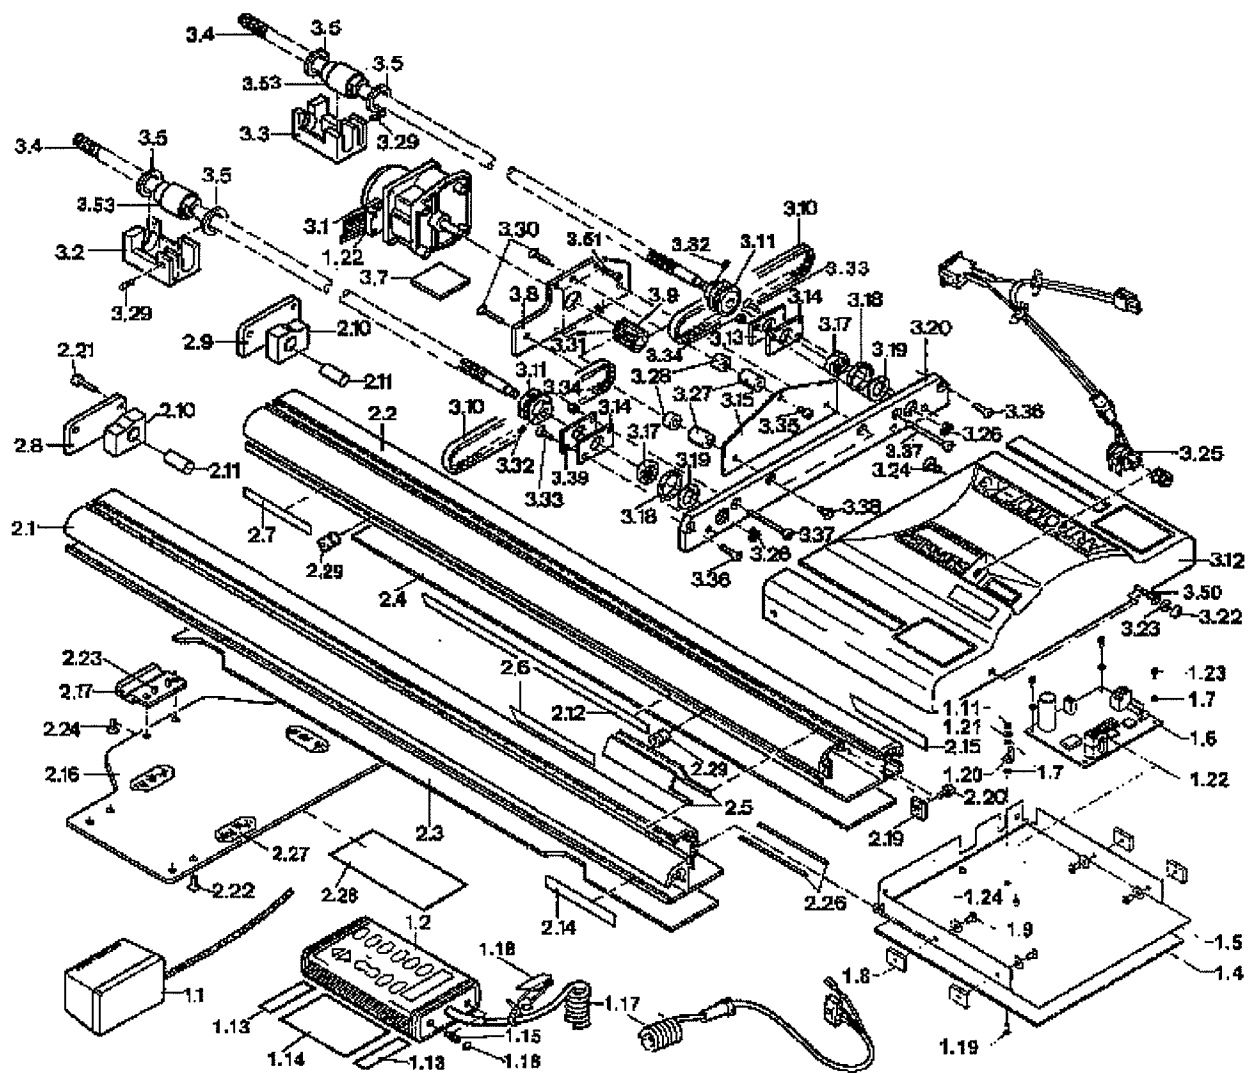

## 9. Explosion drawing part 2

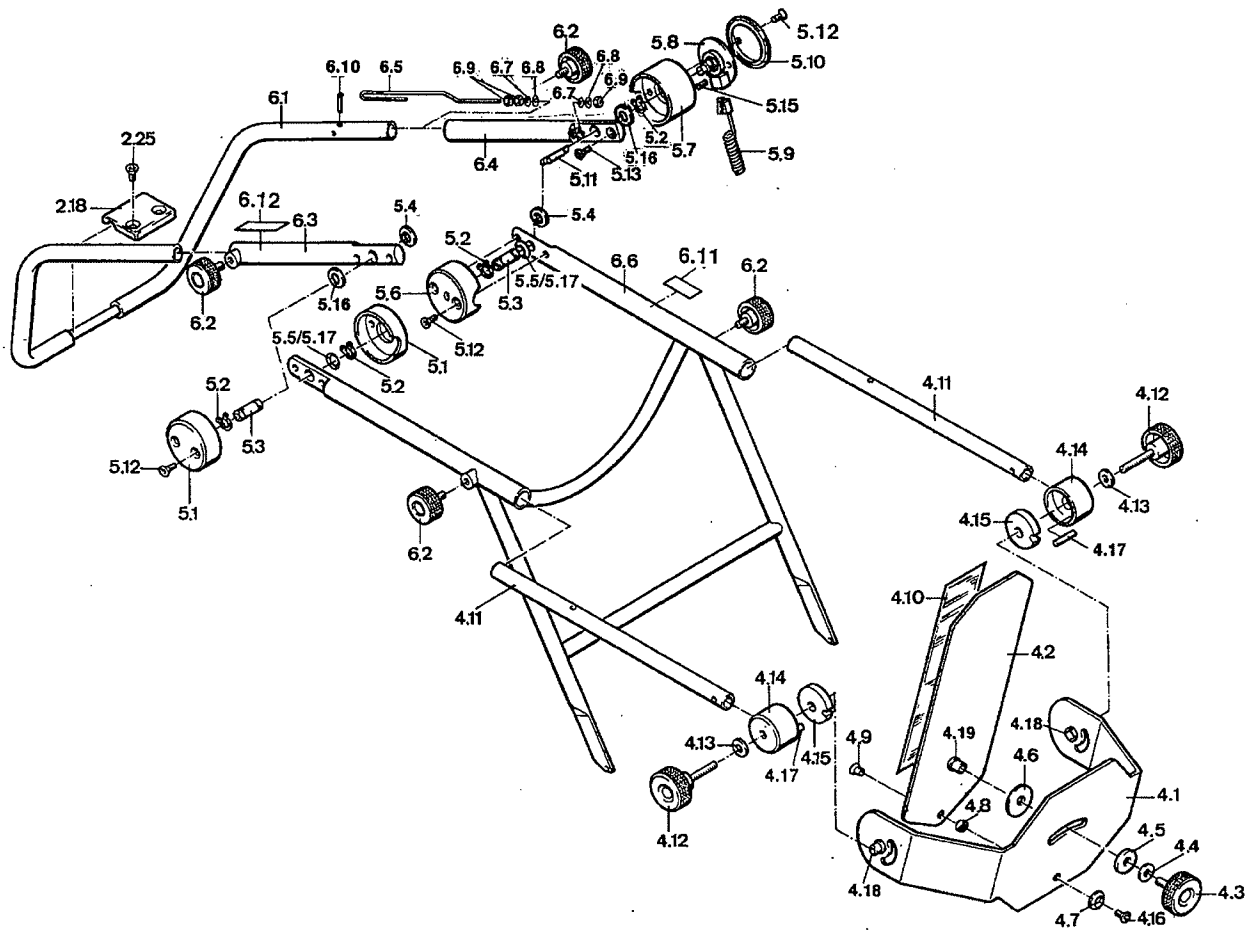

## 10. Checklist for Function- und Safetytest

### Safetytest

	Measuring	Date/Signature
Enclosure Leakage Current EN60601-1/ VDE 0751 $\leq 100 \mu\text{A}$	$\mu\text{A}$	
Or		
Enclosure Leakage Current UL2601 (115 Volt) $\leq 100 \mu\text{A}$	$\mu\text{A}$	

### Functiontest



	OK	Error
1. Turn the power ON at the ARTROMOT® -K3 and press "SET". → Display: Software Version K3 V40 161002		
2. The set range of motion for Extension/Flexion is from -5 to 110 degrees. → Verify the angle in a position of 0 degrees with a tolerance of +/- 5 degrees. → Verify the angle in a position of 60 degrees with a tolerance of +/- 5 degrees. → Verify the angle in a position of 105 degrees with a tolerance of +/- 5 degrees.		
3. Safety - OFF Functions. Start the ARTROMOT® -K3 in a continuous mode. → Press any of the buttons to stop the motor immediately. Verify this for all buttons.		
4. Perform the following settings. Extension: → -5 degrees Flexion: → 110 degrees Pause Ex.: → 5 sec. Pause Flex.: → 10 sec. Force: → 45 kp Speed: → 100% Adjust a maximum femur length.		
5. First press "STOP" and afterwards press "START". → The ARTROMOT®-K3 should then reach both points of changing direction within 60 to 75 seconds.		
6. Change the speed to 50% and afterwards press "START". → The ARTROMOT®-K3 should then reach both points of changing direction within 105 to 120 seconds.		
7. Verify the settings for "Pause Ex." and "Pause Flex." → The tolerance for both is +/- 3 seconds.		

## **K3/ K4 washer between the motor plate and the motor**

For following device we used 8 washer (2 per screw) between the motor plate and the motor

**K3 S/N 4612 – S/N 4675**  
**K4 S/N 3726 – S/N 3741**






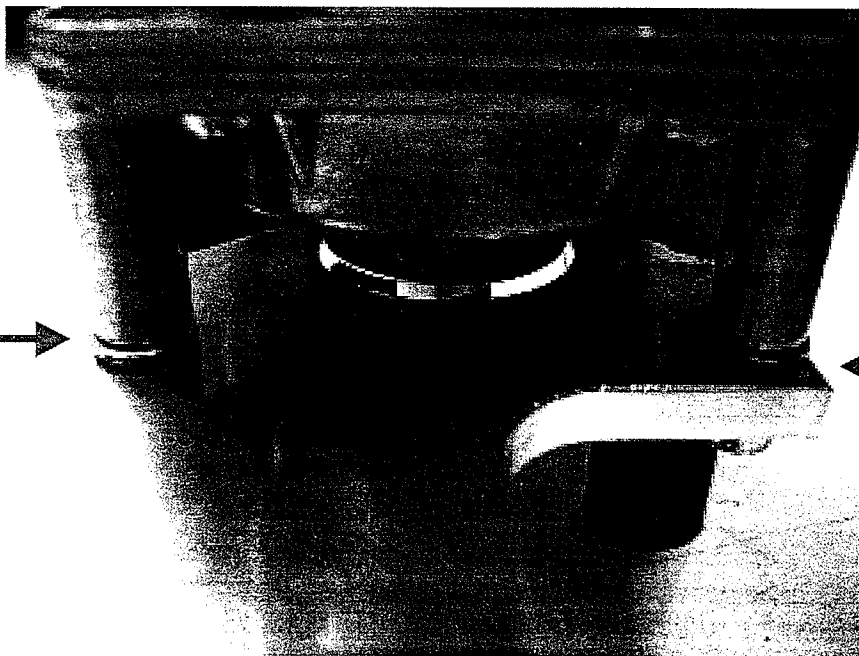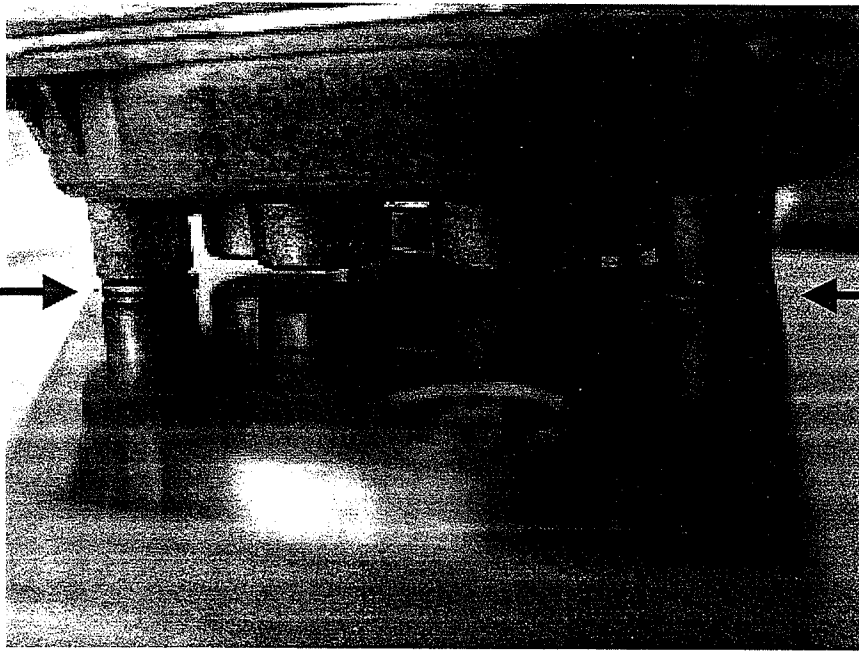


# **K3/ K4 there are no more cuts out on the rubber mat**

In future times there will be no more cut outs on the rubber mat for the white fixing buckles (Service Manual < 3000, explosion drawing, Pos 2.13)

Old rubber mat:

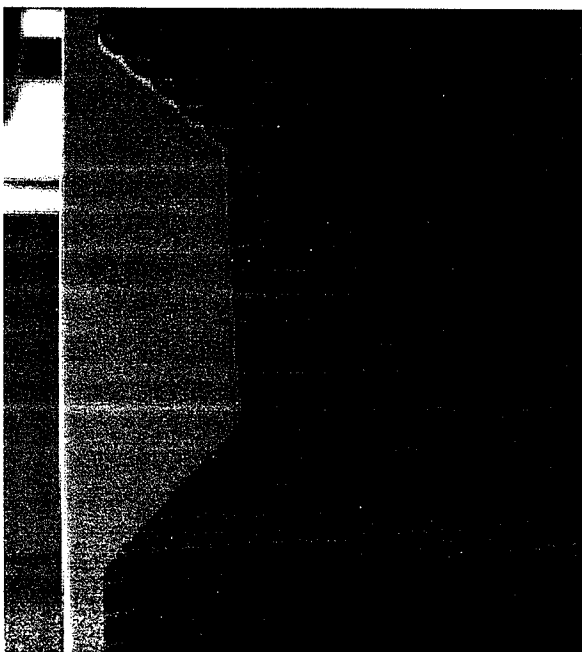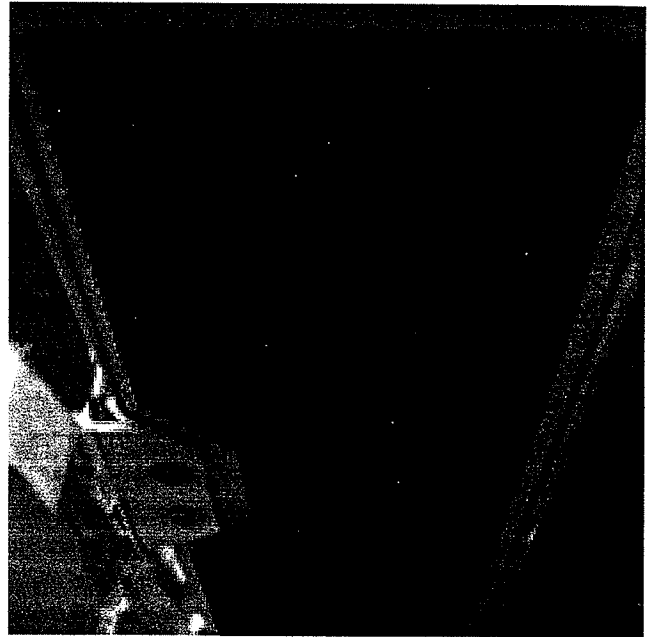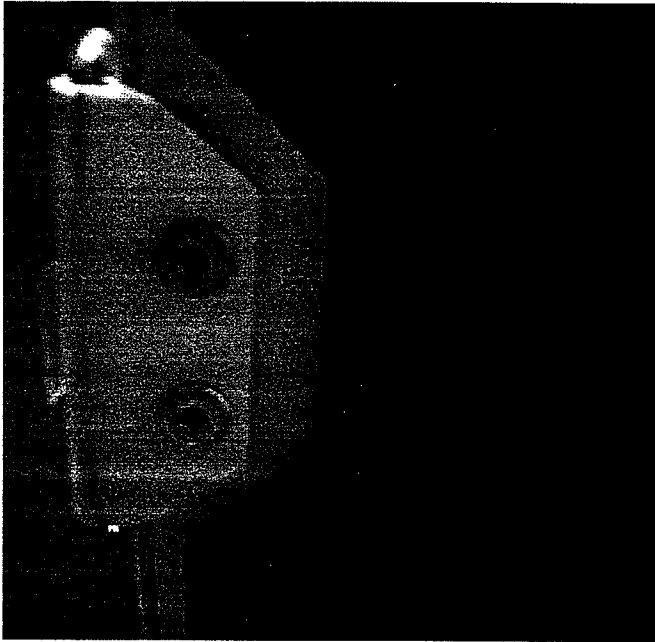

New rubber mat

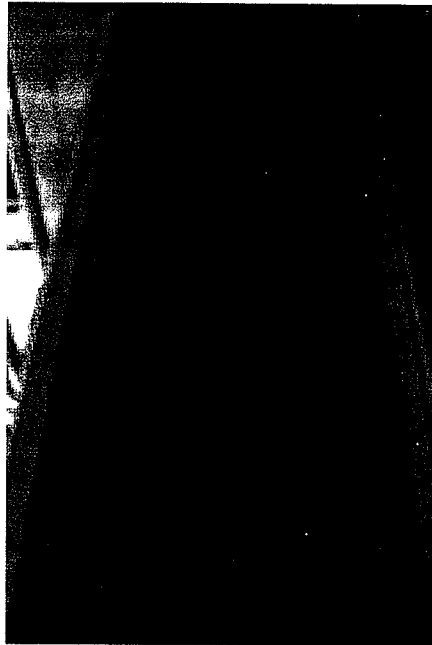





DIN EN 13485




ORMED Nr. 018 829-01

Ormed GmbH & Co. KG • Merzhauser Straße 112 • D-79100 Freiburg  
Phone +49 761 4566-01 • Fax +49 761 4566-5501 • [www.ormed.de](http://www.ormed.de) • E-Mail: [info@ormed.de](mailto:info@ormed.de)  
St. Pauli/USA, Phone +1 800 4402784, Fax +1 651 4157405 • Prague/CR, Phone +420 2 84094650,  
Fax +420 2 84094660 • Vienna/A, Tel +43 1 53 20 83 40, Fax +43 1 53 20 83 431



# ARTROMOT®-K3

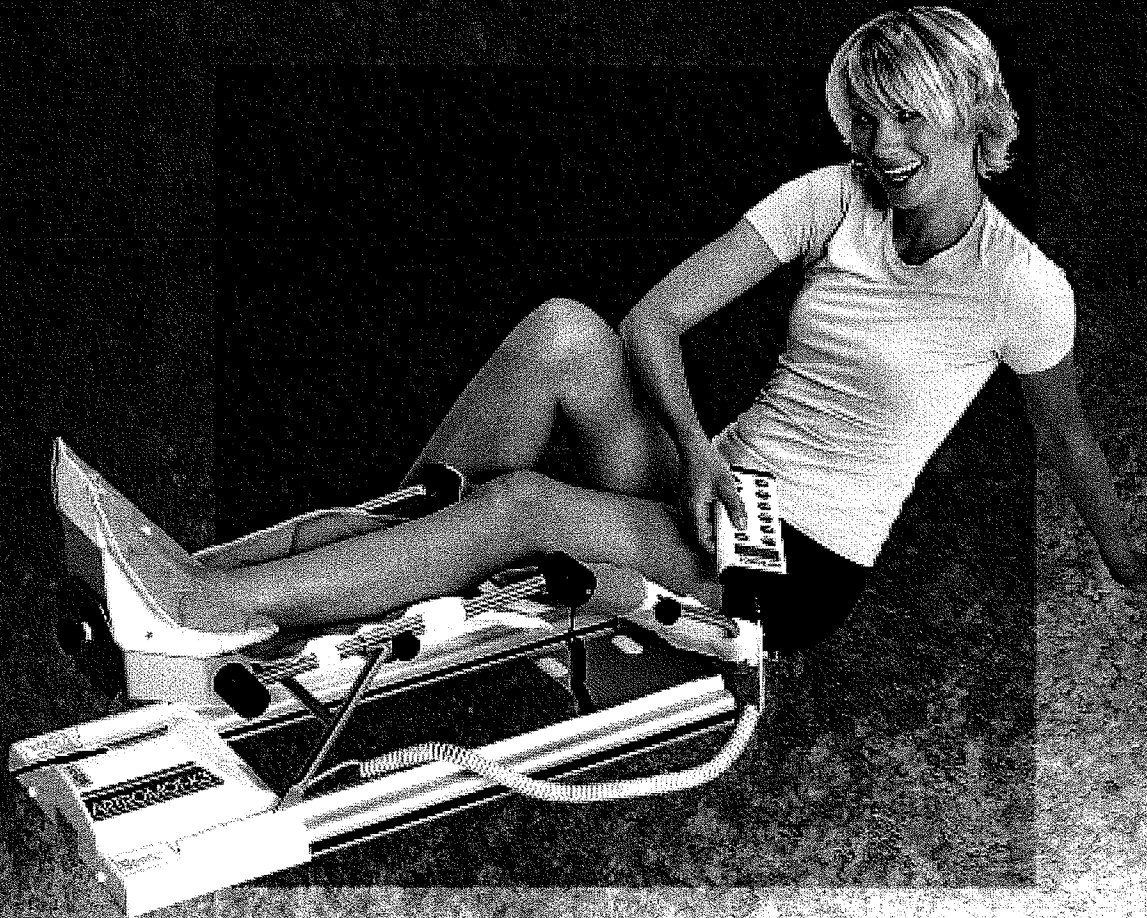

## Service Manual

Up to Serial number 2999