

350-10 Series

*Digital Wheelchair Scales
Software Revision 11439*

Operator Manual

Model 350-10-2



Model 350-10-3



Model 350-10-7



Model 350-10-8



An ISO 9001 registered company
© Rice Lake Weighing Systems. All rights reserved.

Rice Lake Weighing Systems® is a registered trademark of
Rice Lake Weighing Systems.

All other brand or product names within this publication are trademarks or
registered trademarks of their respective companies.

All information contained within this publication is, to the best of our knowledge, complete and
accurate at the time of publication. Rice Lake Weighing Systems reserves the right to make
changes to the technology, features, specifications and design of the equipment without notice.

The most current version of this publication, software, firmware and all other product
updates can be found on our website:

www.ricelake.com

Contents

1.0 Introduction	1
1.1 Safety	2
2.0 Assembly	3
2.1 Unpacking	3
2.2 Repacking	3
2.3 Setup	3
2.4 Inserting Batteries	5
2.5 AC Power Connections	5
3.0 Operation	6
3.1 Weighing	7
3.2 Hold/Release Function	7
3.3 Preset Tare	7
3.4 Toggle Tare	7
3.5 Body Mass Index (BMI) Function	8
4.0 RS-232 Communication	9
4.1 Push-Button Keypad Print	9
4.2 Communication Protocols	10
4.2.1 Escape Protocol	10
4.2.2 Maintenance Protocol	11
4.3 USB Connection	12
5.0 Maintenance and Troubleshooting	15
5.1 Maintenance	15
5.1.1 Basic Maintenance	15
5.1.2 Cleaning	15
5.2 Troubleshooting and Testing	15
5.3 Limited Warranty	16
6.0 Specifications	17



Technical training seminars are available through Rice Lake Weighing Systems. Course descriptions and dates can be viewed at www.ricelake.com/training or obtained by calling 715-234-9171 and asking for the training department.



*Rice Lake continually offers web-based video training on a growing selection of product-related topics at no cost. Visit **www.ricelake.com/webinars***

1.0 Introduction

The Rice Lake Digital Wheelchair Scale is a user-friendly, quality scale, designed for safe weighing of the handicapped and mobility challenged individuals. Movement compensation technology ensures sound, accurate weighments. The scale has roll on ramp access and comes in four different configurations:

- Single ramp folding wheelchair scale
- Single ramp platform wheelchair scale
- Dual ramp folding wheelchair scale
- Dual ramp platform wheelchair scale

The scale has a non-skid rigid platform and two rear heavy duty wheels for easy maneuverability.



Manuals and additional resources are available from the Rice Lake Weighing Systems website at www.ricelake.com/health



Figure 1-1. Digital Wheelchair Scale (single ramp and dual ramp models shown)

The scale is set up to use motion sensing technology, to determine actual weight of a moving patient. The weight can be displayed in pounds or kilograms and you can enter a tare weight. [Section 3.0 on page 6](#) of this manual explains the scale operation and how to obtain a tare weight.

The wheelchair scale has a unique folding feature that enables easy transportation and simplifies assembly, avoiding the need for field wiring and recalibration. All that is required is to open the packaging and unfold the scale.

1.1 Safety

There are certain precautions that should be taken to prevent personal injury to the user and damage to your scale.

Safety Signal Definitions:



Indicates an imminently hazardous situation that, if not avoided, will result in death or serious injury. Includes hazards that are exposed when guards are removed.



Indicates a potentially hazardous situation that, if not avoided, could result in serious injury or death. Includes hazards that are exposed when guards are removed.



Indicates a potentially hazardous situation that, if not avoided, could result in minor or moderate injury.



Indicates information about procedures that, if not observed, could result in damage to equipment or corruption to and loss of data.

General Safety



Do not operate or work on this equipment unless this manual has been read and all instructions are understood. Failure to follow the instructions or heed the warnings could result in injury or death. Contact any Rice Lake Weighing Systems dealer for replacement manuals.



Failure to heed could result in serious injury or death.

Do not drop the scale or subject it to violent shocks.

For accurate weighing, the scale must be placed on a flat, stable surface.

Do not transport the scale while someone is standing on it.

Weight exceeding the maximum capacity (1000 lb/453 kg) may damage your scale.

Operating at voltages and frequencies other than specified could damage the equipment.

If the LO Bat indicator activates, for accurate weighing, replace the batteries or connect the scale to an AC power source as soon as possible.

Rice Lake Weighing Systems offers optional AC adapters, utilizing an adaptor not supplied by us voids all warranties.

To avoid cross contamination, the scale should be cleaned regularly.

Avoid contact with excessive moisture.

Do not allow minors (children) or inexperienced persons to operate this scale.

Do not jump up and down on the scale.

Do not use in the presence of flammable materials.

Do not make alterations or modifications to the scale.

People with disabilities, or who are physically frail, should always be assisted by another person when using this scale.

Do not use the scale on slippery surfaces, such as a wet floor.

Do not use this scale when your body/feet are wet, such as after taking a bath.

2.0 Assembly

2.1 Unpacking

Place the unopened box in an open area that has ample room for unpacking the scale.

Recommended tools needed to set up your scale include:

- Scissors or a box cutter

Using scissors or a box cutter, cut the strapping bands that secure the box together. Immediately after opening the box, visually inspect the scale and components to ensure all parts are included and undamaged.

Parts contained in the shipping box include:

- Scale
- Box containing six AA batteries and four feet

2.2 Repacking

If the Rice Lake Digital Wheelchair Scale must be returned or moved, it must be properly packed with sufficient packing materials. When possible, use the original carton and packing material.

IMPORTANT

Damage caused by improper packaging is not covered by the warranty.

2.3 Setup

Move the scale into the area where the weighing process will occur. It's recommended to place the scale on a hard, level surface for the most accurate weighments. Thin carpeting is acceptable, but not recommended.



Rice Lake recommends using two people for lifting the scale and to use proper lifting techniques to prevent injury.

IMPORTANT

Do not lift the scale out of the box by its handle as this can cause the hinges to break or affect the scale operation.

1. Using two people, lift the scale out of the box by the base.
2. Stand the scale on edge to remove the packing material.



Figure 2-1. Scale on Edge

3. Screw the four feet clockwise into the scale base as far as possible.
4. Turn each foot counterclockwise two full rotations, to ensure there is adequate clearance between the scale and the floor.
5. Lower the scale base down to the floor carefully.
There should be minimal clearance between the scale base and the floor. [Figure 2-2](#) shows the width of a finger being slid between the scale base and the floor.

IMPORTANT *Not having clearance around the scale base creates inaccurate weighments.*



Figure 2-2. Clearance Between Scale Base and Floor

6. Gently press down on all corners of the scale base to ensure there are no high spots or rocking of the scale base. The scale must be completely level.

IMPORTANT *An unlevel base produces inaccurate weight readings.*

7. Turn the knobs to loosen the hinges and raise the handle.
8. Tighten the knobs to secure the handrail and the indicator mounted on it.

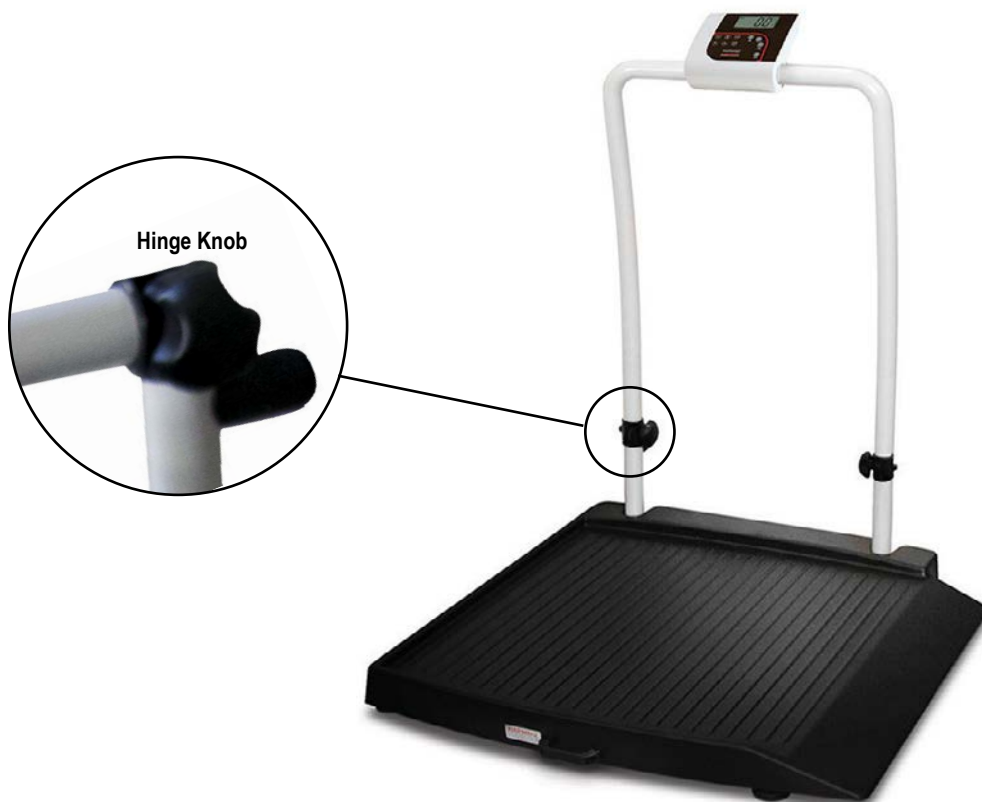


Figure 2-3. Loosen Hinges to Raise Handles

2.4 Inserting Batteries

The six AA batteries that come with the scale offer an average of 25 hours of continuous use.

To install the batteries:

1. Open the battery chamber cover by turning the thumbscrew to the left and remove the cover.
2. Insert batteries into the battery chamber as illustrated in the back of the chamber.



Figure 2-4. Battery Chamber

3. Put the cover in place and turn the thumbscrew to the right to secure it.



Note *Batteries must be removed from the unit prior to long periods of disuse or long term storage.*

If an external power supply or USB power supply is connected, the battery flag on the display is turned off.

When using battery or USB power supply, the back light power is deducted to 60%.

2.5 AC Power Connections

Use the optional 120 VAC or 230 VAC adapter when power is available. Rice Lake Weighing Systems offers optional AC adapters that plug into the back of the indicator as shown in [Figure 2-5](#).

IMPORTANT

Using an adapter not supplied by Rice Lake Weighing Systems voids all warranties.



Figure 2-5. Power Connection

3.0 Operation

The Rice Lake Digital Wheelchair Scale display has various front panel keys as shown in [Figure 3-1](#).



Figure 3-1. Front Panel Display Keys

Key Descriptions

[Table 3-1](#) describes each of the key functions.

Item No	Name	Function
1	BMI	Enables the user to access the BMI (Body Mass Index) function. This key only works if there is a locked weight shown on the display and the BMI function is turned on in the configuration mode.
2	TARE	Used to subtract the weight off the scale, example: oxygen tank, other equipment.
3	CLEAR	Allows the user to return to normal weighing when the BMI value is being displayed. While in BMI mode, the height display causes the value to return to the default of 190.0 cm, 5 ft, 7.5 in.
4	Print LB/KG	Print — A long key press will send data out from the RS-232 port. LB/KG — A short key press allows the user to toggle between kilograms and pounds providing that it's enabled in configuration mode. There is no toggling while in the BMI mode.
5	Zero	Clears the weight off the scale and returns it to zero after three seconds. It works only if the current weight is stable and zero up to 2% of full weight.
6	Hold Release	Hold & Release — The first press holds the most current weight value shown on the display. A second press releases the weight value shown. This key is not active while in BMI mode.
7	On/Off	Switches the scale on or off.
8	ENTER	Used to accept height in BMI mode. Accepts the value of the parameter last entered and moves to the next stage. A long press of the ENTER key during the scale's start up process will enter the ID display (pre-parameter mode).
9	Up/Down Arrows	Used to adjust height input (0.5"/0.5 cm) while in BMI mode. Adjusts the value of the flashing digit/number.

Table 3-1. Rice Lake Digital Wheelchair Scale Key Functions




IMPORTANT

The keys on the front panel display are very sensitive so only a gentle pushing motion is required to obtain results.

The scales have the capability of performing different operations beyond just calculating weight. The various operating instructions are described below.




3.1 Weighing

Use the following steps to weigh a person.

1. Press  to turn the scale on. **0.0** displays with **ZERO** on the upper display.
2. Have a person step on the scale, the weight displays. **LOCK** is displayed on the upper display and the display beeps to indicate the end of the weighing process.
 - Press  to toggle the display between **kg** and **lb**.
 - Press and hold  to turn off the scale, **OFF** displays.

3.2 Hold/Release Function

Use the following steps to use the Hold/Release function.



1. Have a person step on the scale.
2. Press . Have the person step off the scale, the weight and **HOLD & LOCK** remain on the display.
3. Press  to release the hold lock. The  does not work until the hold is released.



Note Pressing  prior to a person stepping on the scale also works.





3.3 Preset Tare

Use the following steps to use the Preset Tare.

1. With **0.0** displayed, place the extra load on the scale.
2. Press  until **0.0** displays again and **NET** displays.
3. Remove the extra load from the scale. The weight displays with a negative symbol to the left of it.
4. Have the person to step on the scale with the extra weight. The persons weight displays and **NET** is displayed. The weight of the extra load remains stored in memory.
5. To cancel the tare weight, press and hold  until the display returns to **0.0** and **GROSS** displays. Tare weight is also canceled by turning off the scale.

3.4 Toggle Tare






Use the following steps to use the Toggle Tare function.

1. With **0.0** displayed, press .
2. The default tare value is displayed (default is programmed to be 33.0 lb/15.0 kg), while the zero is flashing.
3. Use  and  to adjust the value.
4. Press  to start the tare function, **NET** displays.






3.5 Body Mass Index (BMI) Function

Use the following steps in determining the BMI.

LB Mode

1. Ensure that the scale is at zero.
2. Have the person step on the scale to obtain a weight. **LOCK** displays.
3. Press . **BMI** and **FT/IN** are lit on the display and a default value of 5 feet and 7.5 inches (5-07.5) flashes.
4. Use  and  to adjust the height value and press  to move to the next step.
5. The BMI value and **BMI** display. Press  to return to the weighing mode or step off the scale and the BMI function will be turned off.

KG Mode

1. Ensure that the scale is at zero.
2. Have the person step on the scale to obtain a weight. **LOCK** displays.
3. Press . **BMI** and **CM** are lit on the display and a default value of 170.0 cm (170.0) flashes.
4. Use  and  to adjust the height value and press  to move to the next step.
5. The BMI value and **BMI** display. Press  to return to the weighing mode or step off the scale and the BMI function will be turned off.

4.0 RS-232 Communication

The scale comes with an RS-232 port that enables weight data to be transmitted to other equipment, such as a computer or printer. The RS-232 cable with DB-9 connector (PN 100719) is available from Rice Lake Weighing Systems. [Figure 4-3 on page 12](#) shows where the RS-232 connection is.

The RS-232 parameters are 9600 baud (selectable in the programming mode), 8 data bits, 1 stop bit, no parity and no handshaking.

There are three methods of communication:

- Pushbutton keypad print
- Escape protocol
- Maintenance protocol

4.1 Push-Button Keypad Print

With a stable, in-range weight, press and hold the **LB/KG/Print** key for at least three seconds, or until the scale displays **PRINT**. Note that if the scale does not beep after five seconds, then release the button as the weight was either in motion, or out of range.

If displaying weight and not BMI, the scale will send out the following 21 character string:

```
xxxxxxxx<SP>uu<SP>mmmmm<SP><CR><LF>
```

Where:

xxxxxxxx is the weight with decimal point and " - " sign, if negative uu is the unit (lb or kg).

mmmmm is the mode (gross or net)

Example:

```
60.1 KG= <PATIENT><SP><WEIGHT><SP>-60.1<SP>KG<SP><CR><LF>
```

In BMI mode (displaying the BMI value), the scale will send out the following data:

PATIENT WEIGHT	60.1 KG
PATIENT HEIGHT	170.0 CM
PATIENT BMI	20.8

Example in KG:

```
<PATIENT><SP><WEIGHT><SP>-60.1<SP>KG<SP><CR><LF>
<PATIENT><SP><HEIGHT><SP>-170.0<SP>CM<SP><CR><LF>
<PATIENT><SP><B><SP><M><SP><I><SP><SP><SP><SP><20.8<SP><SP><SP><SP><CR><LF>
```

Example in LB:

```
<PATIENT><SP><WEIGHT><SP>132.4<SP>LB<SP><CR><LF>
<PATIENT><SP><HEIGHT><SP>-5-07.5<SP>FT<SP><CR><LF>
<PATIENT><SP><B><SP><M><SP><I><SP><SP><SP><SP><20.4<SP><SP><SP><SP><CR><LF>
```

In case of under weight or over weight, the word **Under** or **Over** will be sent correspondingly.

4.2 Communication Protocols

The Rice Lake Digital Wheelchair Scale has two communication protocols, escape and maintenance protocol.

4.2.1 Escape Protocol

An escape protocol is where the escape (0X1B or ASCII 27) is used to indicate that there is a command following. On the PC side there must be a listener created by the vendor that will interpret this protocol. This listener must also take care of all the issues regarding data integrity to make sure that the data that was sent and received is valid.

Two examples include:

- Scale initiated communication
- PC initiated communication

Table 4-1 is what can be sent across communications lines.

PC Initiated	ESC Value
Request current values/settings	R
Diagnostics	A
Send scale control messages	C
PC Initiated	ESC Value
Send single reading	R
Send diagnostic response	

Table 4-1. Escape Protocol Commands

Table 4-2 lists the ESC characters that will be used.

Name	ESC Character	ESC Value with Parameters	Description
Reading	R	R	Tells PC the scale is sending a reading; immediately following this is the value that is sent Example: <ESC><R>ESC><W0200.0<ESC>Nm<ESC>E
Weight	W	Wnnn.n	The patient weight (Example: W02000 means 200.0). If scale is overloaded or under loaded, 999.99 is returned
Height	H	Hnnn.n	Patient height
BMI	B	Bnn.n	Patient BMI
Units	N	Nc	Indicates the units the values have been taken (<i>m=metric, c=constitutional</i>).
End of Packet (EOP)	E	E	Indicates the end of the command has been reached.
Diagnostics (request)	A	Accc	A request for a diagnostic test on certain parts of the scale (like battery life, load cells).
Diagnostics (response)	Z	Zccc	The response of the diagnostics done on the scale; values include error codes to indicate an issue, or all zeros (Z000) to indicate the scale is performing properly
Control (set a value)	C	Cccc=c	Sets the value of the scale's global settings Example: <ESC><CUOM=m><ESC><E sets the unit of measurement

Table 4-2. ESC Characters

Name of Control	Identifier	Unit
Unit of Measure (metric or constitutional)	UOM	c (m or c)

Table 4-3. Scale Global Values and Identifiers

Samples of Escape Protocol

Examples of what is sent to the computer from the scale.

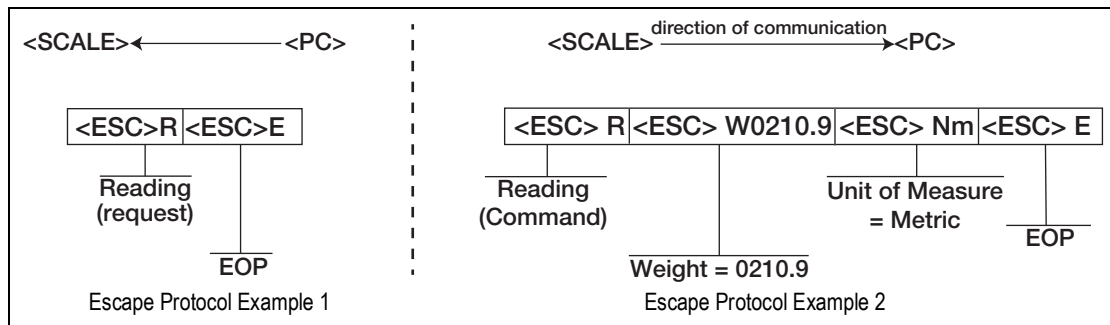


Figure 4-1. Escape Protocol Examples

Examples of diagnosing battery request and responses.

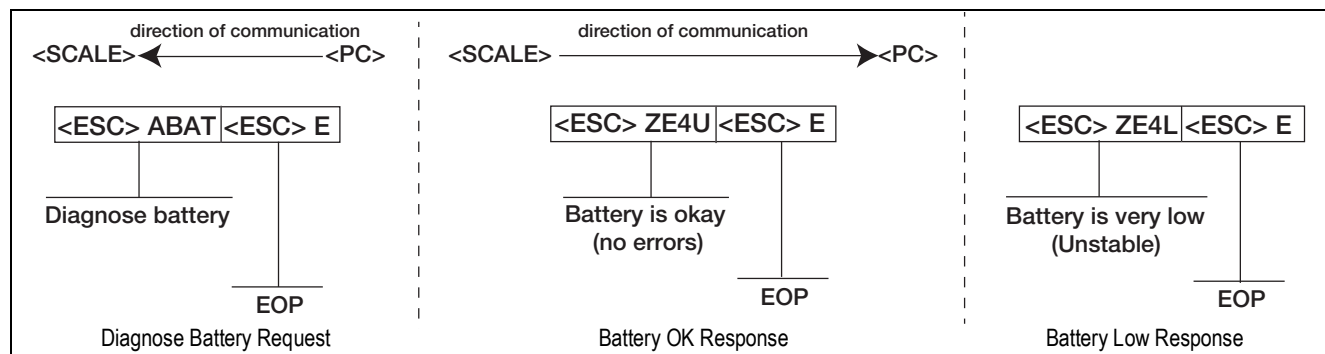


Figure 4-2. Diagnose Battery Examples

4.2.2 Maintenance Protocol

Table 4-4 lists the maintenance protocol commands.

Command	Definition
R	Reboot
V	Firmware ID + development version
W	Current weight
A	Current AD
Z	Zero the scale
F	Show flash values (used for the first flash process)
L	USB On/Off (not available on USB communication)

Table 4-4. Maintenance Protocol Commands

4.3 USB Connection

The Rice Lake Digital Wheelchair Scale has the capability of connecting to a PC using a USB connection and a USB cable (not included).

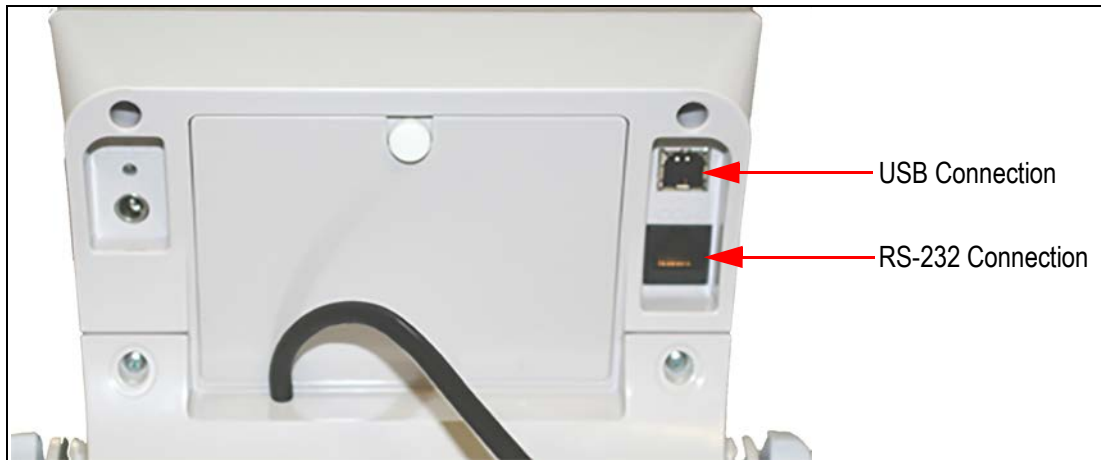


Figure 4-3. USB Connection Port

Connecting software and downloads should be addressed by an IT professional, and can vary depending on the computer platform used. Basic information on USB driver installation using Windows® is described in the following steps and serves only as an example.

A USB driver can be downloaded from the Rice Lake Weighing Systems website at:

<https://www.ricelake.com/resources/software-firmware>

1. Select Software.

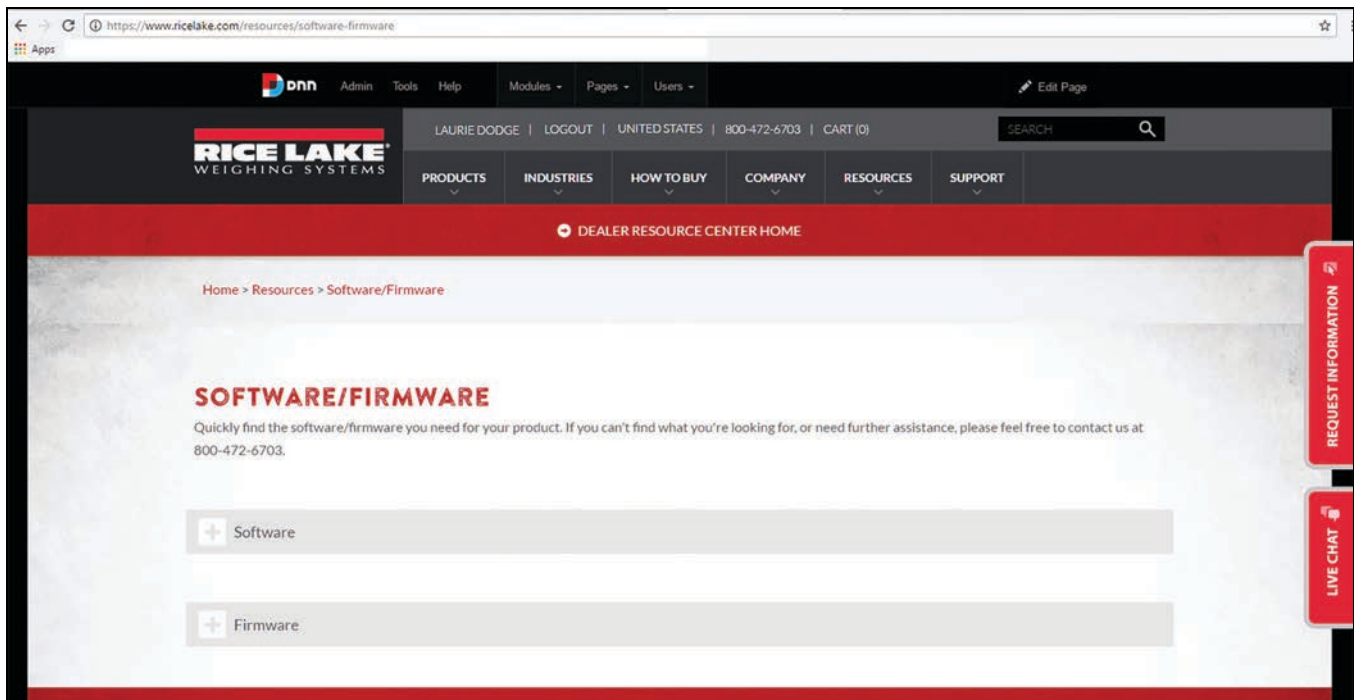


Figure 4-4. Software/Firmware Page

- From the drop down menus select *Health Scales*.

Figure 4-5. Software Download Page

- Find **Titanium USB Driver**. Press **Download** to open and download the driver to a local computer.

TITLE	VERSION	SIZE	RELEASE NOTES	DOWNLOAD	RELEASE DATE	EMAIL
880 USB Driver	1	3.16 MB		Download	Jan 1, 2014	Email
920i USB Driver Installation	1	1.31 MB	Installation Instructions	Download	Dec 14, 2011	Email
Body Composition Analyzer Calibration Software	1.0.03	5.58 MB		Download		Email
Contact Software D1000 Only - Body Composition Analyzer	1.0.00.05	455.28 MB		Download	Apr 20, 2017	Email
Contact Software - Body Composition Analyzers	1.0.00.42	505.68 MB		Download	Mar 22, 2017	Email
RS-232 Communication Files	1	31.3 KB	Specifications	Download	Oct 19, 2009	Email
Titanium USB Driver	1	967 B		Download	Jun 17, 2014	Email
Tripp-Lite USB to Serial Converter Vista Driver	1	166.53 KB		Download	Dec 1, 2009	Email
Tripp-Lite USB to Serial Converter XP Driver	1	219.67 KB		Download	Dec 1, 2009	Email

Figure 4-6. Example of Drivers List Page

- When the USB cable is connected to the indicator and the scale is turned on, a display prompts to navigate through the software install process.



Figure 4-7. Hardware Wizard Menu

- Select **No, not this time** and press **Next**.
- Select **Install the software automatically** press **Next**. A file transfer screen displays as the file downloads and installs to the computer.
- Press **Finish** when the completion screen displays.

8. To verify the installation, the driver can be viewed in the device manager of the computer.

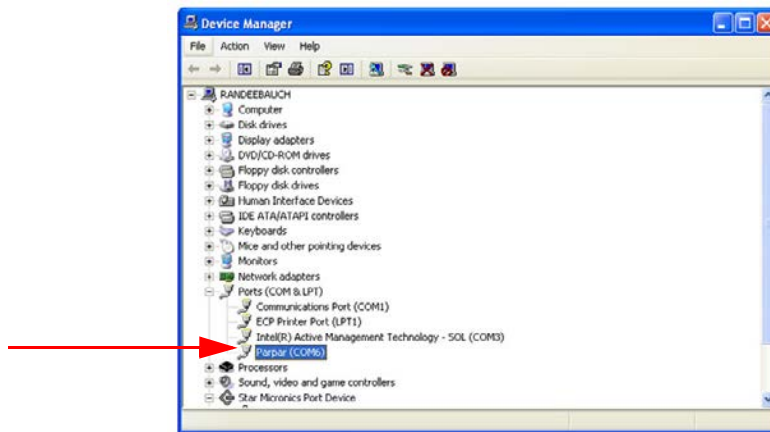



Figure 4-8. Device Manager

9. To configure a printer using the USB driver, open the software driver **Parpar** in the device manager (Figure 4-8). The port assigned to that driver is displayed.
10. Ensure the USB cable is properly connected and the unit is on.
11. Open and connect a terminal emulation program, such as Hyperterminal, via the USB driver. Select the port assigned to the software driver **Parpar** to establish a port. The terminal emulation program is necessary to view information transmitted from the indicator to the PC.
12. Press . The following example tickets print.

PATIENT WEIGHT	199.8 lb
GROSS WEIGHT	199.8 lb
TARE WEIGHT	0.0 lb
NET WEIGHT	199.8 lb
PATIENT HEIGHT	6ft 00.0in
PATIENT B.M.I.	27.1

Figure 4-9. Example Tickets



Note A single print ticket has four spaces after **PATIENT WEIGHT**, one space between the weight value and units (**lb**), and seven **<CR><LF>** after.

```

PATIENT WEIGHT  199.8  lb <CR><LF>
<CR><LF>
<CR><LF>
<CR><LF>
<CR><LF>
<CR><LF>
<CR><LF>

```

Figure 4-10. IT Example (IT Information Only)

5.0 Maintenance and Troubleshooting

5.1 Maintenance

The following section provides instructions for maintaining and cleaning the Rice Lake line of scales.

IMPORTANT

Do not immerse the scale in cleaning or other liquid solutions.

Do not use Isopropyl alcohol or other solutions to clean the indicator display surface.

5.1.1 Basic Maintenance

Before using the scale and after periods of non-use, check the scale for proper operation and function. If the scale does not operate correctly, contact a qualified service personnel.

Basic maintenance includes:

- Check the overall appearance of the entire scale for any obvious signs of damage.
- Inspect the condition of the AC adapter cord for cracking, fraying or broken/bent prongs.
- Using an adapter that has been used elsewhere may cause issues with the scale.
- Change batteries on a regular interval. Leaving in for long periods of time can cause batteries to leak.

5.1.2 Cleaning

Proper care and cleaning is essential to ensure a long life of accurate and effective operation. Before beginning the cleaning process, disconnect the scale from the AC power source.

- Clean all external surfaces with a clean, damp cloth or tissue.
- Mild soap and water solution may be used.
- Standing platform may be cleaned with Isopropyl alcohol
- Dry with a clean soft cloth.

5.2 Troubleshooting and Testing

Refer to [Table 5-1](#) to diagnose and correct failure prior to contacting service personnel.

Symptom	Possible Cause	Corrective Action
Scale does not turn on	Dead battery	Connect the scale to a power source
	Faulty electrical outlet	Use a different electrical outlet
	Bad power supply	Replace adapter
Questionable weight or the scale does not zero	External object is interfering with scale	Remove interfering object from scale
	0.0 was not displayed prior weighing	Have the patient off scale, zero scale and begin weighing process again
	Scale is not level	Level scale and begin weighing process again
	Scale is out of calibration	Check weight with a known weight value
E messages displayed		
E06	Identifier - ADC	AD too high
E07		AD too low
E10	Overload	Scale is overloaded; remove load from scale
E4L	BAT	Battery low but usable — 1 bar on indicator display.
E4U		Battery low and unstable — no bars on indicator display.
E11	CAL	Calibration Error — recalibrate the scale
Err 2	Low saturation state (low A/D)	Load cell is not connected properly; check cables and mechanical connections; if the problem persists, replace load cells.
Err 3	High saturation state (high A/D)	See Err 2
Err 6	Unstable weight; cannot calibrate.	Check the load cells mechanical surroundings to ensure nothing is touching them and the cables are properly welded
SAT	Damaged load cell cable	Replace load cell cable

Table 5-1. Troubleshooting Table for the Rice Lake Scale Line

5.3 Limited Warranty

Rice Lake Weighing Systems (RLWS) warrants that all RLWS equipment and systems properly installed by a Distributor or Original Equipment Manufacturer (OEM) will operate per written specifications as confirmed by the Distributor/OEM and accepted by RLWS. All systems and components are warranted against defects in materials and workmanship for two years.

RLWS warrants that the equipment sold hereunder will conform to the current written specifications authorized by RLWS. RLWS warrants the equipment against faulty workmanship and defective materials. If any equipment fails to conform to these warranties, RLWS will, at its option, repair or replace such goods returned within the warranty period subject to the following conditions:

- Upon discovery by Buyer of such nonconformity, RLWS will be given prompt notice with a detailed explanation of the alleged deficiencies.
- Individual electronic components returned to RLWS for warranty purposes must be packaged to prevent electrostatic discharge (ESD) damage in shipment. Packaging requirements are listed in a publication, **Protecting Your Components From Static Damage in Shipment**, available from RLWS Equipment Return Department.
- Examination of such equipment by RLWS confirms that the nonconformity actually exists, and was not caused by accident, misuse, neglect, alteration, improper installation, improper repair or improper testing; RLWS shall be the sole judge of all alleged non-conformities.
- Such equipment has not been modified, altered, or changed by any person other than RLWS or its duly authorized repair agents.
- RLWS will have a reasonable time to repair or replace the defective equipment. Buyer is responsible for shipping charges both ways.
- In no event will RLWS be responsible for travel time or on-location repairs, including assembly or disassembly of equipment, nor will RLWS be liable for the cost of any repairs made by others.

These warranties exclude all other warranties, expressed or implied, including without limitation warranties of merchantability or fitness for a particular purpose. Neither RLWS nor distributor will, in any event, be liable for incidental or consequential damages.

RLWS and buyer agree that RLWS's sole and exclusive liability hereunder is limited to repair or replacement of such goods. In accepting this warranty, the buyer waives any and all other claims to warranty.

Should the seller be other than RLWS, the buyer agrees to look only to the seller for warranty claims.

No terms, conditions, understanding, or agreements purporting to modify the terms of this warranty shall have any legal effect unless made in writing and signed by a corporate officer of RLWS and the Buyer.

© Rice Lake Weighing Systems, Inc. Rice Lake, WI USA. All Rights Reserved.

RICE LAKE WEIGHING SYSTEMS • 230 WEST COLEMAN STREET • RICE LAKE, WISCONSIN 54868 • USA

6.0 Specifications

Power

120 VAC - 9 VDC - 60Hz / 230 VAC - 9 VDC - 50Hz

Battery Type

6 AA size Alkaline batteries

Battery Use

25 hours continuous use

Automatic power-off can be configured

Data Communications

RS-232 with RJ-45 jack

USB Connection

Selectable baud rate, default - 9600

8 bits

No parity

1 stop bit

No handshaking

Environmental

Operating Temperature 50 to +95°F (10 to 35°C)

Storage Temperature 32 to 122°F (0 to 50°C)

Humidity 85% relative humidity

Capacity and Graduation

1000 lb (453 kg) 0.2 lb (0.1kg)

Certifications and Approvals

RoHS Compliant



Dimensions

Platform Dimensions 48.5 in W x 29.5 in L x 3 in H



© Rice Lake Weighing Systems Specifications subject to change without notice.
Rice Lake Weighing Systems is an ISO 9001 registered company.

230 W. Coleman St. • Rice Lake, WI 54868 • USA

U.S. 800-472-6703 • Canada/Mexico 800-321-6703 • International 715-234-9171 • Europe +31 (0)26 472 1319