

ESCORT 300A

SERVICE MANUAL

ESCORT 300A

SERVICE MANUAL

December, 1995

Revision B

MEDICAL DATA ELECTRONICS, INC.
12720 Wentworth Street
Arleta, CA 91331-4329

(818) 768-6411
(800) 237-5243
FAX (818) 768-0759

STANDARD WARRANTY

The ESCORT 300A Monitor is warranted against defects in materials and workmanship for a period of twelve (12) months from the date of shipment to the original purchaser. Batteries, cables, cuffs, and sensors are warranted ninety (90) days from date of shipment. Warranty is valid only to the original buyer. Defective equipment should be returned freight prepaid to Medical Data Electronics. Equipment returned with defective parts and assemblies will be either repaired or replaced. This warranty is not applicable if repair has been attempted, if the instrument has been damaged due to operation outside the environmental and power specifications for the product, or due to improper handling or use.

If any fault develops, notify MDE Technical Support giving full details of the difficulty, and include the model and serial number of the device. Upon receipt of the shipping instructions, forward the device prepaid and repairs will be made at the factory.

The foregoing warranty is in lieu of all other warranties expressed or implied, including but not limited to any implied warranty or merchantability, fitness or adequacy for any particular purpose or use. Medical Data Electronics shall not be liable for any incidental or consequential damages.

NOTICE

MEDICAL DATA ELECTRONICS MAKES NO WARRANTY OF ANY KIND WITH REGARD TO THIS MATERIAL , INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

Medical Data Electronics shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

This document contains proprietary information which is protected by copyright. All rights reserved. No part of this document may be photocopied, reproduced, or translated to another language without the prior written consent of Medical Data Electronics.

The information in this document is subject to change without notice.

TABLE OF CONTENTS

	PAGE
1.0.0 ESCORT 300A SPECIFICATIONS	1-1
2.0.0 SYSTEM OVERVIEW	2-0
RS-232 Computer Interface	2-2
Interconnection Diagram	2-7
Board Location	2-8
3.0.0 CPU BOARD	3-0
3.1.0 Overview	3-1
3.2.0 Microprocessor	3-1
3.2.1 Timing	3-1
3.2.2 Display Enable	3-2
3.2.3 Chip Enable	3-2
3.2.4 Peripheral I/O	3-2
3.2.5 Keyboard Decoder	3-2
3.2.6 Time of Day Clock	3-2
3.2.7 Memories	3-3
3.2.8 LCD Control	3-3
3.2.9 EL CONTROL	3-3
3.2.10 Analog Voltages	3-3
3.2.11 Auxiliary Outputs	3-4
3.2.12 Regulators	3-5
CPU BLOCK DIAGRAM	3-6
CPU SCHEMATICS	3-7
CPU BOARD LAYOUT	3-10
CPU PARTS LIST	3-11
EL DISPLAY DRIVER BOARD LAYOUT	3-16
EL DISPLAY DRIVER BOARD SCHEMATIC	3-17
EL DISPLAY DRIVER BOARD PARTS LIST	3-18
4.0.0 ECG BOARD	4-0
4.1.0 Overview	4-1
4.2.0 Isolated Section	4-1
4.2.1 Lead Select	4-1
4.2.2 Instrumentation Amplifier/Notch Filter	4-1
4.2.3 Pacer Pulse Detect	4-2
4.2.4 ECG/Respiration Multiplexer	4-2
4.2.5 A to D Sampling Circuit	4-2
4.2.6 Respiration	4-3
4.2.7 Lead Fail	4-3
4.2.8 Isolation Power Supply	4-4
4.3.0 Non Isolated Section	4-4

4.3.1	ECG Digital	4-4
4.3.2	Defibrillator Sync	4-5
4.4.0	Software	4-6
	ECG BLOCK DIAGRAM	4-7
	ECG SCHEMATICS	4-8
	ECG MOTHER BOARD LAYOUT	4-11
	ECG DAUGHTER BOARD LAYOUT	4-12
	ECG MOTHER-DAUGHTER ASSEMBLY DIAGRAM	4-13
	3 LEAD ECG CABLE PINOUT	4-14
	5 LEAD ECG CABLE PINOUT	4-15
	HP CLOVER CONNECTOR WIRING	4-16
	HP MERLIN CONNECTOR WIRING	4-17
	STANDARD DEFIBRILLATOR SYNC WIRING	4-18
	HP DEFIBRILLATOR SYNC WIRING	4-19
	ECG PARTS LIST	4-20
5.0.0	TEMPERATURE-PRESSURE BOARD	5-0
5.1.0	Overview	5-1
5.2.0	Isolation Section	5-1
5.2.1	Temperature Inputs	5-1
5.2.2	Pressure Inputs	5-2
5.2.3	Multiplexers	5-2
5.2.4	Analog to Digital	5-2
5.2.5	Excitation Voltage	5-3
5.2.6	Isolation Power Supply	5-3
5.3.0	Non-Isolated Section	5-3
5.3.1	Temp-Press Digital	5-3
5.4.0	Software	5-4
	PARTIAL LIST OF ADAPTER CABLES	5-5
	TEMP-PRESS BLOCK DIAGRAM	5-6
	TEMP-PRESS SCHEMATICS	5-7
	TEMP-PRESS BOARD LAYOUT	5-9
	PRESSURE CABLE PINOUT	5-10
	HP PRESSURE CONNECTOR HARNESS ASSEMBLY	5-12
	TEMP-PRESS ASSEMBLY	5-13
	TEMP-PRESS PARTS LIST	5-14
6.0.0	NIBP BOARD	6-0
6.1.0	Overview	6-1
6.1.1	AC/DC Channels	6-1
6.1.2	Over pressure Protection and Detection	6-1
6.1.3	Blood Pressure or Temperature Options	6-1
6.2.0	Input Circuit	6-2
6.2.1	AC Channel	6-2
6.2.2	Valve and Pump Control	6-2

6.2.3	Fail Detect	6-2
6.2.4	Reference Voltage	6-3
6.3.0	Digital	6-3
6.4.0	Calibration Check Procedure	6-3
6.4.1	Leak Test Procedure	6-4
6.4.2	Oscillation Waveform Recording	6-5
	NIBP BLOCK DIAGRAM	6-6
	NIBP MOTHER BOARD SCHEMATICS	6-7
	NIBP MOTHER BOARD LAYOUT	6-9
	NIBP MOTHER BOARD PARTS LIST	6-10
	NIBP DAUGHTER (IBP) SCHEMATICS	6-14
	NIBP DAUGHTER (IBP) BOARD LAYOUT	6-15
	NIBP DAUGHTER (IBP) PARTS LIST	6-16
	NIBP DAUGHTER (TEMP) SCHEMATICS	6-19
	NIBP DAUGHTER (TEMP) BOARD LAYOUT	6-20
	NIBP DAUGHTER (TEMP) PARTS LIST	6-21
	NIBP PNEUMATIC ASSEMBLY	6-24
	NIBP PNEUMATIC PARTS LIST	6-25
7.0.0	SAO ₂ BOARD	7-0
7.1.0	Overview	7-1
7.1.1	Nellcor OEM Module	7-1
7.2.0	Interface Circuitry	7-1
7.3.0	Isolated Power Supply	7-2
	ECG/SAO ₂ BLOCK DIAGRAM (SLOT 1)	7-3
	ECG/SAO ₂ SCHEMATICS (SLOT 1)	7-4
	ECG/SAO ₂ BOARD LAYOUT (SLOT 1)	7-9
	ECG/SAO ₂ PARTS LIST (SLOT 1)	7-10
	ECG/SAO ₂ WITH RESP DAUGHTER PARTS LIST	7-15
	SAO ₂ BLOCK DIAGRAM (SLOT 2)	7-18
	SAO ₂ SCHEMATICS (SLOT 2)	7-19
	SAO ₂ DAUGHTER (IBP) SCHEMATICS	7-20
	SAO ₂ BOARD LAYOUT (SLOT 2).....	7-22
	SAO ₂ PARTS LIST (SLOT 2)	7-23
8.0.0	SWITCHING POWER SUPPLY BOARD	8-0
8.1.0	Overview	8-1
8.2.0	Input Circuits	8-1
8.2.1	Voltage Sense	8-1
8.2.2	Indicators and Signals	8-2
8.3.0	Battery Charging Circuitry	8-2
8.3.1	Overview	8-2
8.3.2	Current Sensing	8-2
8.3.3	Temperature Compensation	8-2
8.3.4	Voltage Regulating	8-3

8.3.5	Discharge Protection	8-3
	SWITCHING POWER SUPPLY BOARD BLOCK DIAGRAM	8-4
	SWITCHING POWER SUPPLY SCHEMATICS	8-5
	SWITCHING POWER SUPPLY BOARD LAYOUT	8-6
	SWITCHING POWER SUPPLY PARTS LIST	8-7
9.0.0	PERFORMANCE CHECK	9-0
9.1.0	Overview	9-1
9.2.0	Batteries	9-1
9.3.0	Leakage Testing	9-2
9.3.1	Chassis Leakage	9-2
9.3.2	Patient Input Leakage	9-2
9.4.0	Ground Check	9-2
9.5.0	RAM, ROM Self Test	9-2
9.6.0	Keypad	9-2
9.7.0	ECG Functional Test	9-3
9.8.0	Pressure Functional Test	9-3
9.9.0	Temperature Functional Test	9-4
9.10.0	Respiration Functional Test	9-4
9.11.0	Recorder Functional Test	9-4
9.12.0	NIBP Functional Test	9-5
9.13.0	SAO ₂	9-5
9.14.0	Performance Check List	9-6
10.0.0	MECHANICAL DISASSEMBLY	10-0
10.1.0	Safety	10-1
10.2.0	Fuse Replacement	10-1
10.3.0	Disassembly	10-1
10.3.1	Top Cover	10-1
10.3.2	Bottom Cover	10-1
10.3.3	Recorder Removal	10-2
10.3.4	Processor Unit	10-2
10.3.5	Switching Power Supply/Battery Charger	10-2
10.3.6	CPU Removal	10-3
10.3.7	LCD Removal	10-3
10.3.7	EL Display Removal	10-3
	MECHANICAL DISASSEMBLY DRAWINGS	10-4
	PARTS LIST (CHASSIS ASSEMBLY)	10-11
	PARTS LIST (LCD ASSEMBLY)	10-12
	PARTS LIST (EL DISPLAY OPTION ASSEMBLY)	10-13
	PARTS LIST (AR42 RECORDER ASSEMBLY)	10-14

SPECIFICATIONS

CHAPTER 1

ESCORT 300A SPECIFICATIONS

DISPLAY

Size: 6" diagonal
Type: LCD or Electroluminescent (EL)
Number of Traces: 3
Trace Length: 4 seconds at 25 mm/sec

FRONT PANEL KEY FUNCTIONS

Freeze, Record 1, Record 2, Record 3, Alarm Suspend, Record Stop, Page Home, Next Page, Softkeys (6)

ECG

Range: 10 to 300 BPM
Accuracy: $\pm 2\%$ or ± 2 BPM
Sweep Speed: 12.5, 25 mm/sec selectable
High Limit Range: 50 to 250 BPM
Low Limit Range: 20 to 150 BPM
Limit Resolution: 5 BPM
Asystole Alarm: R to R interval greater than 6 seconds
Bandwidth: 0.5 to 40 Hz (monitor) 0.05 to 100 Hz (diagnostic)
R-wave indicator: Flashing heart
Leads: Full 5 lead selectable,
Fixed lead with option 11AE
Sensitivity: .25 to 3mV/cm selectable (12 levels)
Pacer Rejection: 0.2 to 2 msec; 2 to 700mV
Defib Tolerance: 400 joule with 25 ohm series lead impedance
Connector: Standard 6 pin MS
Isolation: Full electrical isolation
Overload Recovery: 2 sec excluding electrode polarization
Electrosurgical Suppression: Standard
Configuration: Neonatal/Adult softkey

MODULAR BATTERIES

Capacity: 2.5 to 3 hours depending upon configuration
Charge Time: 14 hrs to 90%; Opt. external charger: 2.7 hrs
Type: 12V, 2.3AH sealed lead acid rechargeable (2 each)

RECORDER (OPTION 02E, 03E)

Print Method: Thermal array
Channels: Single (Opt. 02E) or dual (Opt. 03E)
Resolution: 8 dots/mm vertical, 32 dots/mm horizontal
Paper: 40 mm grid; 50 mm paper width
Speed: 6.25, 12.5, 25 mm/sec
Manual Record Duration: 16 seconds
Memory: 12 seconds
Annotation: Time, date, all parameter values, scales, source, speed

TREND (OPTION 04E)

Parameters: HR, RR, IBP, NIBP, SAO_2 , T
Time: 1, 8, 24 hours

RESPIRATION (OPTION 05E)

Range: 4 to 200 BPM
Accuracy: $\pm 2\%$ or ± 2 BPM
Lead: RA to LA
Inspiration Indicator: Flashing lungs
Sensitivity: .25 to 3 ohm/cm selectable
Alarms: High and low rate,
Apnea delay selectable, 10, 15, 20, 30, 40 sec
Sweep Speed: 6.25, 12.5, 25 mm/sec selectable
CVA Rejection: Rejects most cardiovascular coincidence
Configuration: Neonatal/Adult softkey

TEMPERATURE (OPTION 06SE, 06DE)

Range: 0 to 50 degrees C
Accuracy: ± 0.2 degrees C
Probe: YSI 700
Units: Degrees C or degrees F selectable
Channels: One (06SE), two (06DE)
Connector: 1/4 inch stereo phone jack
Isolation: Full electrical isolation

NIBP (OPTION 07NE)

Measurement Method: Oscillometric
Measurement Range: Systolic 30-270 mmHg
Diastolic 20-240 mmHg
Pulse Rate 20-250 BPM
Measurement Time: 30 to 40 seconds typical
Modes: Manual-initiated via START key, Automatic-STAT, 1, 2, 3, 4,
5, 10, 15, 30, 45 minutes, 1, 2, 3, 4 hours
Auto Zero: Prior to each reading
Cuff Inflation: Adult: Selectable 140-190 mmHg
Neonatal: 90 mmHg
Systolic ± 25 mmHg on subsequent inflations
Cuff Deflation: 8 mmHg steps
Alarms: SYS, DIAS, or MEAN selectable in 5 mmHg increments
Electronic Accuracy: ± 3 mmHg or $\pm 2\%$ reading
System Accuracy: ± 5 mmHg mean error with ± 8 mmHg SD
Hose: Dual lumen
Cuff/Hose Connectors: Standard screw fittings
Cuff Sizes: Adult, Large Adult, Adult Thigh, Pediatric, Infant,
Neonatal (Sizes 1, 2, 3, 4)
Tabular Trend: 100 NIBP measurements with time, PR, % SAO_2

HP CONNECTORS (OPTION 10CE, 10ME)

ECG Connector: Opt. 10CE-78534 (8 pin),
 Opt. 10ME - Component Monitoring System (12 pin)
Pressure Connector: 12 pin HP (5 uV/V/mmHg)
Temperature Connector: 2 pin HP
Temperature Probe: YSI 400
Temperature Channel: One
Defib Sync Out/Defib Marker In: 1/4 inch stereo phone jack

SAO₂ (OPTION 11AE, 11BE)

Display: % SaO₂, Plethysmographic Waveform, Pulse Rate, Pulse
 Amplitude Bar, Alarm & Status Messages
SAO₂ Range: 0-100%
SAO₂ Accuracy: Adult 70-100% ± 2 digits
 Adult 50-69% ± 3 digits
 Neonatal 70-94% ± 3 digits
Heart Rate Source: ECG or Pleth, selectable
Pulse Rate Range: 35-250 beats/minute
Pulse Rate Accuracy: ± 3 beats/minute
High Limit Range: High 70-100%
Low Limit Range: Low 50-100%
Operating Modes: NORM = 5-7 seconds
 FAST = 2-3 seconds
 SLOW = 10-15 seconds
Calibration: Automatic
Sensors: Neonatal to Adult (NELLCOR)
Pulse Tone: Pitch varies with O₂ SAT

PRESSURE (OPTIONS 13E, 14E)

Channels: One (Opt. 13E), two (Opt. 14E)
Range: -40 to 300 mmHg
Accuracy: $\pm 1\%$ or ± 1 mmHg
Parameter Display: SYS, DIAS, and MEAN
Alarm Parameter: SYS, DIAS, or MEAN
Limit Range: 5 to 250 mmHg
Sweep Speed: 12.5, 25 mm/sec selectable
Display Scale: 30, 60, 120, 240 mmHg selectable
Cursor Bar: Selectable level, 1 mmHg steps
Input Connector: Standard 6 pin MS
Display: Pulse or scaled waveform, selectable
Heart Rate Source: ECG or BP1, selectable
Sensitivity: 5 uV/V/mmHg, softkey gain adjust
Zero Range: ± 100 mmHg, auto zero
Calibration: 100/50 mmHg squarewave
Isolation: Full electrical isolation
Auto Transducer Detect

INPUT/OUTPUT CONNECTORS

Defib Sync Out	Defib Marker In
Analog Out	HR Out
RS232 Interface	Alarm Out
	Record Out

PHYSICAL

Size: 7" (H) x 7" (W) x 8 1/2" (D) with battery and recorder

Weight: 9 lbs.

Add 1 lb. for NIBP option

Add 1 lb. for Recorder option

Add 3 lbs. for Batteries

Environment: 5 to 40 degrees C

0 to 90% humidity

AC Main: Selectable 110/220 VAC $\pm 10\%$, 60/50 Hz

Power: 35 watts

Certification: UL 544 & CSA pending

PATIENT CONNECTIONS

All inputs are CF protected.

SYSTEM OVERVIEW

CHAPTER 2

2.0.0 SYSTEM OVERVIEW

The **ESCORT 300A** is a three trace patient monitor designed for transport applications. It can be configured at the factory for a variety of uses depending on the requirements of the user. All **ESCORTs** are configured for ECG. With the addition of various processor boards and enhanced software. NIBP, temperatures, invasive BP, respiration, and SaO₂ can also be included.

The **ESCORT 300A** can be equipped with a defibrillator (option 19E), or a defibrillator/noninvasive pacer (option 20E). When the defibrillator or defibrillator/noninvasive pacer option is ordered, a mounting plate is added to the monitor. This will allow the **ESCORT 300A** to mount on to the defibrillator or defibrillator/pacer unit.

The **ESCORT** has a minimum of three PCBAs and a maximum of four. These include a CPU board, ECG board, Temp-Press board, and Switching Power Supply board.

The CPU board handles the various processing tasks for the monitor as well as interfacing between the processor boards, the display (LCD or EL), and the recorder. Keyboard decoding is located on the CPU board, as are the High Level Outputs. The HL outputs are available at the aux connector on the rear Panel .

ECG, temperature, respiration, NIBP/BP, and SaO₂ signals are input to the processor boards via the connector plate on the right side of the monitor. These inputs are isolated from line current by the use of opto-couplers. The signals that are input are filtered and then converted from analog to digital format. Further processing and calculating will be done before the data is sent to the CPU board through the edge connector. The CPU will then process the data and send it to the display and the Recorder.

The Switching Power Supply provides necessary operating voltages through one of two methods: An AC outlet, or internal battery power. Battery level indication is measured on the Switching Power Supply board.

The Switching Power Supply board also incorporates battery charging by providing charging current to the batteries. When the unit is *not* being used for monitoring, the batteries are charged at the maximum current rate; when the **ESCORT 300A** is *in use*, the batteries are charged at minimum current to reduce total power consumption.

2.1.0 ESCORT RS-232 Communication Protocol

ESCORT 300A monitors include an RS-232 interface for data acquisition by the user's clinical information system. Virtually all information displayed on the ESCORT monitor is available for serial transmission, including parameter values, alarm status, leads status, remote status and waveform information. The clinical information system used should have an unused serial port that operates under the EIA (Electronics Industry Association) RS-232C standard. This protocol is only valid for main software versions 7.66 and higher and ESCORT monitors with a main CPU board level Revision O as a minimum. The software version may be obtained by calling up the TEST page of the ESCORT monitor. Refer to the ESCORT 300A Operator's Manual for instructions.

WARNING!

Do not attempt accessing RS-232 information unless you are familiar with UART (Universal Asynchronous Receiver and Transmitter) operation and setup. Only qualified and experienced technicians or programmers should attempt using the following protocol. The user will be required to develop program code to access and display the acquired data.

UART configuration for serial communications is 9600 baud, one (1) start bit, eight (8) data bits, two (2) stop bits, and no parity. In its default condition, ESCORT monitors transmit two packets of information: a parameter packet followed by an ECG waveform packet.

A parameter packet is illustrated below. Parameter sequence and identification are outlined in Table 1. The tabular references located above some of the blocks in the figure below will point toward additional information. All checksums are modulo 256 over the indicated ranges.

Table 2	Table 3		Table 3				Table 4		
2 byte ID ESC,P	3 byte parameter #0	3 byte parameter #1	<i>parameters #2 thru #11</i>	3 byte parameter #12	1 byte HR limit HIGH	1 byte HR limit LOW	1 byte Remote Status	2 byte Spare	1 byte CHECK SUM

Parameter Packet: The two byte ID is generated by the ESCORT monitor, see Table 5 for details

The three byte parameter blocks (referenced #0 through #12 above) are broken down as follows:

2 byte Data (0-500)	1 byte ECG Status
---------------------------	-------------------------

3 Byte - Parameter #0 (ECG)

The *first two bytes* contain the value of the parameter measured (in this case, ECG) within a range of zero to five hundred (0 -500). Data is transmitted LSB, MSB.

The *third byte* contains ECG status information as described in Table 2.

2 byte Data (0-500)	1 byte Status
---------------------------	------------------

3 Byte - Parameters #1 through #12

The *first two bytes* contain the value of the parameter measured within a range of zero to five hundred (0 -500). Data is transmitted LSB, MSB.

The *third byte* contains parameter status information as described in Table 3.

1 byte HR limit HIGH

1 Byte - Number representing heart rate HIGH alarm limit

1 byte HR limit LOW

1 Byte - Number representing heart rate LOW alarm limit

1 byte Remote Status

1 Byte - Remote Status (See Table 4)

The ECG waveform packet immediately follows the parameter packet. It is identified by its three byte ID (ESC, W, <Waveform No.>) followed by a length byte. The length byte represents the number of bytes that include waveform data. Waveform resolution is limited to 00h - FEh (254 decimal). FFh (255d) sets a pacer flag which may be used for pacer detection (only sent when PACER ON is selected, and the ECG software version is 7.11 or later).

Transmitted waveform information varies in ESCORT monitors configured for 110V/60Hz and 220V/50Hz. Please note caption information in the following waveform packet descriptions to determine the anticipated waveform information for your ESCORT monitor.

3 byte ID ESC, W, <Waveform No.>	1 byte length (bytes)	approx. 160ms of data sent at a sample rate of 120Hz; length is specified by length byte	1 byte CHECK SUM
--	-----------------------------	--	------------------------

**Waveform packet information for
110V/60Hz ESCORT monitors
ONLY**

3 byte ID ESC, W, <Waveform No.>	1 byte length (bytes)	approx. 200ms of data sent at a sample rate of 100Hz; length is specified by length byte	1 byte CHECK SUM
--	-----------------------------	--	------------------------

**Waveform packet information for
220V/50Hz ESCORT monitors
ONLY**

As previously stated, the ESCORT monitor transmits two packets of information: a parameter packet and an ECG waveform packet. The user's computer may request an additional waveform by issuing the following command:

ESC, R, <Waveform No.>

The ESCORT monitor will respond by sending the additional waveform packet in the previously described format (i.e., ESC, W, <Waveform No.>). Only one additional waveform may be acquired at a time. *IMPORTANT - Remember differences in transmission information for 110V/60Hz and 220V/50Hz!*

The additional waveform packet will be sent in sequence after the ECG waveform packet. A review of the overall sequence would be:

PARAMETER - ECG WAVEFORM - ADDITIONAL WAVEFORM

It is particularly important that special attention is applied when counting the number of bytes received and to properly use the waveform length byte to locate the appropriate waveform data. To change to a different *additional* waveform or to simply stop the acquisition of the current waveform, the selection in use must be turned off. This is accomplished by issuing the following command:

ESC, R, O

Note: The ECG waveform packet always follows the Parameter packet by default and may not be turned off.

Wiring information may be found in Figure 1, located at the end of this section.

Parameter	Order	Waveform Number
ECG	0	0
RESP	1	1
BP1 systolic	2	2
BP1 diastolic	3	
BP1 mean	4	
BP2 systolic	5	5
BP2 diastolic	6	
BP2 mean	7	
NIBP systolic	8	not available
NIBP diastolic	9	not available
NIBP mean	10	not available
SaO ₂	11	11
TEMP	12	not available

Table 1
Order of parameters within packet

Note: TEMP (Temperature) is transmitted as an integer value with a range between 200 and 500 (Base 10). Each integer represents one tenth degree Celsius (0.1° C). This translates to an actual temp range transmitted that is between 20 and 50 degrees Celsius (20° — 50° C).

ECG Status	Bit Position	Description
ECG Lead Loose (no connection)	0	leads not connected or loose
HR Alarm ON	1	an alarm is set for ECG
HR "IN ALARM"	2	a heart rate limit has been violated
HR Source Not ECG	3	heart rate is set for another source
Telemetry in Squelch (lead-fail)	4	send lead-fail message when telemetry is in squelch

Table 2
ECG Status (Bit Value: 1 = true, 0 = false)

Parameter Status	ASCII Value	Hex Value	Description
Connected and Alarms On	N	4Eh	Parameter is installed, connected and alarm is enabled
Connected and Alarms Off	F	46h	Parameter is installed, connected and alarm is disabled
Connected in Alarm	A	41h	Parameter is installed, connected and in alarm condition
Disconnected	D	44h	Parameter is installed but not connected
Not Available	V	56h	Parameter is not installed
Not Zeroed	Z	5Ah	BP1 or BP2 have not been zeroed

Table 3
Parameter Status (ECG, see Table 2)

Remote ESCORT Status	Hex Value	Description
Null Status	00h	No activity
Low Battery	10h	Battery Voltage is Low
ESCORT Alarm Suspend	70h	Alarm Suspend Activated

Table 4
Remote Status

Note: In the event that a low battery condition occurs coincident with an alarm suspend, the ESCORT monitor will prioritize the event. Priority will be given to the low battery signal and ESCORT will transmit 10h.

Action	Identification Commands (ASCII)	Identification Commands (HEX)	Source
Parameter Packet Transmission	ESC , P	1B, 50	ESCORT
Waveform Packet Transmission	ESC , W , <Waveform No.> (See Table 1)	1B, 57, <Waveform No.> (See Table 1)	ESCORT
Request by User's computer for additional waveform	ESC , R , <Waveform No.> (See Table 1)	1B, 52, <Waveform No.> (See Table 1)	Clinical Information System
Turn off transmission of all waveforms except ECG	ESC , R , O	1B, 52, 4F	Clinical Information System

Table 5
Packet Identification Codes




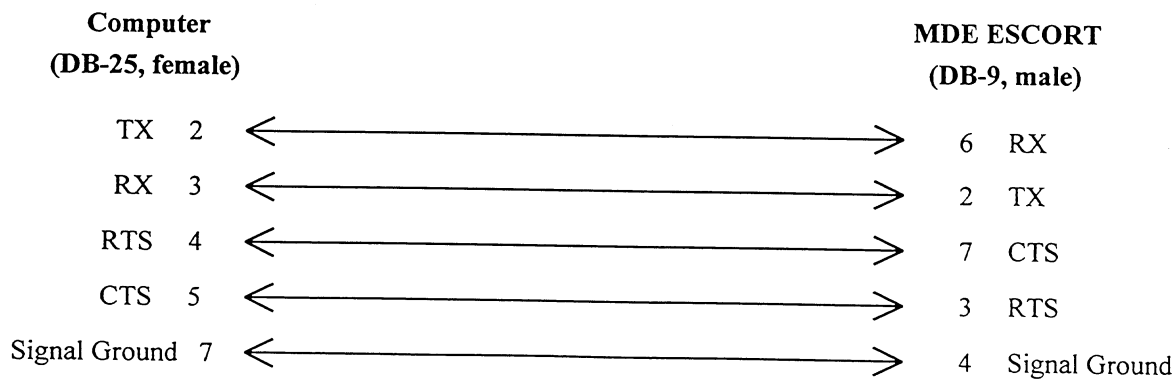


Figure 1
RS-232 Wiring Diagrams

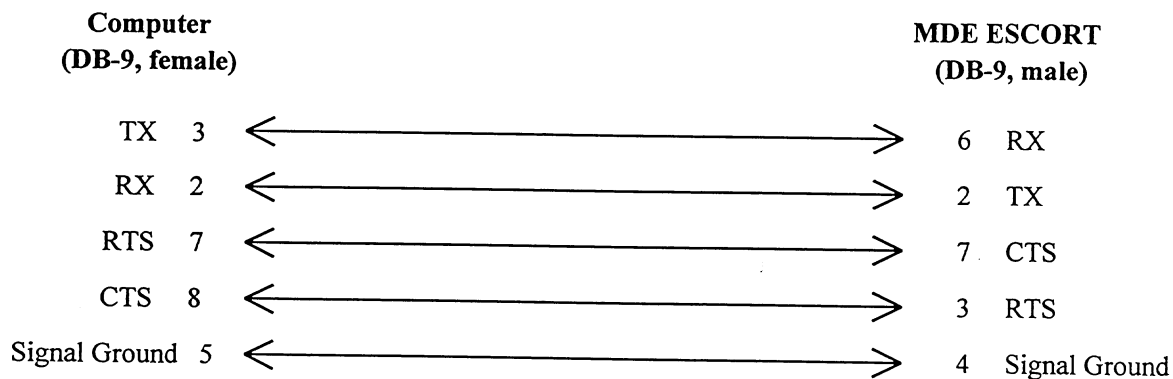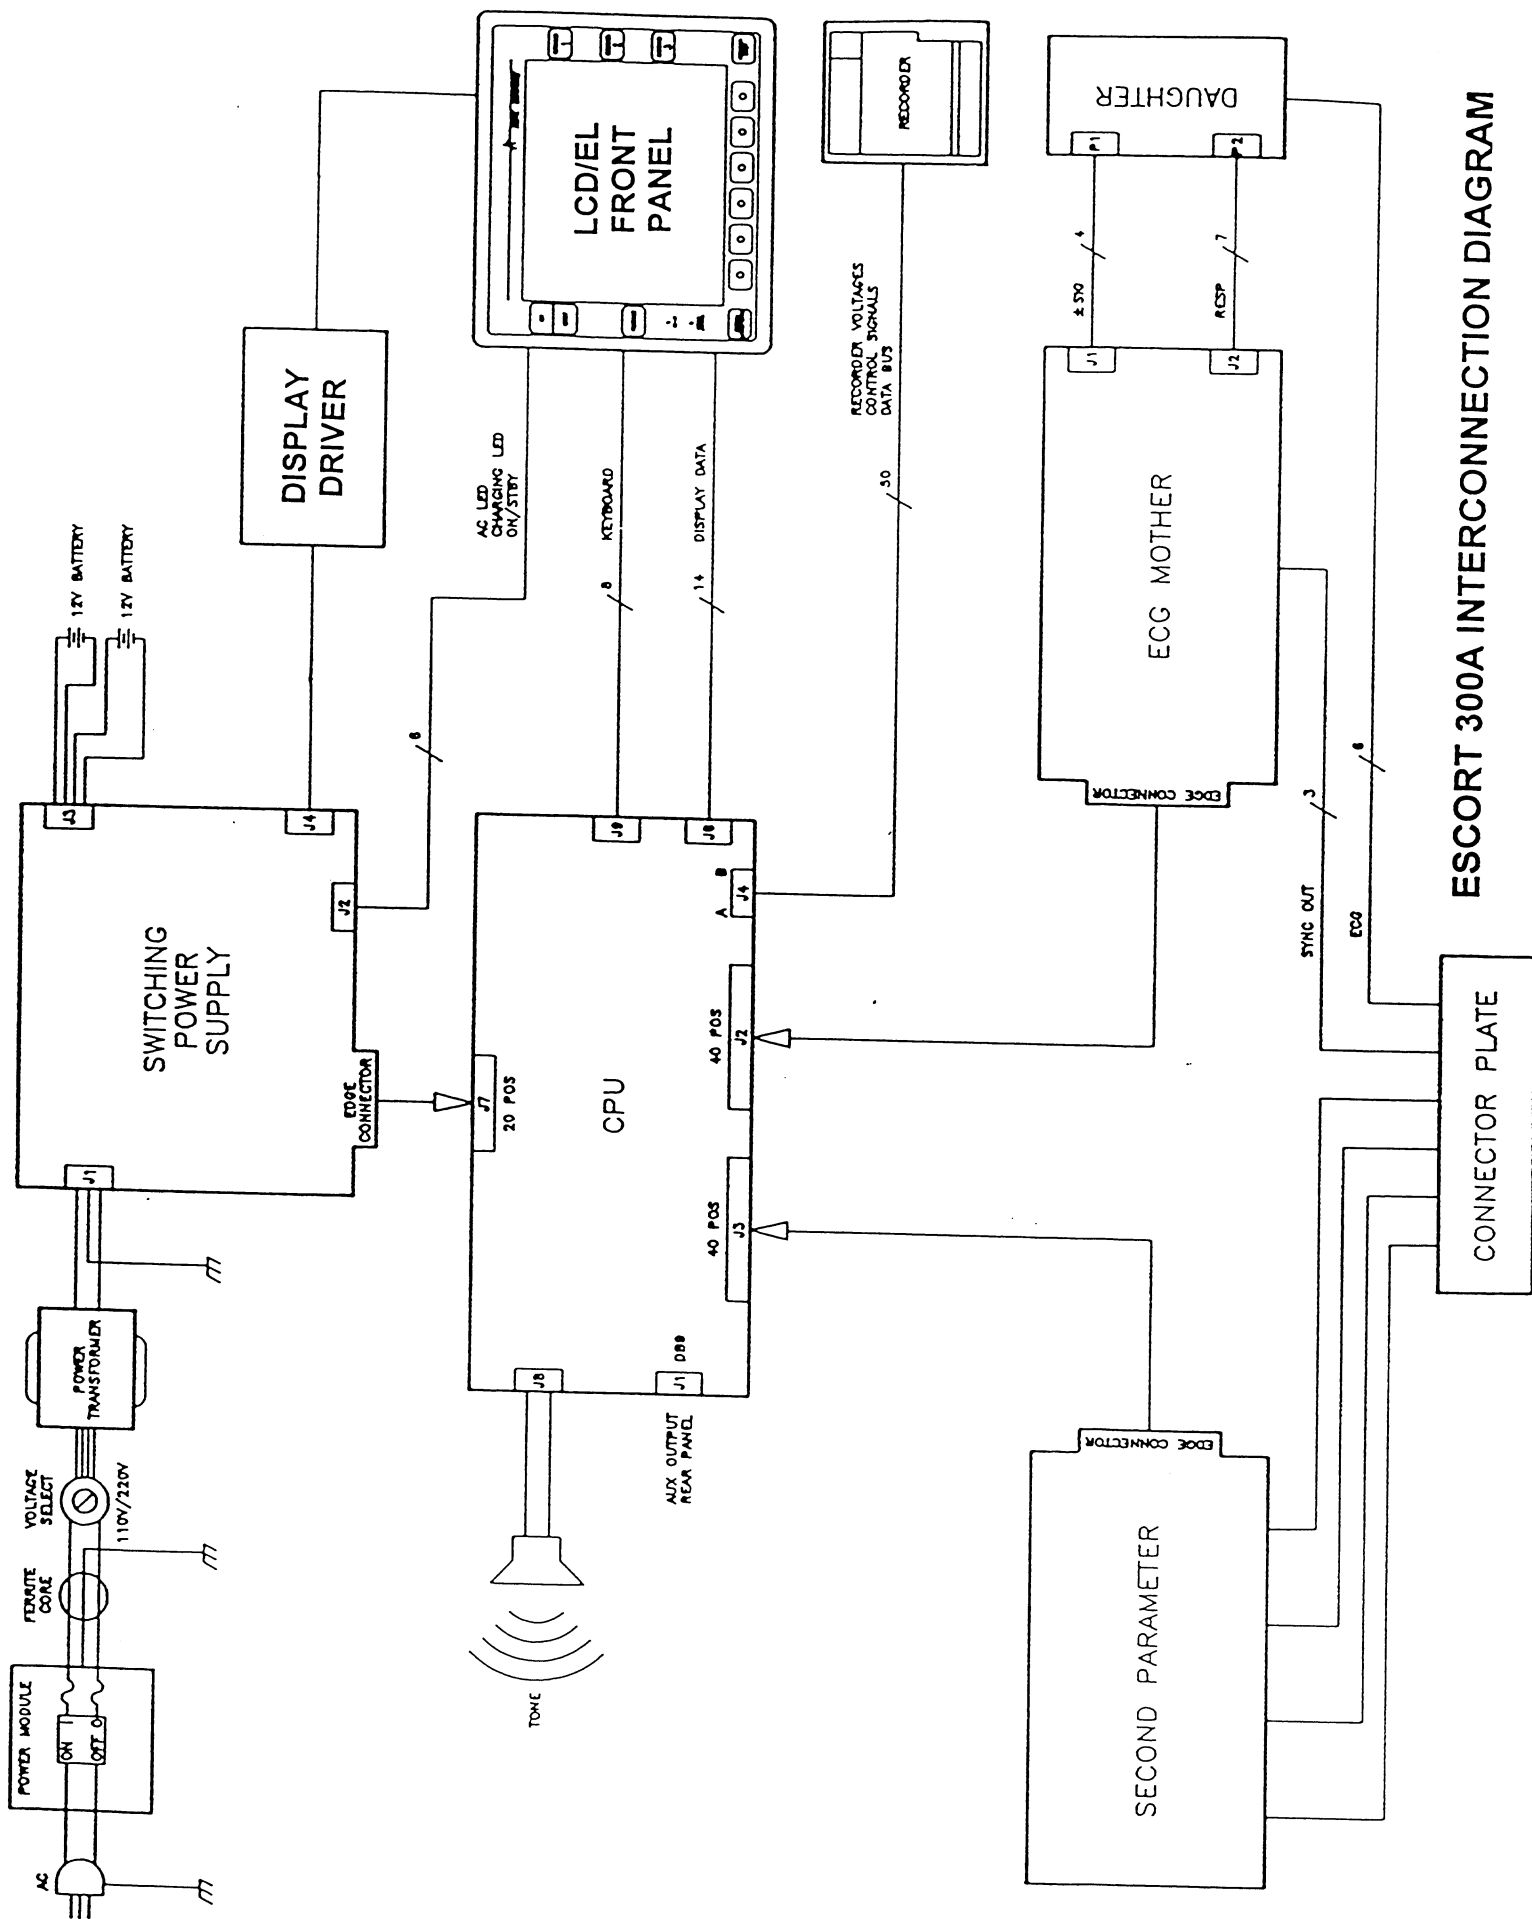

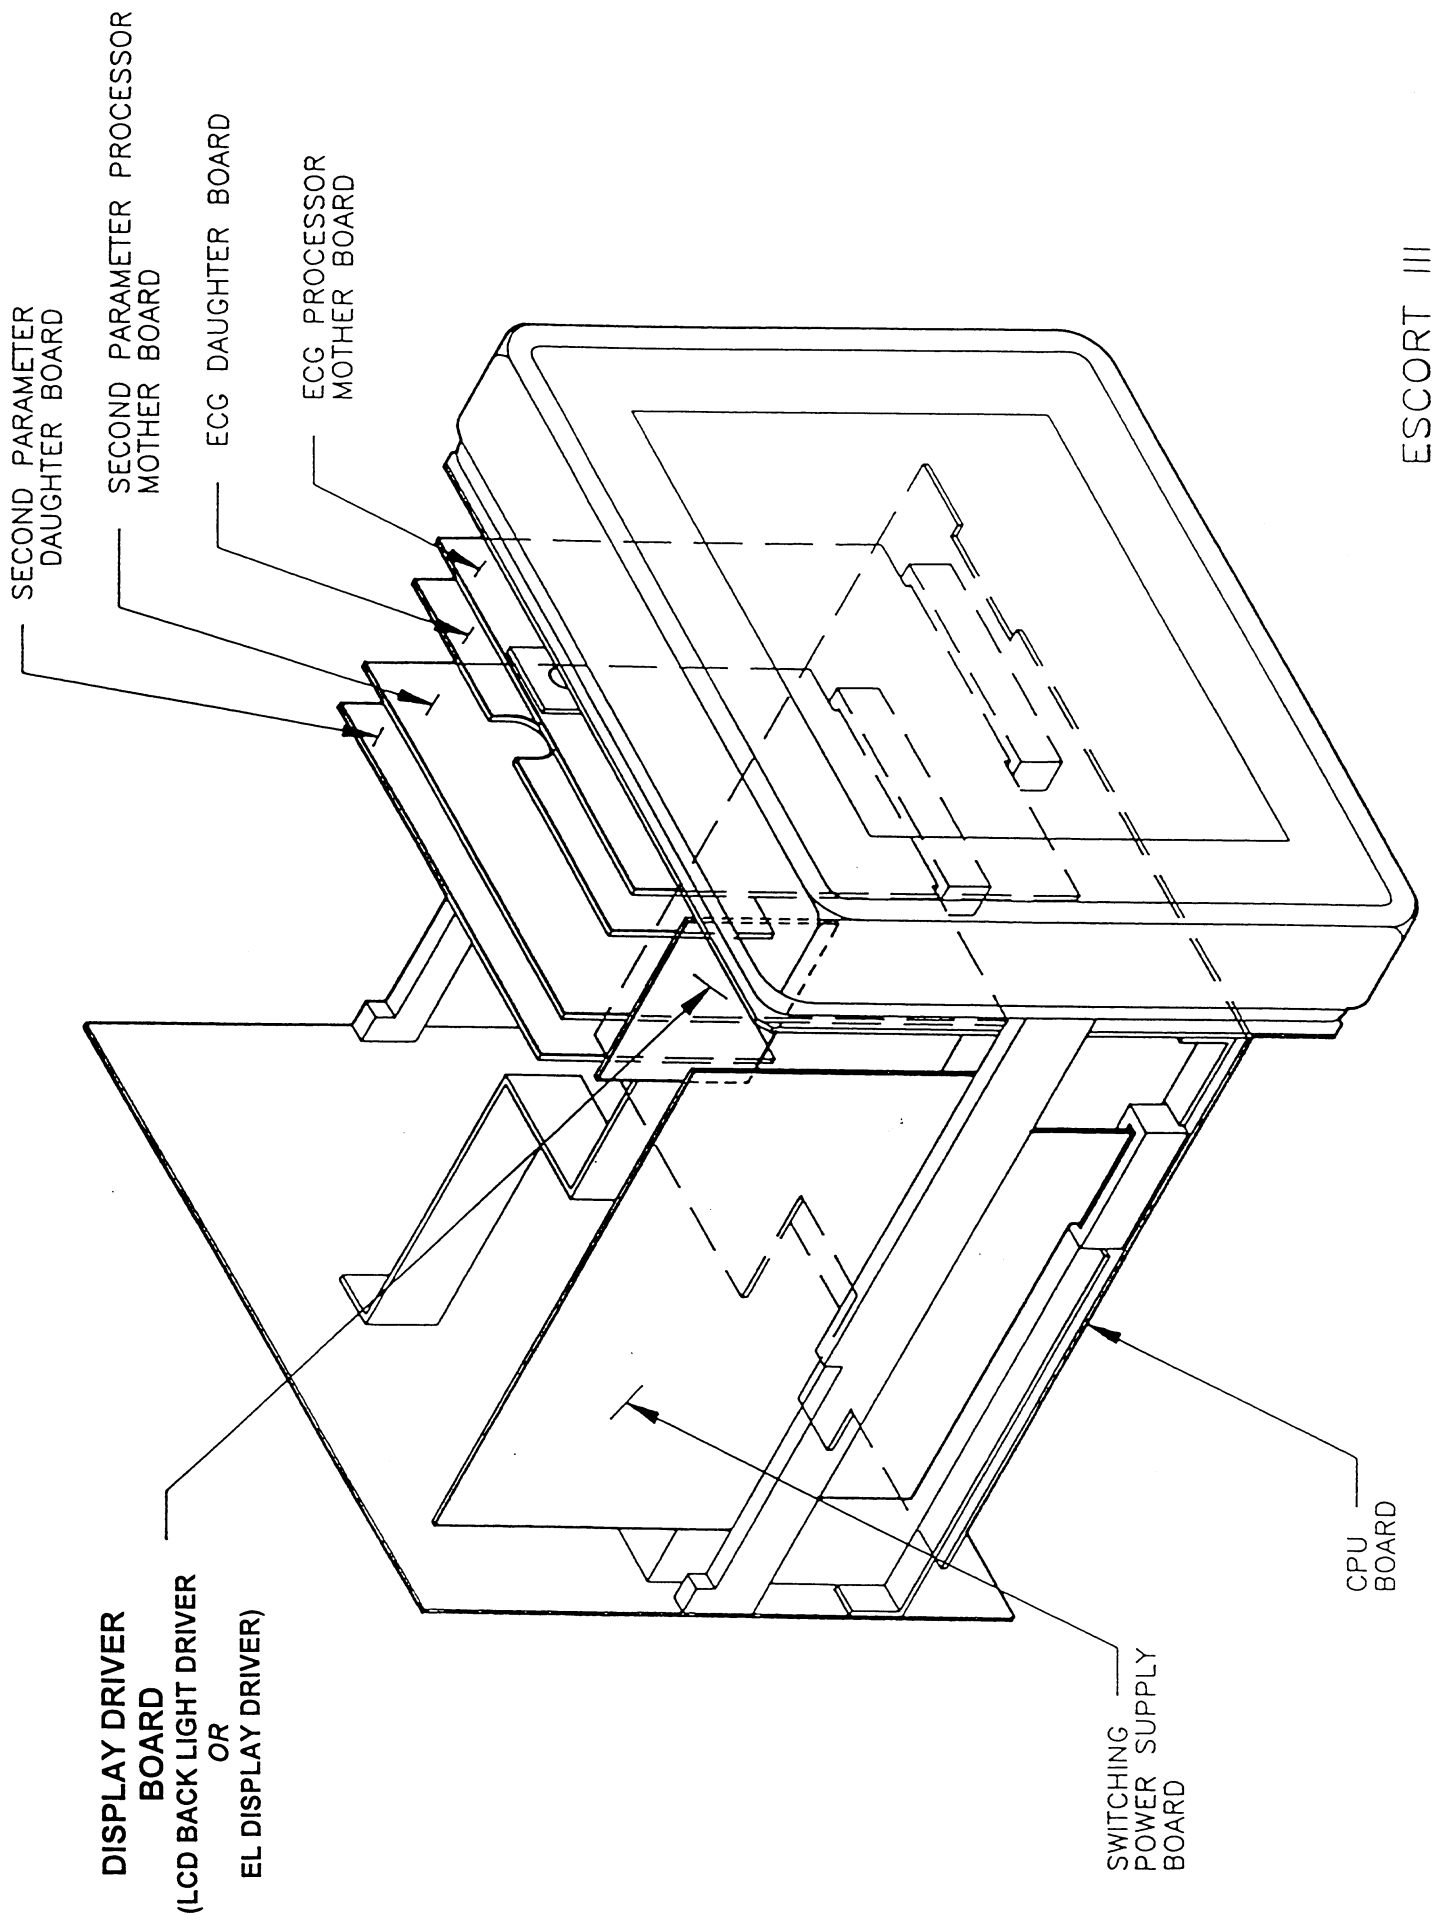

ESCORT III
BOARD LOCATION DIAGRAM

CPU BOARD

CHAPTER 3

3.0.0 CPU OVERVIEW

3.1.0 OVERVIEW

The CPU board controls the system functions of the ESCORT. It generates timing signals and holds the monitor configuration in the EPROM. It stores the softkey setup in the RAM, and retains it with a battery backup. A peripheral I/O chip generates and receives essential operating signals, and a keyboard decoder identifies and debounces key depressions. The microprocessor controls the display, either a backlit Liquid Crystal Display (LCD) or an Electroluminescent (EL), via a video controller chip. CPU computing, softkeys, alarms and recorder functions are also controlled by the CPU board.

3.2.0 MICROPROCESSOR

The microprocessor chip used on the CPU board is a Hitachi 64180. It is an 8-bit high integration CMOS chip with internal memory management, DMA control and a Z80 type CPU. It has 18 address lines that can access 512K memory or I/O. Pins 34-41 are on the data bus and pins 13-30 are on the address bus. Basic timing for the processor is derived from Y1, a 16 MHz crystal input to pins 2 and 3. The processor divides this signal internally by two for an 8 MHz timing output at pin 64. The WAIT* signal at pin 4 is to introduce bus cycle waits as needed by the Dual Port RAM. Pins 47 and 54 are used for DMA Requests. The RECORDER SYNC (REC. SYNC) input at pin 11 of U13 will let the CPU know if the recorder's buffer is full. This enters the CPU at pin 10 as the signal INT1*. Rec Busy (INT2*) at pin 11 is not used. Pin 8 is a non-maskable interrupt. A soft start circuit is implemented by, RESET*, pin 7, being held low by C50 slowly charging. MEMORY ENABLE* (ME*) pin 59 and READ* (RD*), WRITE* (WR*) pins 63 and 62 are gated together to produce the signals Memory Read* (M/R*) and Memory Write* (M/W*). These signals are used to write to and read from the ROM and RAM chips, U16 and U17. The same gating logic is used to derive I/O Read* (IO/R*) and I/O Write* (IO/W*) from IOE* pin 58 and WR*, RD* pins 62 and 63.

3.2.1 TIMING

The 8 MHz clock from pin 64 is further divided by the flip flop, U10. The 4 MHz clock goes to U11 pin 2. U10 clocks U11, producing the POWER SUPPLY SYNCHRONIZING signal (P.S. SYNC) at pin 15. This signal coordinates all generated voltages to switch on the same edge. The 4 MHz clock from also goes to U12 pin 2, which divides the 4 MHz clock by 13. The signal then returns to U10 at pin 11 where it is divided by two. The result is a 153.8 KHz signal called BAUD RATE at pin 12. This signal goes to the microprocessor U4 at pin 50 and controls external baud rate communications.

3.2.2 DISPLAY ENABLE

U9 controls reading and writing to and from the processor boards and the display (LCD or EL) with the signals SLOT1*, SLOT2*, and LCDEA*. The SLOT1* and SLOT2* signals go out to the connectors J2 and J3 respectively, while the LCDEA* goes to Display Driver U21 at pin 56 and enables the display.

3.2.3 CHIP ENABLE

The multiplexer U6 issues control signals to enable most of the monitor's functions. The PORTIO* signal enables the Peripheral I/O U14 at pin 6. The ADCSEL* signal enables the analog to digital converter U25 at pin 1. The DACSEL* signal enables the digital to analog converter U20 at pin 1. The CLKSEL* signal enables the clock U19 at pin 2. The SOUND* signal enables the sound chip U30 at pin 2.

3.2.4 PERIPHERAL I/O (P I/O)

U14 is a peripheral I/O chip that is enabled through U6 by PORTIO* and address line A9. U14 interfaces critical system information and tasks to and from the microprocessor, including BATTERY CHARGER CONTROL, AC DETECT, RECORDER RESET and KEYBOARD DATA.

3.2.5 KEYBOARD DECODER

The keyboard decoder, U18, has a four-line matrix of four rows (Y) and four columns (X). The columns are scanned at a rate set by C7 and C8. With a key depression, the appropriate X and Y input will go low, disabling the counter. Internal and external circuitry (C9) will debounce the key by locking out the other Y inputs, timing out and then latching the data. DATA AVAILABLE (KEY DA) will also go high. U18 is enabled via U7 at pin 13 and will put data on the bus through pins 14-17.

3.2.6 TIME OF DAY CLOCK

U19 is a real time clock module (RTC-72421). It has a built in quartz oscillator, time and date function and CMOS circuitry for low power consumption. The time and date are displayed on the test page and annotated on the recorder strip. U15 monitors +5 volts, which is the operating voltage for U19. If +5 volts drops below a critical level, U15 will switch to the battery backup for the operating voltage. This will retain accurate time and date.

3.2.7 MEMORIES

The memory chips are U17, a 64K X 8 bit EPROM and U16, a 32K X 8 bit static RAM. U17 is enabled by the address line A17 at pin 22 and U16 is enabled from the address decoder U9 through U8. The enable signal is received by U16 at pin 22. U15 monitors +5V at pin 1; if the voltage falls below critical level, U15 will inhibit the select line (CEO) at pin 12 and switch VCC to the battery. The 2.4V nicad battery supplies enough voltage to retain RAM information, but not for operation in the event of the loss of +VCC. The battery is trickle charged through R16 and D3.

3.2.8 LCD CONTROL

The E300A standard display is a flat screen LCD controlled by the video driver U21. The LCD is enabled by the signal LCDEA* from address decoder U9. The 8 MHz signal from pin 64 of the CPU enters at pin 54. Resetting takes place via the signal RESET*, originating at the reset timer, U15, and entering the video driver at pin 47.

U23 is the video RAM, allowing access of stored information by the video driver U21.

The signal CONTRAST is generated at U28 and sent directly to the LCD through J6. This signal is incremented up or down by the user via the keypad in order to adjust the viewing angle.

3.2.9 EL CONTROL

The E300A may be configured with an Electroluminescent (EL) display (Option 22E). The EL display is controlled by the video driver U21. The EL display is enabled by the signal LCDEA* from address decoder U9. The 8 MHz signal from pin 64 of the CPU enters at pin 54. Resetting takes place via the signal RESET*, originating at the reset timer, U15, and entering the video driver at pin 47.

U23 is the video RAM, allowing access of stored information by the video driver U21.

The EL Display receives its power from the EL Display Driver Board. The EL Display Driver produces the voltages necessary for operation and control of the EL Display. It is sourced by the Switching Power Supply (+15V and +24V). The +15V from the Switching Power Supply is regulated to +5V and +12V. T1 on the EL Display Driver Board outputs -175V, -87V, +215V, +107V, +40V, and +20V. All voltages are then routed to the EL Display via the EL Interface Board. The EL Display Driver Board schematic and layout may be found later in this chapter.

3.2.10 ANALOG VOLTAGES

Various analog voltages for the CPU board are generated by the DAC, U20, and the sample and hold circuitry that includes U24. U20 is addressed as an I/O device. It takes data off the bus and decodes it for the appropriate voltage. U20 then outputs this voltage to U24. U24 selects an output by the signals DMUX1, DMUX2, DMUX3 and DMUX4. U24 will route the input at pin 3 to the selected output. The capacitors at the output pins will charge and hold the voltage. U27 and U28 are unity gain buffers. The exception to unity gain is the output at pin 7, which controls the LCD contrast. Its associated opt-amp has gain built into the circuitry.

3.2.11 AUXILIARY OUTPUTS

Two high level output pins are available to the user. These pins are located on the J1 connector at the rear panel. Port #1 is pin 9. Port #2 is pin 8. Pin 5 is analog ground.


Each port can be defined by the user under the CONFIG page of the ESCORT softkeys. Each key has three modes, each with a number of possibilities:

1. The WAVEFORM (WF) mode causes the port to output a waveform or parameter value. The selections are as follows:
 - AUTO — The waveform that is currently displayed on the screen is output. Port 1 reflects Trace 2.
 - ECG — The ECG waveform is always output. Signal level is approximately 1V/mV and rides on a 2.5V baseline level.
 - BP1 or BP2 — The pressure waveform is always output. 0mmHg = 0V, and 250mmHg = 2.5V.
 - RESP — The respiration waveform is always output. The signal level is approximately 1V/1 ohm and rides on a 2.5V baseline level.
 - HR — The cardiach information will be output and updated every 200ms. 1V = 50BPM, and 2V = 100 BPM.
 - T1 or T2 — The temperature values are always output. 0 degrees C = 0V and 50 degrees C = 5V.
 - Pleth — Pleth waveform output is centered on 2.5V level.
 - SaO₂ — Percentage is SaO₂ output (4V = 100%).
2. The ALARM (ALM) mode can send different alarm conditions to the port. In all cases 0V = no alarm and 5V = alarm condition.
 - ANY Enables on any alarm condition.
 - FLASH Will toggle the port on any alarm condition.
 - ECG Enables on ECG alarms only.
 - BP1 Enables on BP1 alarms only.
 - BP2 Enables on BP2 alarms only.
 - RESP Enables on respiration alarms only.
 - T1 Enables on temperature 1 alarm only.
 - T2 Enables on temperature 2 alarm only.
 - SaO₂ Enables on SaO₂ alarm only.
3. The KEY mode will reflect recorder condition:
 - ANY Enables when either REC1, REC2, or REC3 key has been selected.
 - REC1 Enables only when REC1 key is selected.
 - REC2 Enables only when REC2 key is selected.
 - REC3 Enables only when REC3 key is selected.


3.2.12 REGULATORS

U33 regulates +5V from the +8V input at pins 1 and 2 of J7 . U34 and U35 will regulate +12V and -12V from the +15V and -15V input. These input voltages are from the switching power supply board. VRAW comes in on J7 pin 11, to the ADC U2, to determine battery condition. LOW=10.6V or lower, MID=10.6V to 11V, and HIGH=11V and above.

ESCORT III CPU BLOCK DIAGRAM

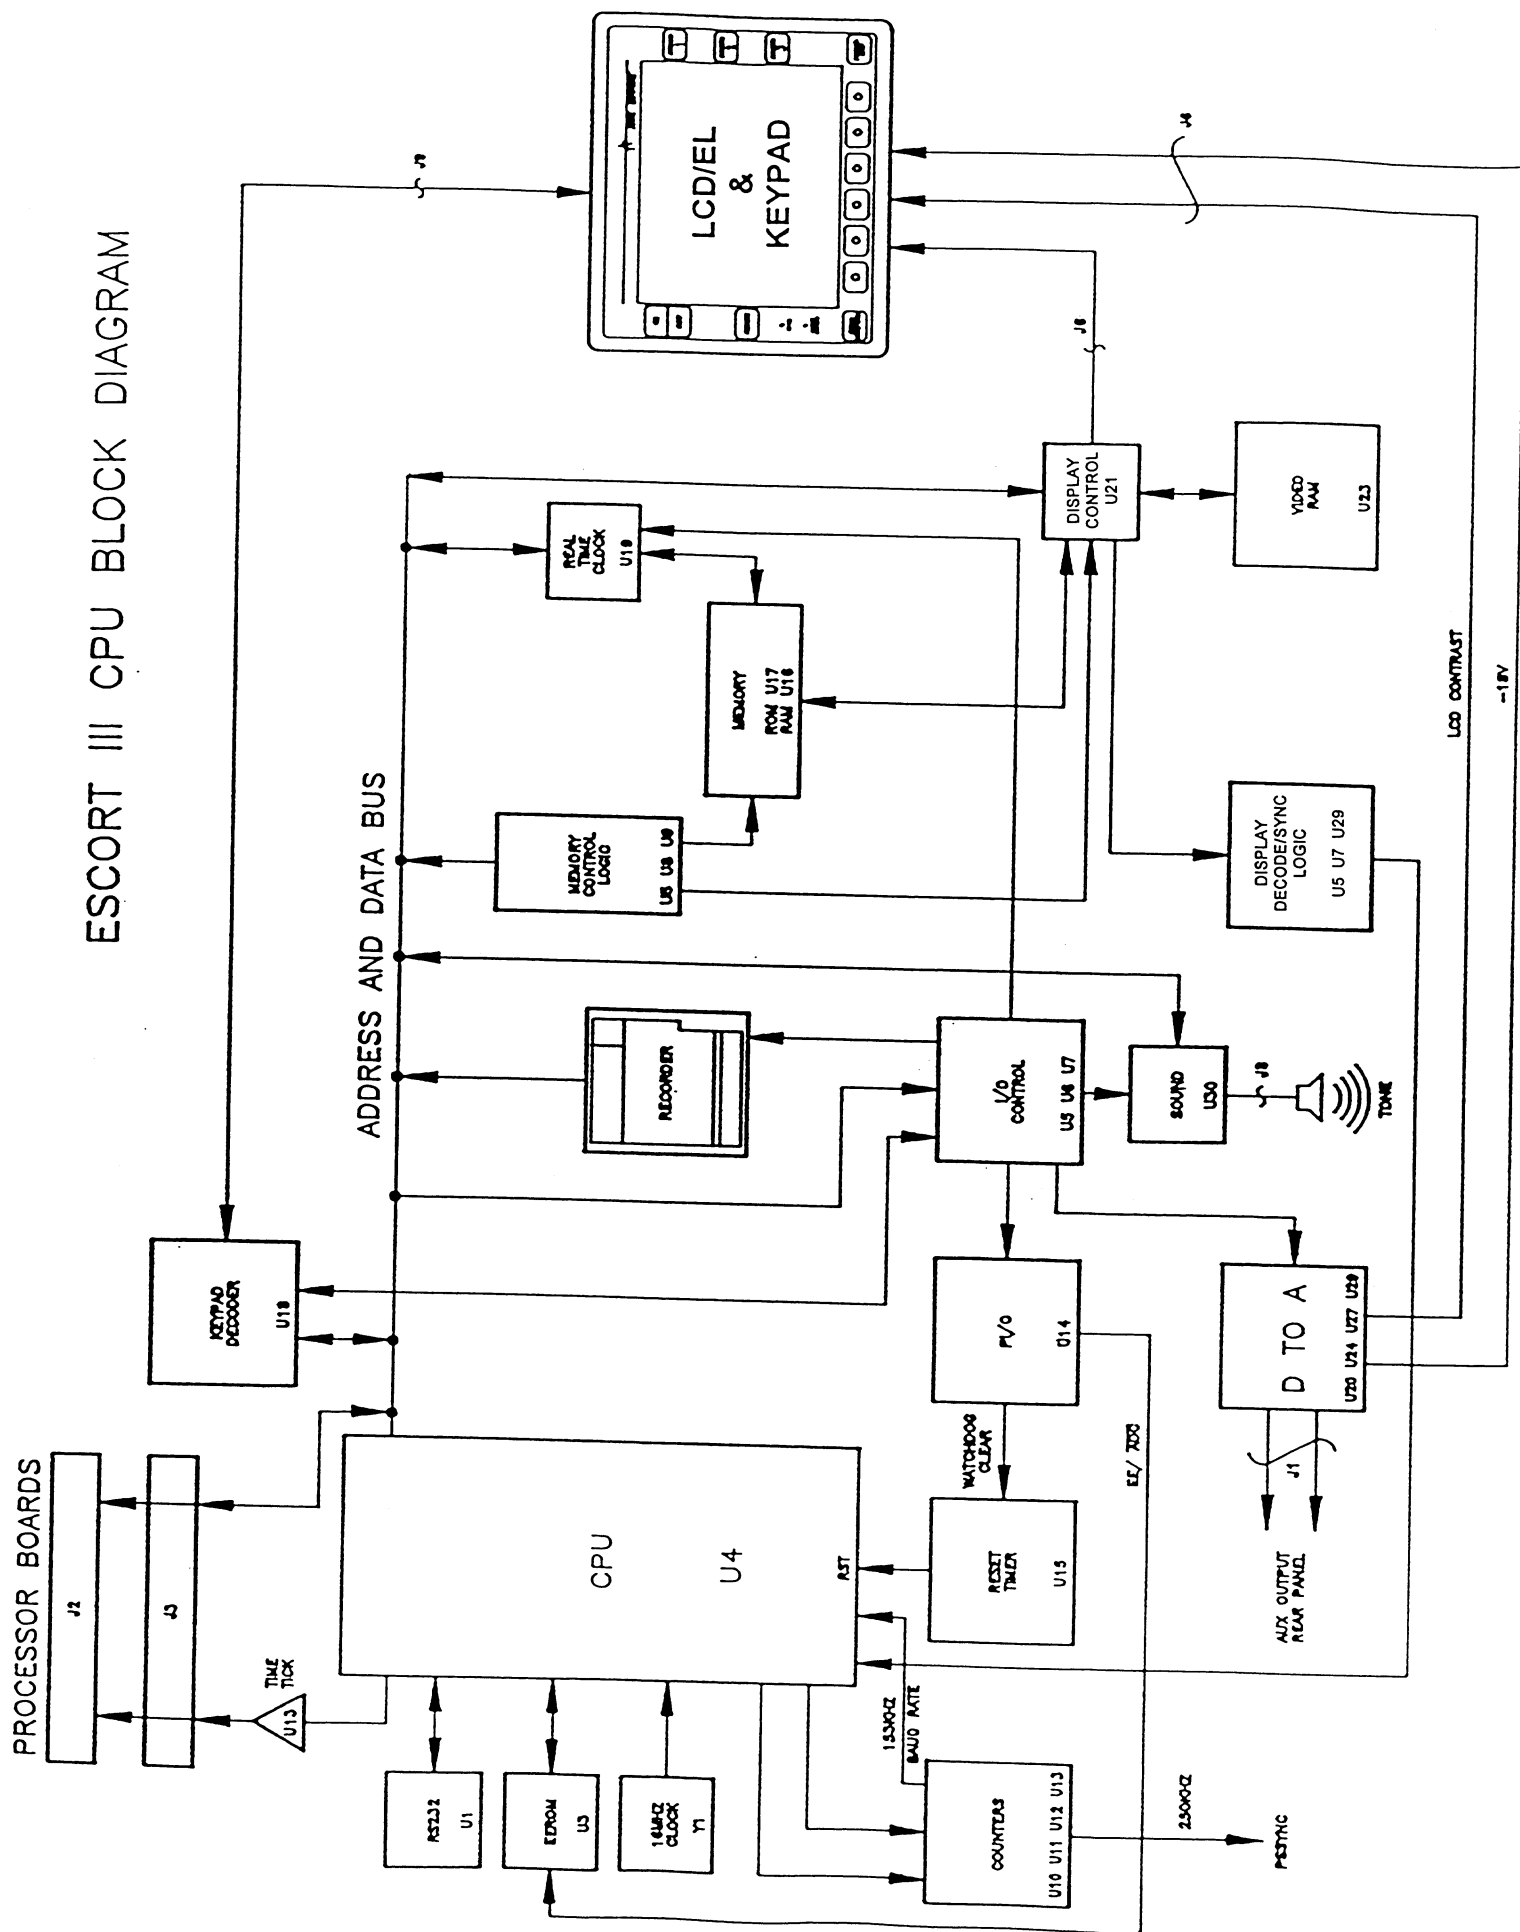

REV	DESCRIPTION	DATE
1	ECO 713	5-3-1991
2	ECO 713	5-3-1991
3	ECO 713	5-3-1991
4	ECO 713	5-3-1991
5	ECO 713	5-3-1991
6	ECO 713	5-3-1991
7	ECO 713	5-3-1991
8	ECO 713	5-3-1991
9	ECO 713	5-3-1991
10	ECO 713	5-3-1991
11	ECO 713	5-3-1991
12	ECO 713	5-3-1991
13	ECO 713	5-3-1991
14	ECO 713	5-3-1991
15	ECO 713	5-3-1991
16	ECO 713	5-3-1991
17	ECO 713	5-3-1991
18	ECO 713	5-3-1991
19	ECO 713	5-3-1991
20	ECO 713	5-3-1991
21	ECO 713	5-3-1991
22	ECO 713	5-3-1991
23	ECO 713	5-3-1991
24	ECO 713	5-3-1991
25	ECO 713	5-3-1991
26	ECO 713	5-3-1991
27	ECO 713	5-3-1991
28	ECO 713	5-3-1991
29	ECO 713	5-3-1991
30	ECO 713	5-3-1991
31	ECO 713	5-3-1991
32	ECO 713	5-3-1991
33	ECO 713	5-3-1991
34	ECO 713	5-3-1991
35	ECO 713	5-3-1991
36	ECO 713	5-3-1991
37	ECO 713	5-3-1991
38	ECO 713	5-3-1991
39	ECO 713	5-3-1991
40	ECO 713	5-3-1991
41	ECO 713	5-3-1991
42	ECO 713	5-3-1991
43	ECO 713	5-3-1991
44	ECO 713	5-3-1991
45	ECO 713	5-3-1991
46	ECO 713	5-3-1991
47	ECO 713	5-3-1991
48	ECO 713	5-3-1991
49	ECO 713	5-3-1991
50	ECO 713	5-3-1991
51	ECO 713	5-3-1991
52	ECO 713	5-3-1991
53	ECO 713	5-3-1991
54	ECO 713	5-3-1991
55	ECO 713	5-3-1991
56	ECO 713	5-3-1991
57	ECO 713	5-3-1991
58	ECO 713	5-3-1991
59	ECO 713	5-3-1991
60	ECO 713	5-3-1991
61	ECO 713	5-3-1991
62	ECO 713	5-3-1991
63	ECO 713	5-3-1991
64	ECO 713	5-3-1991
65	ECO 713	5-3-1991
66	ECO 713	5-3-1991
67	ECO 713	5-3-1991
68	ECO 713	5-3-1991
69	ECO 713	5-3-1991
70	ECO 713	5-3-1991
71	ECO 713	5-3-1991
72	ECO 713	5-3-1991
73	ECO 713	5-3-1991
74	ECO 713	5-3-1991
75	ECO 713	5-3-1991
76	ECO 713	5-3-1991
77	ECO 713	5-3-1991
78	ECO 713	5-3-1991
79	ECO 713	5-3-1991
80	ECO 713	5-3-1991
81	ECO 713	5-3-1991
82	ECO 713	5-3-1991
83	ECO 713	5-3-1991
84	ECO 713	5-3-1991
85	ECO 713	5-3-1991
86	ECO 713	5-3-1991
87	ECO 713	5-3-1991
88	ECO 713	5-3-1991
89	ECO 713	5-3-1991
90	ECO 713	5-3-1991
91	ECO 713	5-3-1991
92	ECO 713	5-3-1991
93	ECO 713	5-3-1991
94	ECO 713	5-3-1991
95	ECO 713	5-3-1991
96	ECO 713	5-3-1991
97	ECO 713	5-3-1991
98	ECO 713	5-3-1991
99	ECO 713	5-3-1991
100	ECO 713	5-3-1991

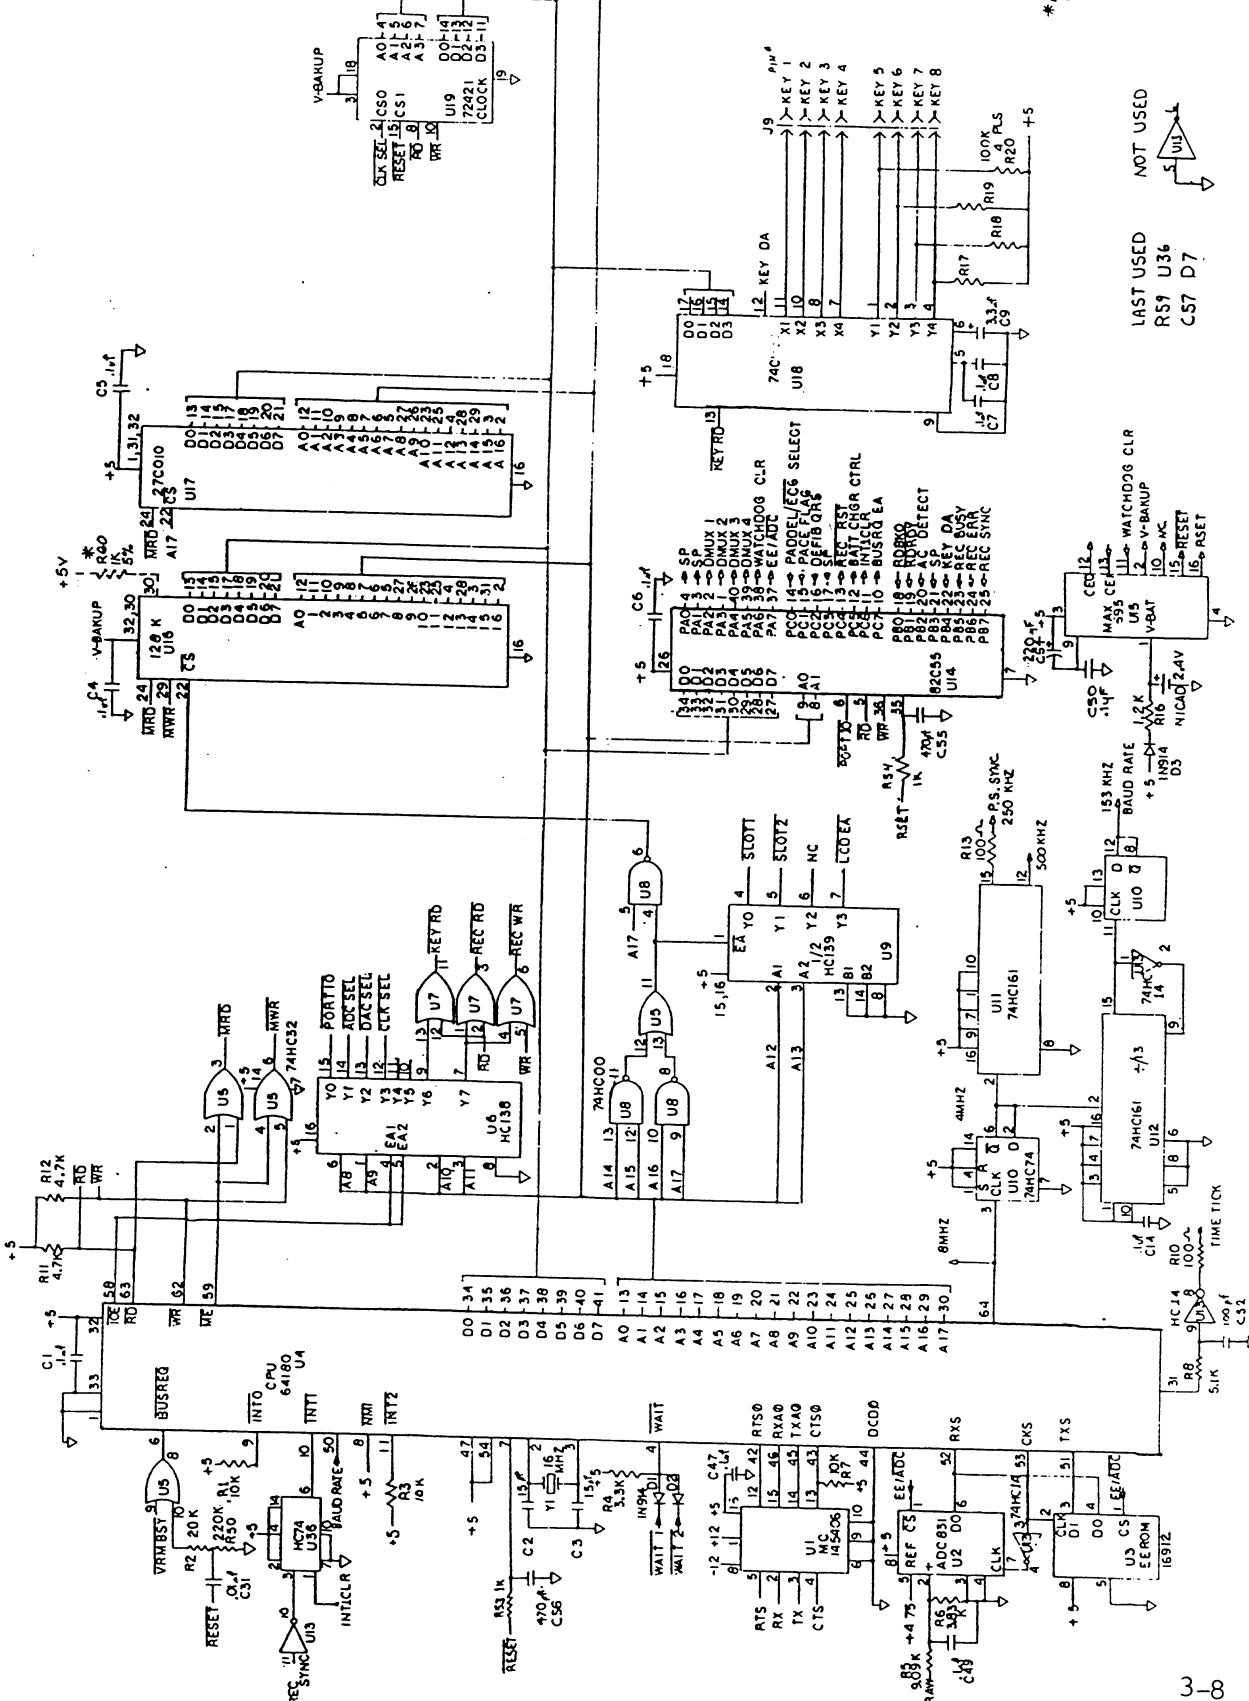



* DASHED LINES INDICATE COMPONENTS (LYING) OFF THE BOARD.

NOT USED
R59 U36
C57 D7

REV	DESCRIPTION	DATE
1	ECO 713	5-3-1991
2	ECO 713	5-3-1991
3	ECO 713	5-3-1991
4	ECO 713	5-3-1991
5	ECO 713	5-3-1991
6	ECO 713	5-3-1991
7	ECO 713	5-3-1991
8	ECO 713	5-3-1991
9	ECO 713	5-3-1991
10	ECO 713	5-3-1991
11	ECO 713	5-3-1991
12	ECO 713	5-3-1991
13	ECO 713	5-3-1991
14	ECO 713	5-3-1991
15	ECO 713	5-3-1991
16	ECO 713	5-3-1991
17	ECO 713	5-3-1991
18	ECO 713	5-3-1991
19	ECO 713	5-3-1991
20	ECO 713	5-3-1991
21	ECO 713	5-3-1991
22	ECO 713	5-3-1991
23	ECO 713	5-3-1991
24	ECO 713	5-3-1991
25	ECO 713	5-3-1991
26	ECO 713	5-3-1991
27	ECO 713	5-3-1991
28	ECO 713	5-3-1991
29	ECO 713	5-3-1991
30	ECO 713	5-3-1991
31	ECO 713	5-3-1991
32	ECO 713	5-3-1991
33	ECO 713	5-3-1991
34	ECO 713	5-3-1991
35	ECO 713	5-3-1991
36	ECO 713	5-3-1991
37	ECO 713	5-3-1991
38	ECO 713	5-3-1991
39	ECO 713	5-3-1991
40	ECO 713	5-3-1991
41	ECO 713	5-3-1991
42	ECO 713	5-3-1991
43	ECO 713	5-3-1991
44	ECO 713	5-3-1991
45	ECO 713	5-3-1991
46	ECO 713	5-3-1991
47	ECO 713	5-3-1991
48	ECO 713	5-3-1991
49	ECO 713	5-3-1991
50	ECO 713	5-3-1991
51	ECO 713	5-3-1991
52	ECO 713	5-3-1991
53	ECO 713	5-3-1991
54	ECO 713	5-3-1991
55	ECO 713	5-3-1991
56	ECO 713	5-3-1991
57	ECO 713	5-3-1991
58	ECO 713	5-3-1991
59	ECO 713	5-3-1991
60	ECO 713	5-3-1991
61	ECO 713	5-3-1991
62	ECO 713	5-3-1991
63	ECO 713	5-3-1991
64	ECO 713	5-3-1991
65	ECO 713	5-3-1991
66	ECO 713	5-3-1991
67	ECO 713	5-3-1991
68	ECO 713	5-3-1991
69	ECO 713	5-3-1991
70	ECO 713	5-3-1991
71	ECO 713	5-3-1991
72	ECO 713	5-3-1991
73	ECO 713	5-3-1991
74	ECO 713	5-3-1991
75	ECO 713	5-3-1991
76	ECO 713	5-3-1991
77	ECO 713	5-3-1991
78	ECO 713	5-3-1991
79	ECO 713	5-3-1991
80	ECO 713	5-3-1991
81	ECO 713	5-3-1991
82	ECO 713	5-3-1991
83	ECO 713	5-3-1991
84	ECO 713	5-3-1991
85	ECO 713	5-3-1991
86	ECO 713	5-3-1991
87	ECO 713	5-3-1991
88	ECO 713	5-3-1991
89	ECO 713	5-3-1991
90	ECO 713	5-3-1991
91	ECO 713	5-3-1991
92	ECO 713	5-3-1991
93	ECO 713	5-3-1991
94	ECO 713	5-3-1991
95	ECO 713	5-3-1991
96	ECO 713	5-3-1991
97	ECO 713	5-3-1991
98	ECO 713	5-3-1991
99	ECO 713	5-3-1991
100	ECO 713	5-3-1991

CPU E3
SCHEMATIC
REV D 4/21/88

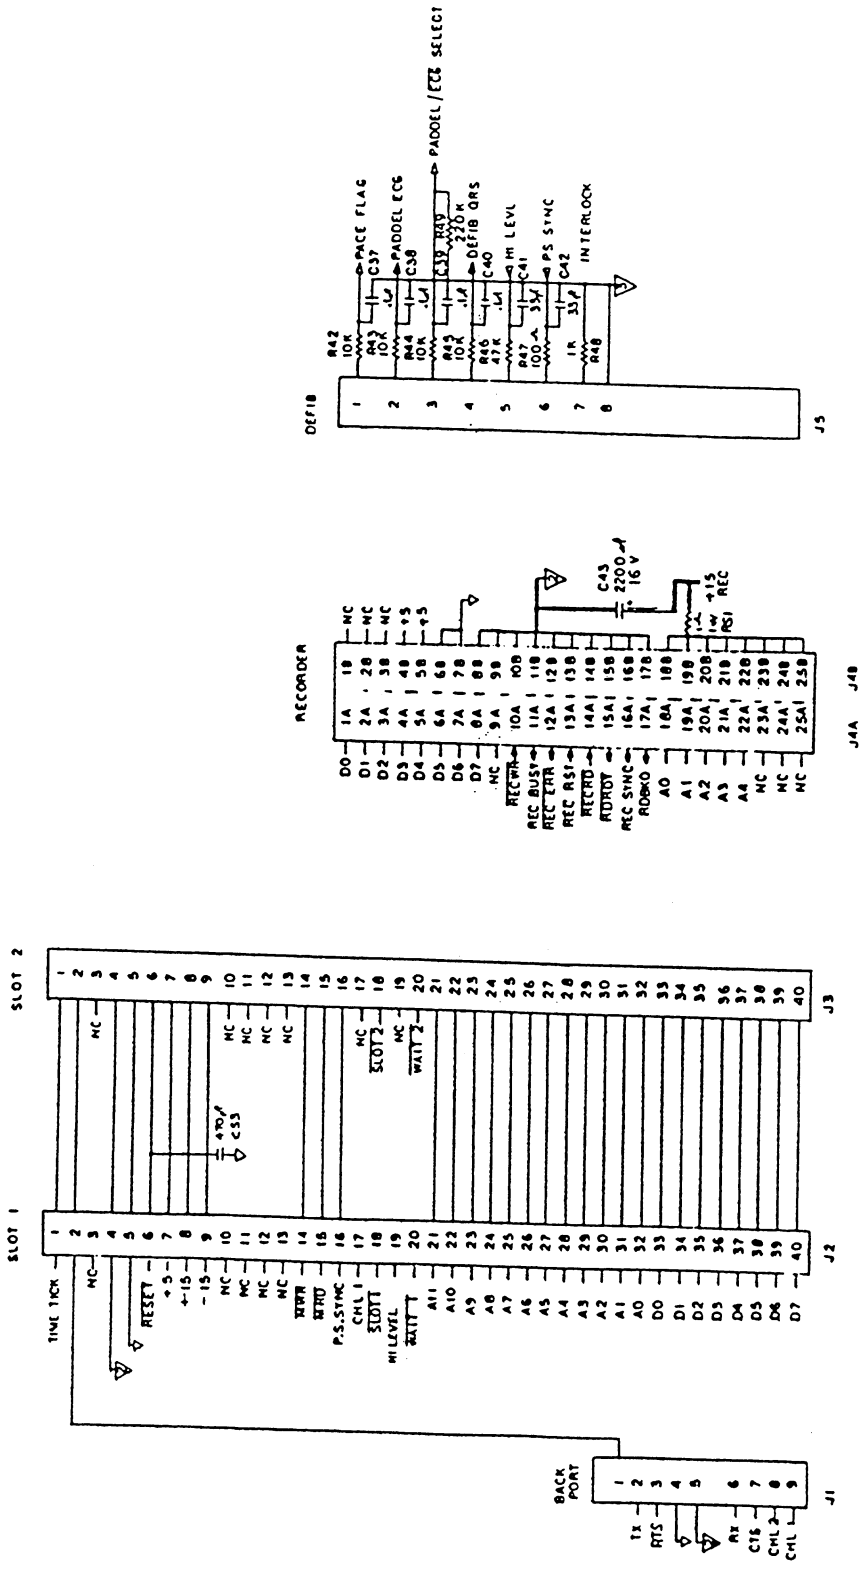

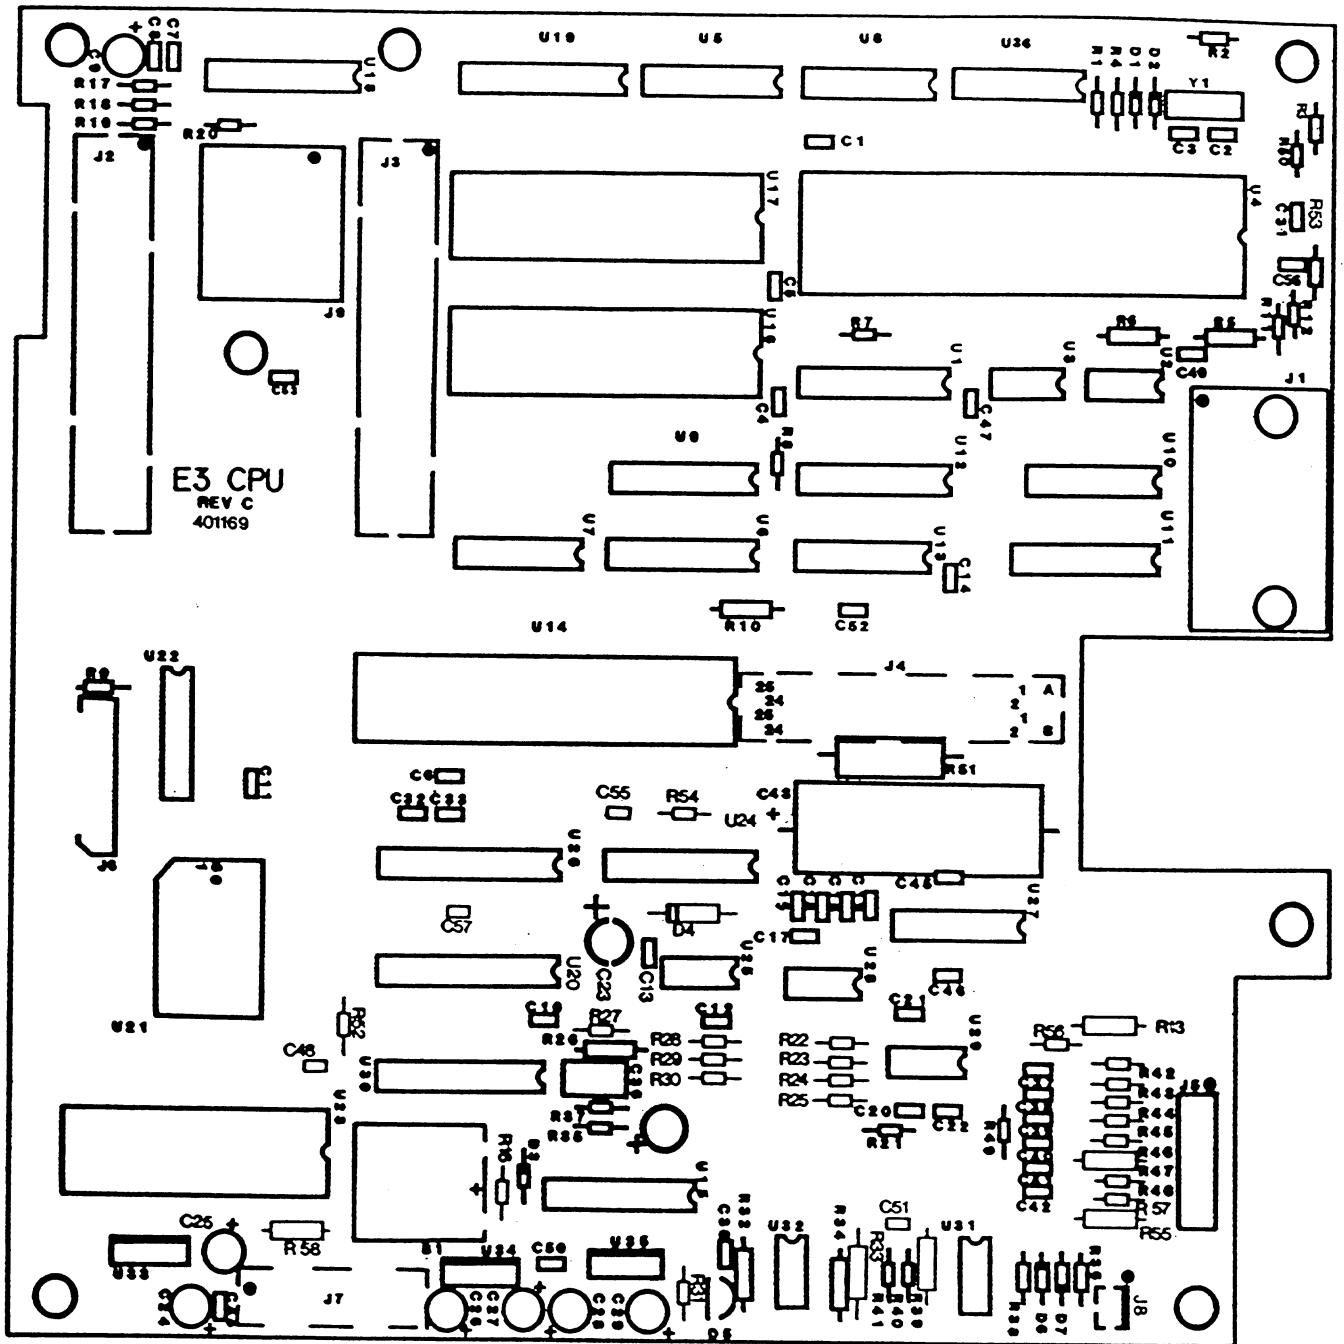

CPU BOARD

Assembly	Description	Group	PFC	Commodity	Class	Planner	Buyer	Drawing	Rev	LT
401168-0000	PCBA, E3 CPU MOTHER REV. J1 (D187)				A				J1	14

Shrinkage Factor: 0.000

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
401169-0000	*1	1	PCB, E3 CPU MOTHER BD REV D .D (E986)	R		33	1.000	EA		Yes		
352100-0104A	*1	2	CAP, .1UF,50V,10%,RAD,X7R	R		11	8.000	EA	C1,4,5,6,10,12,14,45	Yes		
352100-0104A	*1	3	CAP, .1UF,50V,10%,RAD,X7R	R		11	7.000	EA	C11,13,22,44,57,47,49	Yes		
352100-0471A	*1	4	CAP, 470PF,25V,10%,RAD,X7 R	R		22	5.000	EA	C51,55,56,53,48	Yes		
352101-0330A	*1	5	CAP, 33PF,100V,5%,RAD,NPO	R		22	2.000	EA	C41, C42	Yes		
352201-0227A	*1	6	CAP, 220UF,10V,RAD,ELECT, .248 X .433 CS	R		66	3.000	EA	C24,25,54	Yes		
352202-0228A	*1	7	CAP, 2200uF,16V,AX,ELECT, 12x30mm	R		22	1.000	EA	C43	Yes		
352300-0010A	*1	8	CAP., .001UF,5%,MYLAR SOR T FROM 352300-0007A	R		66	1.000	EA	C20	Yes		
352300-0102A	*1	9	CAP, 1000PF,50V,20%,RAD,M YLAR	R		66	1.000	EA	C21	Yes		
352300-0103A	*1	10	CAP, .01UF,50V,20%,RAD,MY LAR	R		22	4.000	EA	C15, C16, C17, C18	Yes		
352300-0103A	*1	11	CAP, .01UF,50V,20%,RAD,MY LAR	R		22	2.000	EA	C19,31	Yes		
352300-0104A	*1	12	CAP, .1UF,50V,20%,RAD,MYL AR	R		22	3.000	EA	C7,8,30	Yes		
352300-0104A	*1	13	CAP, .1UF,50V,20%,RAD,MYL AR	R		22	4.000	EA	C37, C38, C39, C40	Yes		
352400-0686A	*1	14	CAP, 68UF,25V,20%,RAD,TAN T,.5 IN MAX.HT/.15LS	R		22	1.000	EA	C23	Yes		
352200-0476A	*1	15	CAP, 47UF,25V,RAD,ELECT	R		55	4.000	EA	C26, C27, C28, C29	Yes		
352400-0335A	*1	16	CAP, 3.3UF,20V,20%,RAD,TA NT	R		11	1.000	EA	C9	Yes		
354000-0102A	*1	17	CONN, SNAP,R/A,SG L.ROW,SG L.PINS	R		11	8.000	PIN	J9 - DO NOT ISSUE	Yes		
354000-0106A	*1	18	CONN, DBL ROW,STRT,SG L PI N,SNAP-AWAY	R		11	14.000	PIN	J5 - DO NOT ISSUE	Yes		
354000-0138A	*1	19	CONN, 2-P,M,STRT LOCK,.1 CTR,HDR	R		11	1.000	EA	J8	Yes		
354000-0145A	*1	20	CONN, 9-P,F,DB 9,PLASTIC, R/A	R		22	1.000	EA	J1	Yes		
354000-0146A	*1	21	CONN, 40-PIN,CARD EDGE,.1 CTR,.437-.460 HIGH	R		22	2.000	EA	J2, J3	Yes		
354000-0199A	*1	22	CONN, 50-PIN,HIGH DENSITY ,MALE	R		33	1.000	EA	J4	Yes		
354000-0200A	*1	23	CONN, 20-PIN,EDGE,DUAL 10	R		22	1.000	EA	J7	Yes		
354000-0201A	*1	24	CONN, 14-PIN,FLAT FLEX	R		44	1.000	EA	J6	Yes		

Assembly Description
401168-0000 PCBA, E3 CPU MOTHER REV. J1 (D187)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
J1 14

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
356000-0001A	*1	25	XTAL, 16MHZ,QUARTZ,MICROP ROCESSOR	R		11	1.000	EA	Y1	Yes		
364000-0002A	*1	26	IC, DAC-083X, NOTE: X = EITHER 0, 1, OR 2.	R		22	1.000	EA	U20	Yes		
364000-0173A	*1	27	IC, LF347 SCREENED FROM - 0009, -0130, -0135	A		5	1.000	EA	U27	Yes		
364000-0011A	*1	28	IC, LM358	R		11	1.000	EA	U31	Yes		
364000-0024A	*1	29	IC, 74HC00	R		11	1.000	EA	U8	Yes		
364000-0025A	*1	30	IC, 74HC04	R		11	1.000	EA	U22	Yes		
364000-0027A	*1	31	IC, 74HC32	R		11	2.000	EA	U5, U7	Yes		
364000-0028A	*1	32	IC, 74HC74	R		11	2.000	EA	U10,36	Yes		
364000-0029A	*1	33	IC, 74HC138	R		11	1.000	EA	U6	Yes		
364000-0031A	*1	34	IC, 74HC161	R		11	2.000	EA	U11, U12	Yes		
364000-0040A	*1	35	IC, 4051	R		11	1.000	EA	U24	Yes		
364000-0059A	*1	36	IC, 555, TIMER CHIP, LINE AR	R		11	1.000	EA	U29	Yes		
364000-0062A	*1	37	IC, 74C922	R		22	1.000	EA	U18	Yes		
364000-0092A	*1	38	IC, HD 64180 RP-8 (Z180-8 MHZ)	R		11	1.000	EA	U4	Yes		
364000-0100A	*1	39	IC, MC145406	R		11	1.000	EA	U1	Yes		
364000-0101A	*1	40	IC, 82C55 **MITSUBISHI ON LY**	R		22	1.000	EA	U14	Yes		
364000-0104A	*1	41	IC, 74HC139	R		11	1.000	EA	U9	Yes		
364000-0105A	*1	42	IC, TL55257 PL12 32 X 8 RAM, STATIC	R		22	1.000	EA	U23	Yes		
364000-0107A	*1	43	IC, 7812 CT	R		11	1.000	EA	U34	Yes		
364000-0108A	*1	44	IC, 7912 CT	R		11	1.000	EA	U35	Yes		
364000-0115A	*1	45	IC, L4941, 5V REG, TO-220, LOW DROP	R		11	1.000	EA	U33	Yes		
364000-0123A	*1	46	IC, RTC 72421A	R		22	1.000	EA	U19	Yes		
364000-0129A	*1	47	IC, ADC0831CCN	R		22	1.000	EA	U2	Yes		
364000-0133A	*1	48	IC, TL062ACP	R		11	2.000	EA	U25, U28	Yes		

Assembly Description
401168-0000 PCBA, E3 CPU MOTHER REV. J1 (D187)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
J1 14

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
364000-0136A	*1	49	IC, LT1013,OP AMP	R		33	1.000	EA	U32	Yes		
364000-0137A	*1	50	IC, ADC1005	R		22	1.000	EA	U26	Yes		
364000-0159A	*1	51	IC, SAA1099P	R		33	1.000	EA	U30	Yes		
364000-0139A	*1	52	IC, E-1330,SM LCD CONTROL LER	R		33	1.000	EA	U21	Yes		
364000-0140A	*1	53	IC, MAX695,SUPERVISOR	R		33	1.000	EA	U15	Yes		
364000-0141A	*1	54	IC, EPROM,27C010,1 MEG	R		33	1.000	EA	U17	Yes		
364000-0142A	*1	55	IC, 1000K RAM	R		33	1.000	EA	U16	Yes		
364000-0143A	*1	56	IC, MSM16912RS,EEPROM	R		33	1.000	EA	U3	Yes		
370100-0101A	*1	57	RES, 100,1/4W,5%,CF	R		11	4.000	EA	R10,13,26,58	Yes		
370101-0243A	*1	58	RES, 24K,1/8W,5%,CF	R		11	1.000	EA	R24	Yes		
370101-0393A	*1	59	RES, 39K,1/8W,5%,CF	R		11	1.000	EA	R23	Yes		
370101-0472A	*1	60	RES, 4.7K,1/8W,5%,CF	R		11	2.000	EA	R11,12	Yes		
370101-0752A	*1	61	RES, 7.5K,1/8W,5%,CF	R		11	1.000	EA	R31	Yes		
370101-0102A	*1	62	RES, 1K,1/8W,5%,CF	R		11	2.000	EA	R27,28	Yes		
370101-0102A	*1	63	RES, 1K,1/8W,5%,CF	R		11	5.000	EA	R40,48,52,53,54	Yes		
370101-0103A	*1	64	RES, 10K,1/8W,5%,CF	R		11	4.000	EA	R1,3,7,37	Yes		
370101-0103A	*1	65	RES, 10K,1/8W,5%,CF	R		11	6.000	EA	R22,25,30,35,36,38	Yes		
370101-0103A	*1	66	RES, 10K,1/8W,5%,CF	R		11	4.000	EA	R42, R43, R44, R45	Yes		
370101-0104A	*1	67	RES, 100K,1/8W,5%,CF	R		11	2.000	EA	R17,18	Yes		
370101-0104A	*1	68	RES, 100K,1/8W,5%,CF	R		11	2.000	EA	R19,20	Yes		
370101-0113A	*1	69	RES, 11K,1/8W,5%,CF	R		11	1.000	EA	R41	Yes		
370101-0203A	*1	70	RES, 20K,1/8W,5%,CF	R		11	2.000	EA	R2,29	Yes		
370101-0224A	*1	71	RES, 220K,1/8W,5%,CF	R		11	2.000	EA	R49,50	Yes		
370101-0332A	*1	72	RES, 3.3K,1/8W,5%,CF	R		22	2.000	EA	R4, R16	Yes		

Assembly Description
401168-0000 PCBA, E3 CPU MOTHER REV. J1 (0187)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
J1 14

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
370202-2492A	*1	73	RES, 24.9K,1/8W,1%	R		11	1.000	EA	R21	Yes		
									R21 = 11.0K, 1% for EL	Units		
370101-0473A	*1	74	RES, 47K,1/8W,5%,CF	R		11	2.000	EA	R46,59	Yes		
370100-0510A	*1	75	RES, 51,1/4W,5%,CF	R		11	1.000	EA	R55	Yes		
370200-3831A	*1	76	RES, 3.83K,1/4W,1%,MF	R		22	1.000	EA	R6	Yes		
370200-9091A	*1	78	RES, 9.09K,1/4W,1%,MF	R		11	1.000	EA	R5	Yes		
370204-1002A	*1	79	RES, 10K,1/4W,0.1%,MF	R		22	1.000	EA	R32	Yes		
370204-4751A	*1	80	RES, 4.75K,1/4W,0.1%,MF	R		22	1.000	EA	R33	Yes		
370204-9531A	*1	81	RES, 9.53K,1/4W,0.1%,MF	R		66	1.000	EA	R34	Yes		
378000-0001A	*1	82	DIO, 1N270 T&R	R		11	1.000	EA	D4	Yes		
378000-0005A	*1	83	DIO, 1N914,SIGNAL T&R	R		11	5.000	EA	D1,2,3,6,7	Yes		
378000-0043A	*1	84	DIO, LT1029ACZ,5V,PRES	R		22	1.000	EA	D5	Yes		
384000-0036A	*1	85	BATT, 2.4V (1 PIN NEG; 2 PINS POS.)	R		11	1.000	EA	B1	Yes		
352100-0150A	*1	86	CAP, 15PF,50V,10%,RAD,NPO EDPT	R		22	2.000	EA	C2, C3	Yes		
352100-0101A	*1	87	CAP, 100PF,25V,10%,RAD,NP O - .1 LEAD SPACING	R		11	1.000	EA	C52	Yes		
352301-0105A	*1	88	CAP, 1UF,63V,20%,MYLAR	R		66	1.000	EA	C36	Yes		
364000-0169A	*1	89	IC, 74HC14	R		22	1.000	EA	U13	Yes		
370101-0512A	*1	90	RES, 5.1K,1/8W,5%,CF	R		11	1.000	EA	R8	Yes		
370101-0304A	*1	91	RES, 300K,1/8W,5%,CF	R		11	1.000	EA	R9	Yes		
370201-0010A	*1	92	RES, 1,1W,M.O.	R		11	1.000	EA	R51	Yes		
370100-0474A	*1	93	RES, 470K,1/4W,5%,CF	R		11	1.000	EA	R39	Yes		
352100-0104A	*1	94	CAP, .1UF,50V,10%,RAD,X7R	R		11	4.000	EA	C32,33,50,46	Yes		
370101-0204A	*1	95	RES, 200K,1/8W,5%,CF	R		11	2.000	EA	R56,57	Yes		
100000	*1	98	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	CUT TRACE & ADD	Yes		
100000	*1	99	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	JUMPER ON CKT SIDE	Yes		


Assembly Description
401168-0000 PCBA, E3 CPU MOTHER REV. J1 (D187)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
J1 14

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
100000	*1	100	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	AS PER MARKED UP DRW.	Yes		
365000-0064A	*1	101	SKT, 64-PIN, .07 LEADS	R		11	1.000	EA	U4	Yes		
365000-0032A	*1	102	SKT, 32-PIN LOW PROFILE	R		22	1.000	EA	U17	Yes		
365000-0040A	*1	103	SKT, 40-POS, DIP, TIN PLATE , L.P.	R		11	1.000	EA	U14	Yes		
100000	*1	104	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	FOR ASSEMBLY	Yes		
100000	*1	105	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	FOR RESISTORS CHECK	Yes		
100000	*1	106	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	BIN - FILL IF REQUIRE	Yes		
370101-0242A	*1	107	RES, 2.4K, 1/8W, 5%, CF	R		11	1.000	EA	R47	Yes		
900000	*1	120	ASSEMBLY LABOR & BURDEN	L		0	1.555	HR		Yes		


Cumulative Lead Time for 401168-0000 = 80

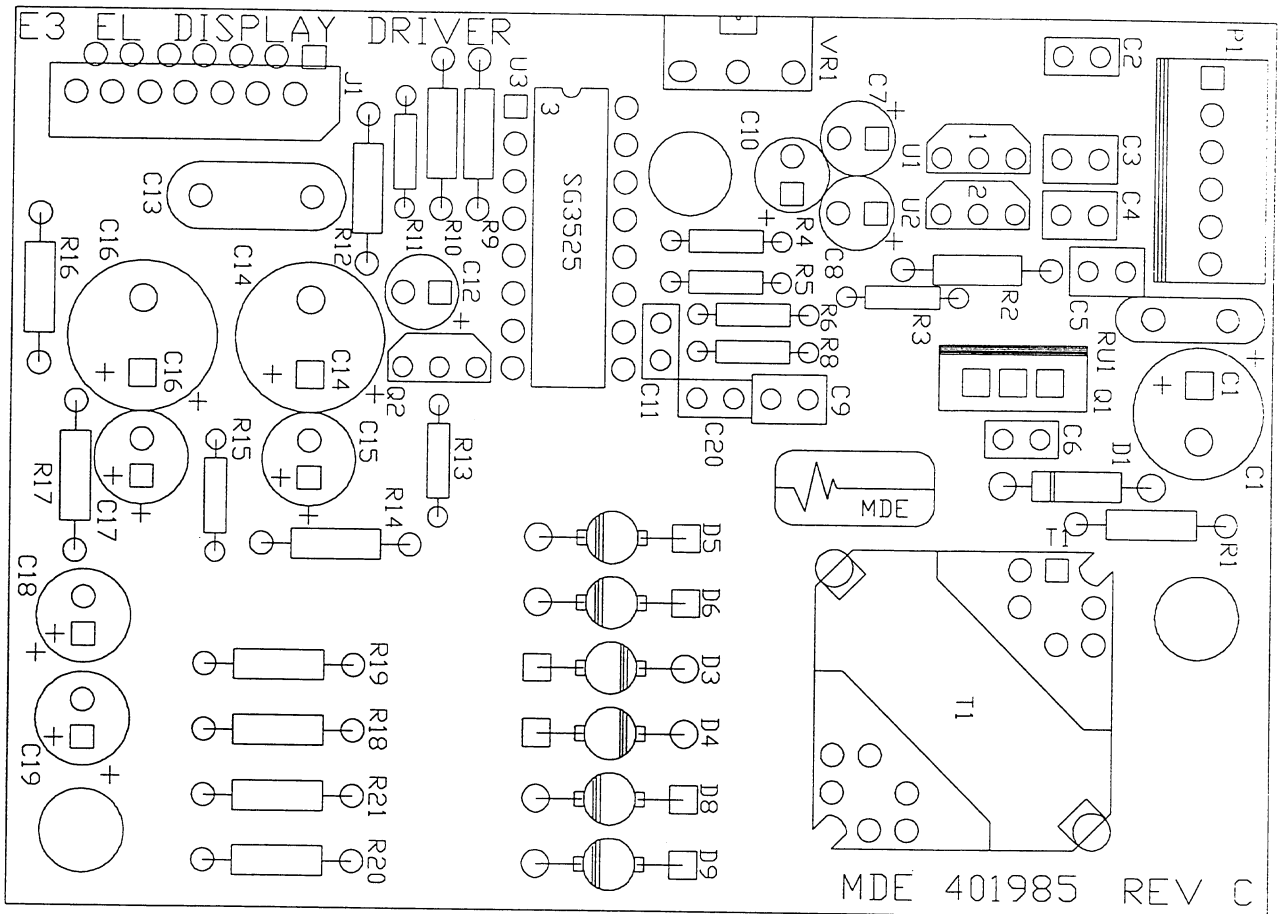

EL Display Driver - Board Layout


REVISIONS

REV	DESCRIPTION	DATE/AUTH	FOR UPDATE
A	RELEASED FOR A JURY	1-1-88 JCP	
B	ECO #11860	4-12-88 JCP	
C	ECO #11868	4-22-88 JCP	
D	ECO #11867	5-18-88 JCP	
E	ECO #11867	5-18-88 JCP	
F	ECO #11867	5-18-88 JCP	
G	ECO #11867	5-18-88 JCP	
H	ECO #11867	5-18-88 JCP	
I	ECO #11867	5-18-88 JCP	
J	ECO #11867	5-18-88 JCP	
K	ECO #11867	5-18-88 JCP	
L	ECO #11867	5-18-88 JCP	
M	ECO #11867	5-18-88 JCP	
N	ECO #11867	5-18-88 JCP	
O	ECO #11867	5-18-88 JCP	
P	ECO #11867	5-18-88 JCP	
Q	ECO #11867	5-18-88 JCP	
R	ECO #11867	5-18-88 JCP	
S	ECO #11867	5-18-88 JCP	
T	ECO #11867	5-18-88 JCP	
U	ECO #11867	5-18-88 JCP	
V	ECO #11867	5-18-88 JCP	
W	ECO #11867	5-18-88 JCP	
X	ECO #11867	5-18-88 JCP	
Y	ECO #11867	5-18-88 JCP	
Z	ECO #11867	5-18-88 JCP	

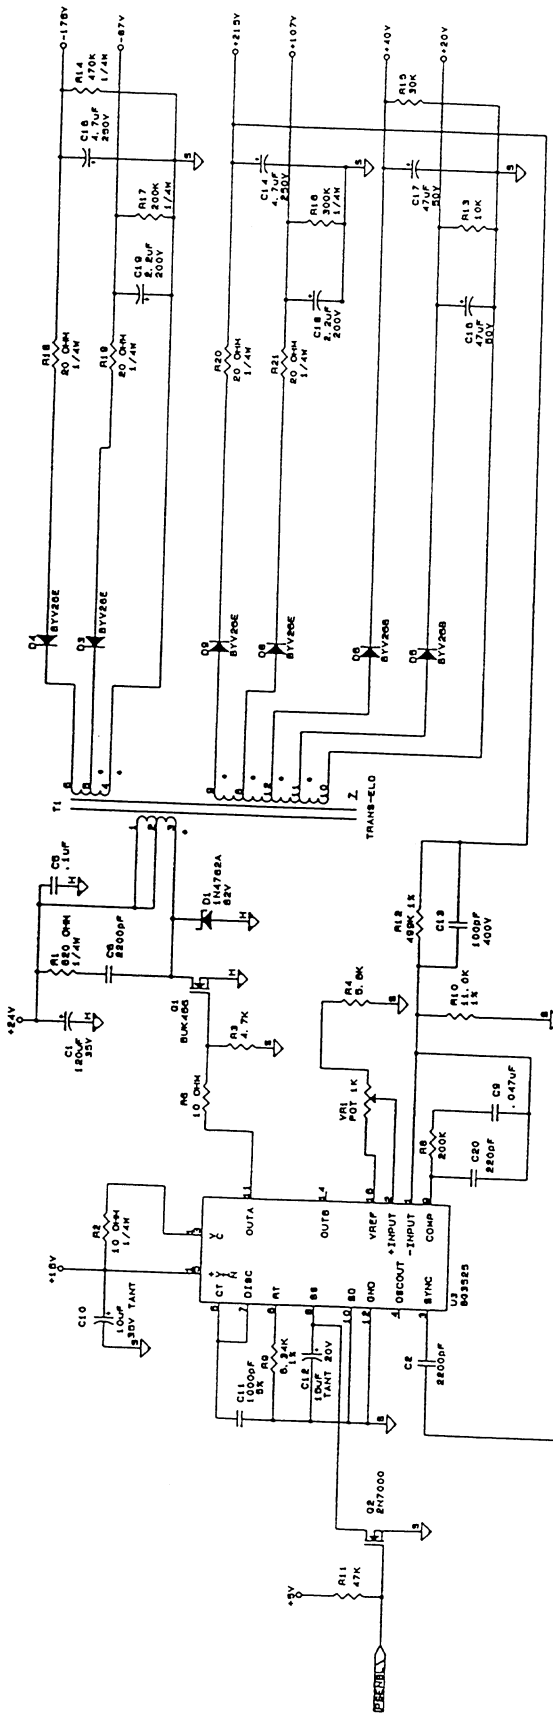

FROM E3
POWER SUPPLY

TO EL INTERFACE BD.



LAST USED

C10 RUI U3 R21
D14 Q2 J2

UNUSED LABELS

R7 L1 Q2 D7 D10-D14

REV. C. PCB

TOLERANCES UNLESS
OTHERWISE SPECIFIED
RESISTORS 1% 1/4W
CAPACITORS 20%

APPROVALS	DATE
DRANN CDP	11-17-82
CHECKED SPH	
APPROVED SPH	7-3-89
E3ELDR1 SCH	

TITLE

E3 EL DISPLAY
DRIVER SCHEMATIC

SCALE	SIZE	ORIGIN NO.	REV
FULL	C	401986	D1
NO NOT SCALE DRAWING			

SHEET 1 OF 2

=====		
401986-0000	PCBA,E3 ELECTROLUMIN DISPLAY DRIVER	
=====		
352102-0101A	CAP, 100PF, 20%, 400VAC, 2500V CS CER DISC, INT'L APPR.	1 C13
352200-0127A	CAP, 120uF, 35V, 20%, LOW ESR, .15/.35, ELECT	1 C1
352200-0225A	CAP, 2.2uF, 20%, 200V, RAD, 6.3 x 11mm, ELECT	2 C18, 19
352200-0475A	CAP, 4.7uF, 20%, 250V, RAD, 10 x 12mm, ELECT	2 C14, 16
352200-0476A	CAP, 47uF, 25V, RAD, ELECT 2.5mm LEAD SPACE	2 C7, 8
352202-0476A	CAP, 47uF, 20%, 50V, RAD, 6.3 x 11mm, ELECT	2 C15, 17
352300-0010A	CAP., 1000pF, 5%, MYLAR SORT FROM 352300-0007A	1 C11
352300-0104A	CAP, .1uF, 50V, 20%, RAD, MYLAR	3 C3, 4, 5
352300-0221A	CAP, 220PF, 50V, 20%, RAD, MYLAR, .1 L.S.	1 C20
352300-0473A	CAP, .047uF, 50V, 20%, MYLAR	1 C9
352301-0222A	CAP, 2200PF, 50V, 20%, MYLAR	2 C2, 6
352400-0156A	CAP, 15uF, 20V, 20%, RAD, TANT.1 IN L.S.	1 C12
352401-0106A	CAP, 10uF, 35V, 20%, RAD, TANT TAPE & REEL	1 C10
354000-0201A	CONN, 14-POS, STRT, FFC, .049 CTR	1 J1
354000-0211A	CONN, 6-PIN, M, STRT, 0.1- CTR	1 P1
364000-0091A	IC, SG 3525	1 U3
364000-0109A	IC, 78L05 +5V REG. TO-92 PKG.	1 U1
364000-0207A	IC, LM78L12ACZ, + 12V REG TO92	1 U2
370100-0100A	RES, 10, 1/4W, 5%, CF TAPE & REEL	1 R2
370100-0200A	RES, 20, 1/4W, 5%, CF TAPE & REEL	4 R18, 19, 20, 21
370100-0204A	RES, 200K, 1/4W, 5%, CF TAPE & REEL	1 R17
370100-0304A	RES, 300K, 1/4W, 5%, CF TAPE & REEL	1 R16
370100-0474A	RES, 470K, 1/4W, 5%, CF TAPE & REEL	1 R14
370100-0821A	RES, 820, 1/4W, 5%, CF TAPE & REEL	1 R1
370101-0100A	RES, 10, 1/8W, 5%, CF TAPE & REEL	1 R6
370101-0103A	RES, 10K, 1/8W, 5%, CF TAPE & REEL	1 R13
370101-0204A	RES, 200K, 1/8W, 5%, CF TAPE & REEL	1 R8
370101-0303A	RES, 30K, 1/8W, 5%, CF TAPE & REEL	1 R15
370101-0472A	RES, 4.7K, 1/8W, 5%, CF TAPE & REEL	1 R3
370101-0473A	RES, 47K, 1/8W, 5%, CF TAPE & REEL	1 R11
370101-0561A	RES, 560, 1/8W, 5%, CF TAPE & REEL	1 R5
370101-0562A	RES, 5.6K, 1/8W, 5%, CF TAPE & REEL	1 R4
370200-1102A	RES, 11K, 1/4W, 1%, MF TAPE & REEL	1 R10
370200-4993A	RES, 499K, 1/4W, 1%, MF TAPE & REEL	1 R12
370200-6341A	RES, 6.34K, 1/4W, 1%, MF TAPE & REEL	1 R9
374300-0102A	POT, 1K, TRIM, SIDE ADJ, CERMET, 3/8 IN. QR, .15LS	1 VR1
376000-0017A	XSTR, BUK456-100A, (OR IRF 540) (TO-220) MOSFET ONLY	1 Q1
376000-0019A	XSTR, 2N7000, FET	1 Q2
378000-0060A	DIO, BYV26B RECT. TAPE & REEL	2 D5, 6
378000-0061A	DIO, 1N4762A, 82V, 1W, ZENER TAPE & REEL	1 D1
378000-0069A	DIO, BYV26E, 1000V, ULTRA FAST TAPE & REEL	4 D3, 4, 8, 9
380000-0037A	SW, RUE090, POLY, RESETTABLE FUSE PTC DEV	1 RU1
401985-0000	PCB, E3 ELECTROLUMINESCENT DISPLAY DRVR REV C(E1467	1 -
402194-0000	XFMR, SWITCHING E3/E3B EL DRIVER REV B2 (D551)	1 T1

ECG BOARD

CHAPTER 4

4.0.0 ECG BOARD

4.1.0 OVERVIEW

One of the two processor boards in the **ESCORT 300A** is the ECG Board. The primary function of this board is to detect an ECG signal and reproduce it on the monitor screen. If the **ESCORT 300A** is configured for Respiration, then the ECG Board will detect and reproduce a respiration waveform. Both waveforms are received in analog, and converted to a digital format to be stored in RAM on the CPU Board. If the **ESCORT 300A** is equipped with five lead select, the ECG Daughter Board will interpret and implement the selection.

The ECG Board also provides electrical isolation for the patient from the monitor. All signals are isolated through opto-couplers creating a barrier, separating line voltages from the patient. Necessary operating voltage for the isolated section are provided by T1 and U8 completing the isolation barrier.

Circuits will be described in 2 major sections: The **ISOLATED SECTION** including Lead Select, Instrumentation amp and Notch filter, Pacer detect, ECG MUX, A to D Sampling, Iso DC Power Supply, and the Respiration circuit if included in configuration. In the **NON ISOLATED** section are the Digital portion and Defib Buffer.

4.2.0 ISOLATED SECTION

4.2.1 LEAD SELECT

For **ESCORT 300A**'s equipped with Lead Select and/or Respiration, an ECG Daughter Board is installed. ECG from patient leads is input to and selected on the Daughter Board. Each lead has its own defibrillator protection circuitry comprised of a current limiting resistor and two back-to-back zener diodes (for RA: R17 and D1, D2). In addition, each lead has its own electro-surgical filtering circuits consisting of a 63 mH inductor and a 2200 pF capacitor in parallel with it.

The multiple gang waffer switch (S1) selects the lead configuration to produce the signals -SIG, +SIG and ISO GRD. These signals go to the main ECG Board via J1.

4.2.2 INSTRUMENTATION AMPLIFIER/NOTCH FILTER

U1 on the ECG Mother Board is a high impedance differential amplifier. The two signals are combined and amplified with a gain of 26 at U1 pin 8. R66 is adjusted to compensate for any phase difference in the two signals; R8 will balance and offset any common mode on top of the ECG signal.

The Notch filter will eliminate any respiration drive signal (125KHz) that might be present on the ECG signal.

4.2.3 PACER PULSE DETECT

If Pace key is ON, the ESCORT 300A will reject pacer artifact and insert a pacer flag into the ECG waveform. C10, C11, R12 and R13 form a bandpass filter which is used to recognize the pacer pulse. If a quick spike, +150mV, occurs, U3 pin 13 or 14 will be forced to - 15V for 2ms. This will inhibit U2 pin 7, effectively stripping the spike from the ECG signal. The U3 output also goes to opto coupler U7, generating the signal FLAG. When FLAG goes LOW for 5 - 15mS, a pacer spike has been detected.

The pacer detection circuit can be disabled by the user with the softkey PACE ON/OFF. The signal PACE ENABLE* goes through opto coupler U6 to U2 pin 9. U2 pin 11 will force U3 pins 9 and 10 to ground, disabling the pacer detect circuit.

4.2.4 ECG/RESPIRATION MULTIPLEXER

R16, R18, R19, C14, C13, C15, D11 and D12 all comprise another band pass filter that sets the monitor frequency response at .05Hz to 100Hz. The next section will multiplex the respiration signal (RESP) and the ECG signal according to the control signals RESP SEL and ECG SEL from the digital portion. Q1 is turned on and off by ECG SEL through opto coupler U5 pin 11. If respiration is selected, (RESP SEL high) Q2 is turned on, passing the respiration signal on to the A to D sampling circuit. For ESCORT 300A's not configured with respiration, ECG only will be selected.

BASELINE RST will quickly drive the ECG signal back on the screen if the amplitude of the signal becomes too large, as in the case of replacing a loose lead.

4.2.5 A TO D SAMPLING CIRCUIT

This circuit provides analog to digital conversion for use by the digital portion of the ECG Board. An oscillator and ramp waveform create a window to sample the instantaneous analog voltage and calculate a digital data point. Reference voltages are used by the integrating A to D converter to initiate timing cycles. The ramp voltage has a rise rate of 1 volt per 60us: If the ECG signal voltage has not been reached by the ramp voltage by 900 microseconds, the digital circuitry will set the SAMPLE RST to start a new cycle.

The sampling circuit starts with the signal SAMPLE RST. When SAMPLE RST goes high, it turns on Q4, shorting U4 pin 1 to -10.5V. The voltage then starts to ramp up. When it reaches -10V, U3 pin 2 will go high, starting the count and signifying the beginning of the digital conversion. U3 pin 1 and U3 pin 2 outputs are wired OR'd together. The ramp will continue up until its voltage is equal to the signal at U3 pin 7, ECG or RESP. At that time, U3 pin 1 will pull the

outputs low, stopping the counter and completing the square wave. The higher the voltage, the longer the square wave. This signal will go to opto coupler U7, and then to the digital portion of the board.

4.2.6 RESPIRATION

In addition to lead select, respiration detection is on the Daughter Board. Respiration is detected by the impedance change that occurs with the inhalation and exhalation of air by the lungs. The signal RESP DRIVE is a 125 KHz square wave that is generated by pulse width modulator U8 through T1 on the Mother Board. It gets clipped and stabilized by U8, D11, D12 and L2. U1A will amplify the square wave to approximately $\pm 7.2V$. C9 and R11 couple this signal to T1. T1 will limit this signal to less than 1mA at the outputs RA and LA.

The patient is seen by T1 as a resistance load on the secondary of the transformer. As the patient breathes, the primary drive signal changes amplitude according to how much resistance it sees across the two leads. This signal is rectified and filtered by D13, C10 and R12 to a DC level. C11 will strip off the DC component, leaving only the respiration component. This signal will change very slightly (mV), reflecting the patient's breathing pattern.

U1B has a gain of 2K to amplify this respiration component and create RESP SIGNAL. If for some reason the signal is too large to be seen on the screen, RESP RESET will shorten the RC time constant by adding R10 in parallel with R14 to drive the signal back onto the screen quickly.

4.2.7 LEAD FAIL

The LEAD FAIL detect circuit is standard in all monitors. Most of the circuitry is located on the ECG daughter board. A LEAD FAIL message will be displayed if the +SIG, the -SIG, or both leads, have been dislodged, or if the base line impedance for respiration is 4k ohms or more. In any of these instances, LEAD FAIL will be displayed on the parameter message line, but no recording will be generated. In addition, all alarms are inhibited at this time.

U2 pin 12 will detect an interruption of current flow on the -SIG, and U2 pin 3 will monitor +SIG. When the current loop, through ISO GROUND, is broken, as in the case of a lead off, the affected input will be pulled high through R23 or R24. U2c is looking for a differential of 160mV or more to signify the lead at -SIG is off. If both leads are off, D14 and D15 will drop approximately 3 volts, leaving 2 volts at the input of U3d.

U3d will detect if the lead is off at +SIG or if both leads are off. U3c will detect a lead off at -SIG, and U3a will detect if the respiration signal is higher than 4K ohms base line impedance. These signals are wired or'd together at this point. R33 and C15 form a 500ms RC time constant to filter ECG and artifact. U2b and U3b are

buffers for the signal LEAD FAIL. This signal goes to the ECG mother board through J2 pin 2.

At this point if LEAD FAIL is low, a lead fail condition exists. This signal will go through opto-coupler U7 where it becomes the signal FLAG. Software determines whether the FLAG is a pacer spike or a lead fail. If the signal remains low for 10 to 15ms, then it is considered a pacer spike. If FLAG remains low for more than 3 seconds, it is considered a lead fail.

4.2.8 ISOLATION POWER SUPPLY

Plus and minus voltages for the isolation section of the ECG Board are supplied by T1 and U8. PS SYNC drives the pulse width modulator U8 and synchronizes it with all other voltages in the monitor. T1 furnishes isolation to complete the isolation barrier. The 125 KHz RESP DRIVE signal is taken from pin 5 of T1. D7, D8, D9, and D10 rectify the AC, and a filtering circuit smoothes out the DC. ISO Ground, +V, and -V are obtained from this circuit.

4.3.0 NON ISOLATED SECTION

4.3.1 ECG DIGITAL

The processor chip on the ECG Board is a Z-80 type microprocessor. Y1 clocks U9 at 4MHz. I/O reads and writes (IORD, IOWR) and memory reads and writes (MRD, MWR) are decoded by U14 from the signals at pins 19-22. The ECG data address bus directs information to the EPROM, Dual Port RAM, CTC and address decoders. The microprocessor is reset by the CPU Board signal RSTOUT*. WAIT at pin 24 inserts wait cycles to the CPU from the Dual Port RAM. The interrupt on pin 16 will indicate to the microprocessor that 900 microseconds have elapsed since the start of the sampling cycle and request the processor to terminate this cycle. Pin 17 is the signal TIMETIC* which synchronizes the sampling cycle so that each TIMETIC* denotes getting and decoding one data point.

The EPROM (U10) stores software for the ECG Board and is enabled by U12 and the MRD signal.

The Dual Port RAM (U11) is a 2K x 8 bit CMOS RAM MS6132. It provides two ports with separate controls, address and I/O that permit separate access to memory reads and writes. The Dual Port RAM interfaces the CPU Board data address bus to the ECG Board.

U13 and U16 are input and output ports. U13 has two input signals, DEFIB SYNC and FLAG that, when requested, it places on the ECG data bus. U16 outputs control signals to the isolated section of the board.


U17 is a Counter Timer Chip. It is programmable with four

independent channels for counting and timing functions. It is enabled by IOWR, IORD and A2, and it is clocked by Y1.

At SAMPLE RST the counter will start counting at the rate of 4MHz and will continue to count for 900 microseconds if it is not stopped before by the ramp voltage equaling the sample voltage in the A to D sample circuit.

4.3.2 DEFIBRILLATOR SYNC

The defibrillator sync circuit sends a high level ECG signal to the defibrillator via the stereo jack on the connector plate. The defibrillator will detect the R wave and respond with a square wave, or RC spike flag to the ESCORT 300. This signal will turn Q5 on sending a low to the input port U13. The microprocessor will take this information and place a flag on the ECG waveform indicating the defibrillator sync position. Defibrillator sync requirements follow:

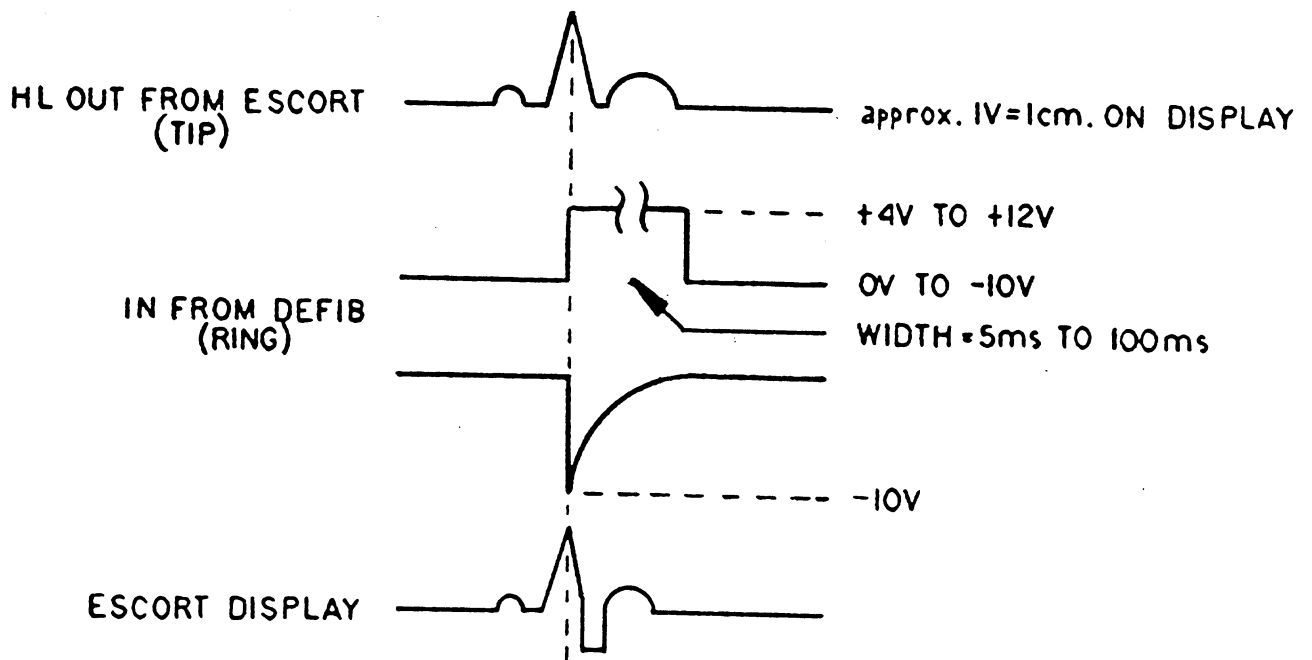

4.4.0 SOFTWARE


Software for the ECG board is stored in the EPROM, U10. Software version number can be obtained by calling up the TEST softkey page. All **ESCORT 300A's** will feature software for ECG functions. If your monitor is configured for respiration, then the EPROM will include software for respiration tasks.

Software tasks:

ECG Waveform sizing and gain control
High pass filtering
Low pass filtering
Line frequency notch filtering
R-wave picking
Baseline reset
Heart rate counting

RESPIRATION Waveform sizing and gain control
High pass filtering
Low pass filtering
Respiration waveform picking
Baseline reset
Pneumotach tach rate
CVA detection
Apnea delay


REV. 100-1	DATE	BY	APPROVED
1. INITIAL RELEASE 04/02/83			
2. ADD R18 PER DCD 126			
3. CHANGE PER DCD 179			

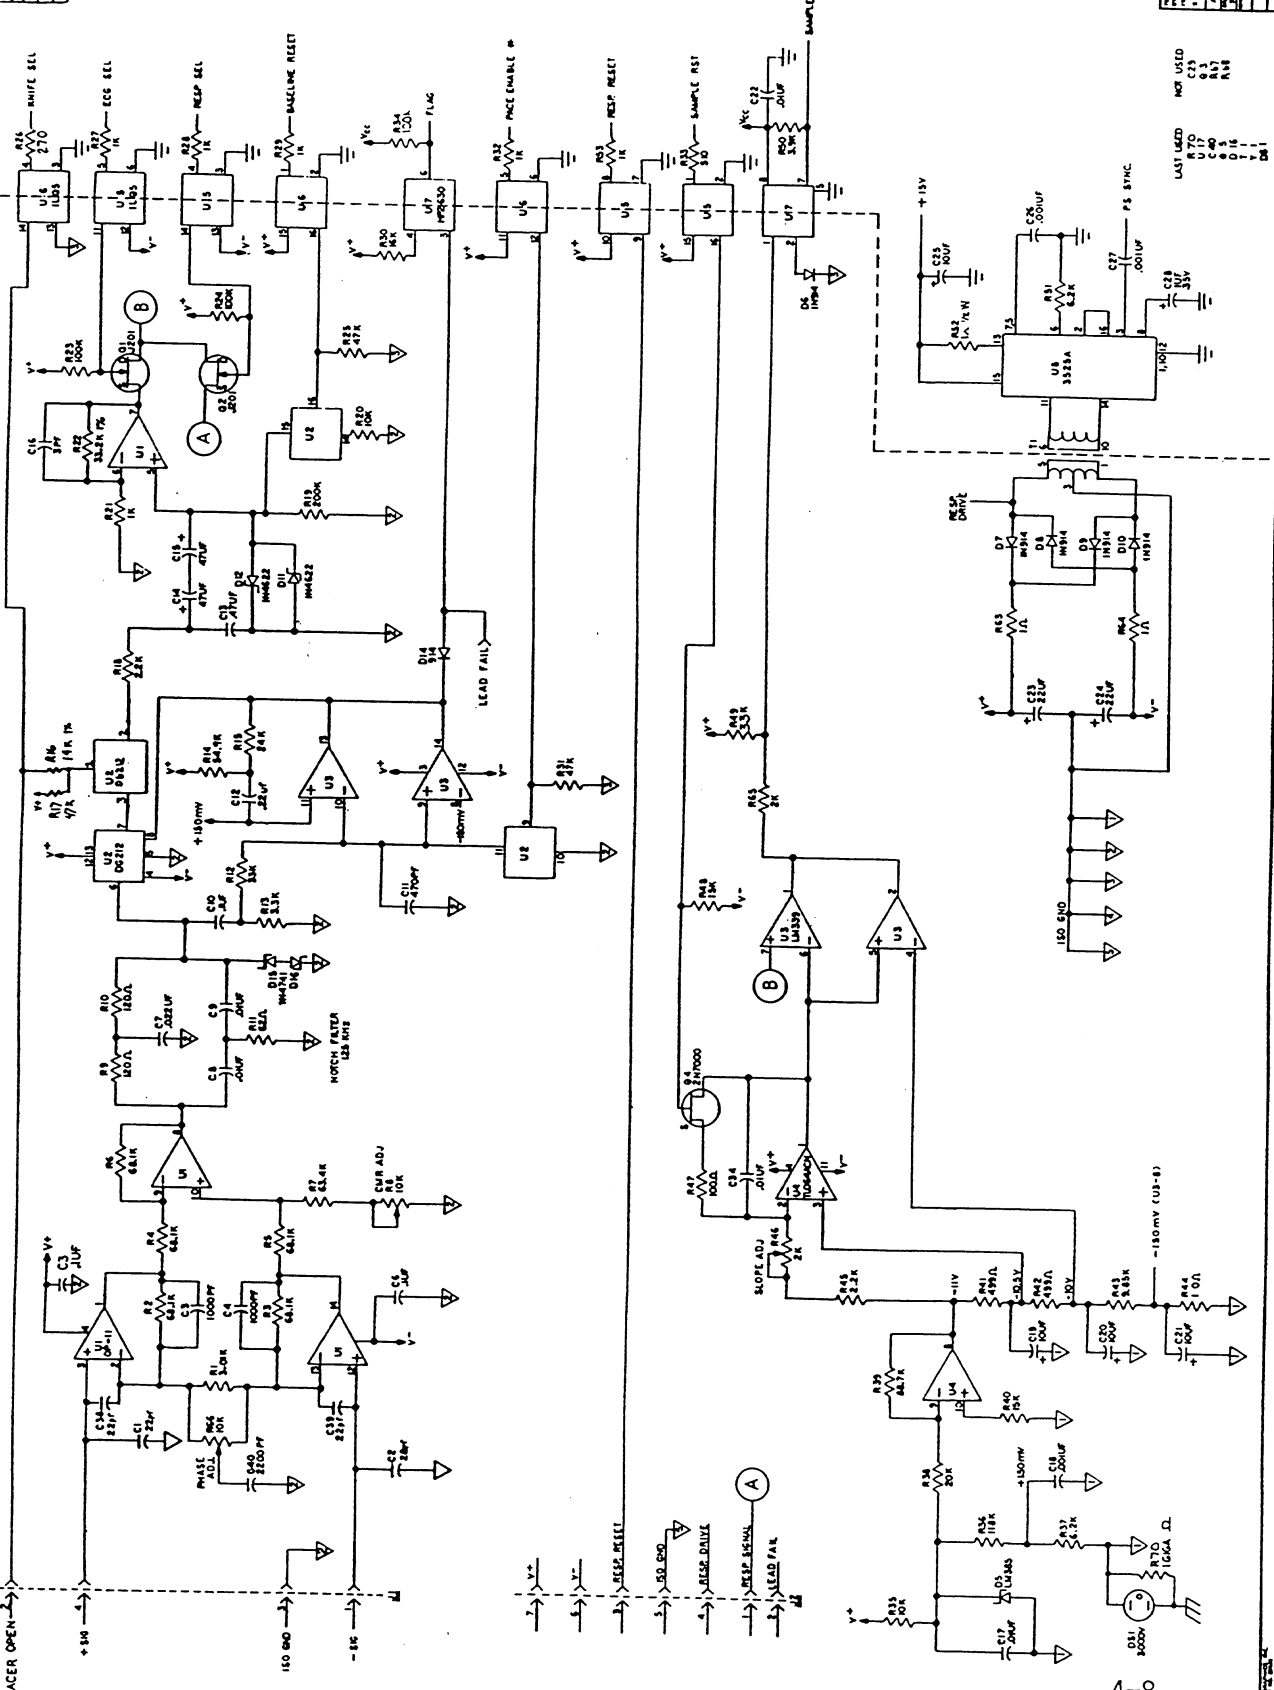


REV: B

DATE	BY	APPROVED	REVISION
04/02/83			1
04/02/83			2
04/02/83			3
04/02/83			4
04/02/83			5
04/02/83			6
04/02/83			7
04/02/83			8
04/02/83			9
04/02/83			10

NOT USED
C13
U7D
R17
R18
C40
D1
D2
D3
D4
D5
D6
D7
D8
D9
D10
D11
D12
D13
D14
D15
D16
D17
D18
D19
D20
D21
D22
D23
D24
D25
D26
D27
D28
D29
D30
D31
D32
D33
D34
D35
D36
D37
D38
D39
D40
D41
D42
D43
D44
D45
D46
D47
D48
D49
D50
D51
D52
D53
D54
D55
D56
D57
D58
D59
D60
D61
D62
D63
D64
D65
D66
D67
D68
D69
D70
D71
D72
D73
D74
D75
D76
D77
D78
D79
D80
D81
D82
D83
D84
D85
D86
D87
D88
D89
D90
D91
D92
D93
D94
D95
D96
D97
D98
D99
D100

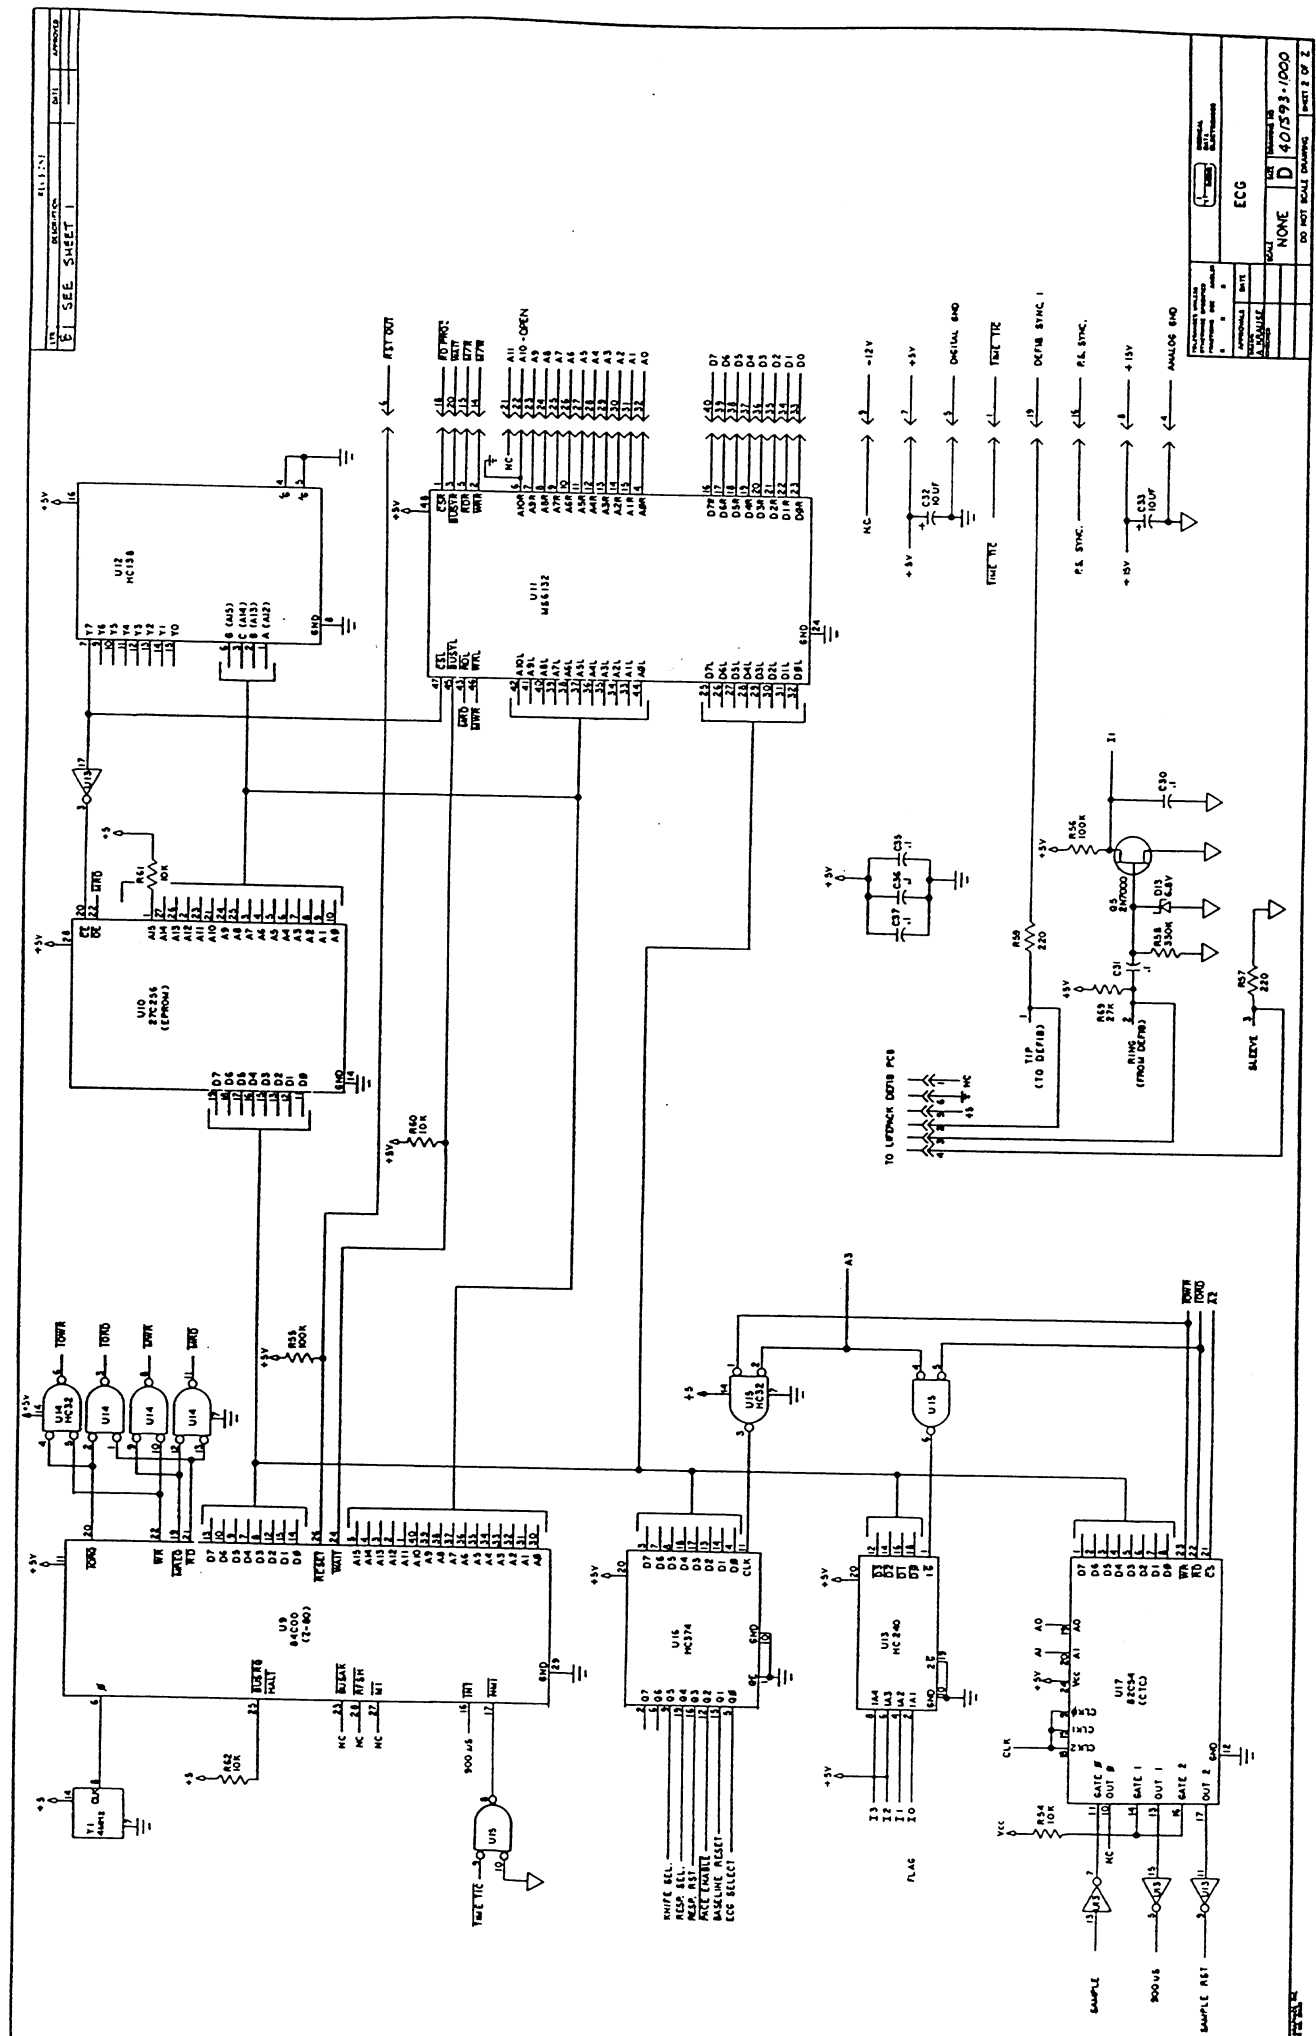

REV	DESCRIPTION	DATE	BY
1	INITIAL RELEASE (PCE 442 012)	8-11-73	
2	REV'D PER DEC. 78	10-22-78	

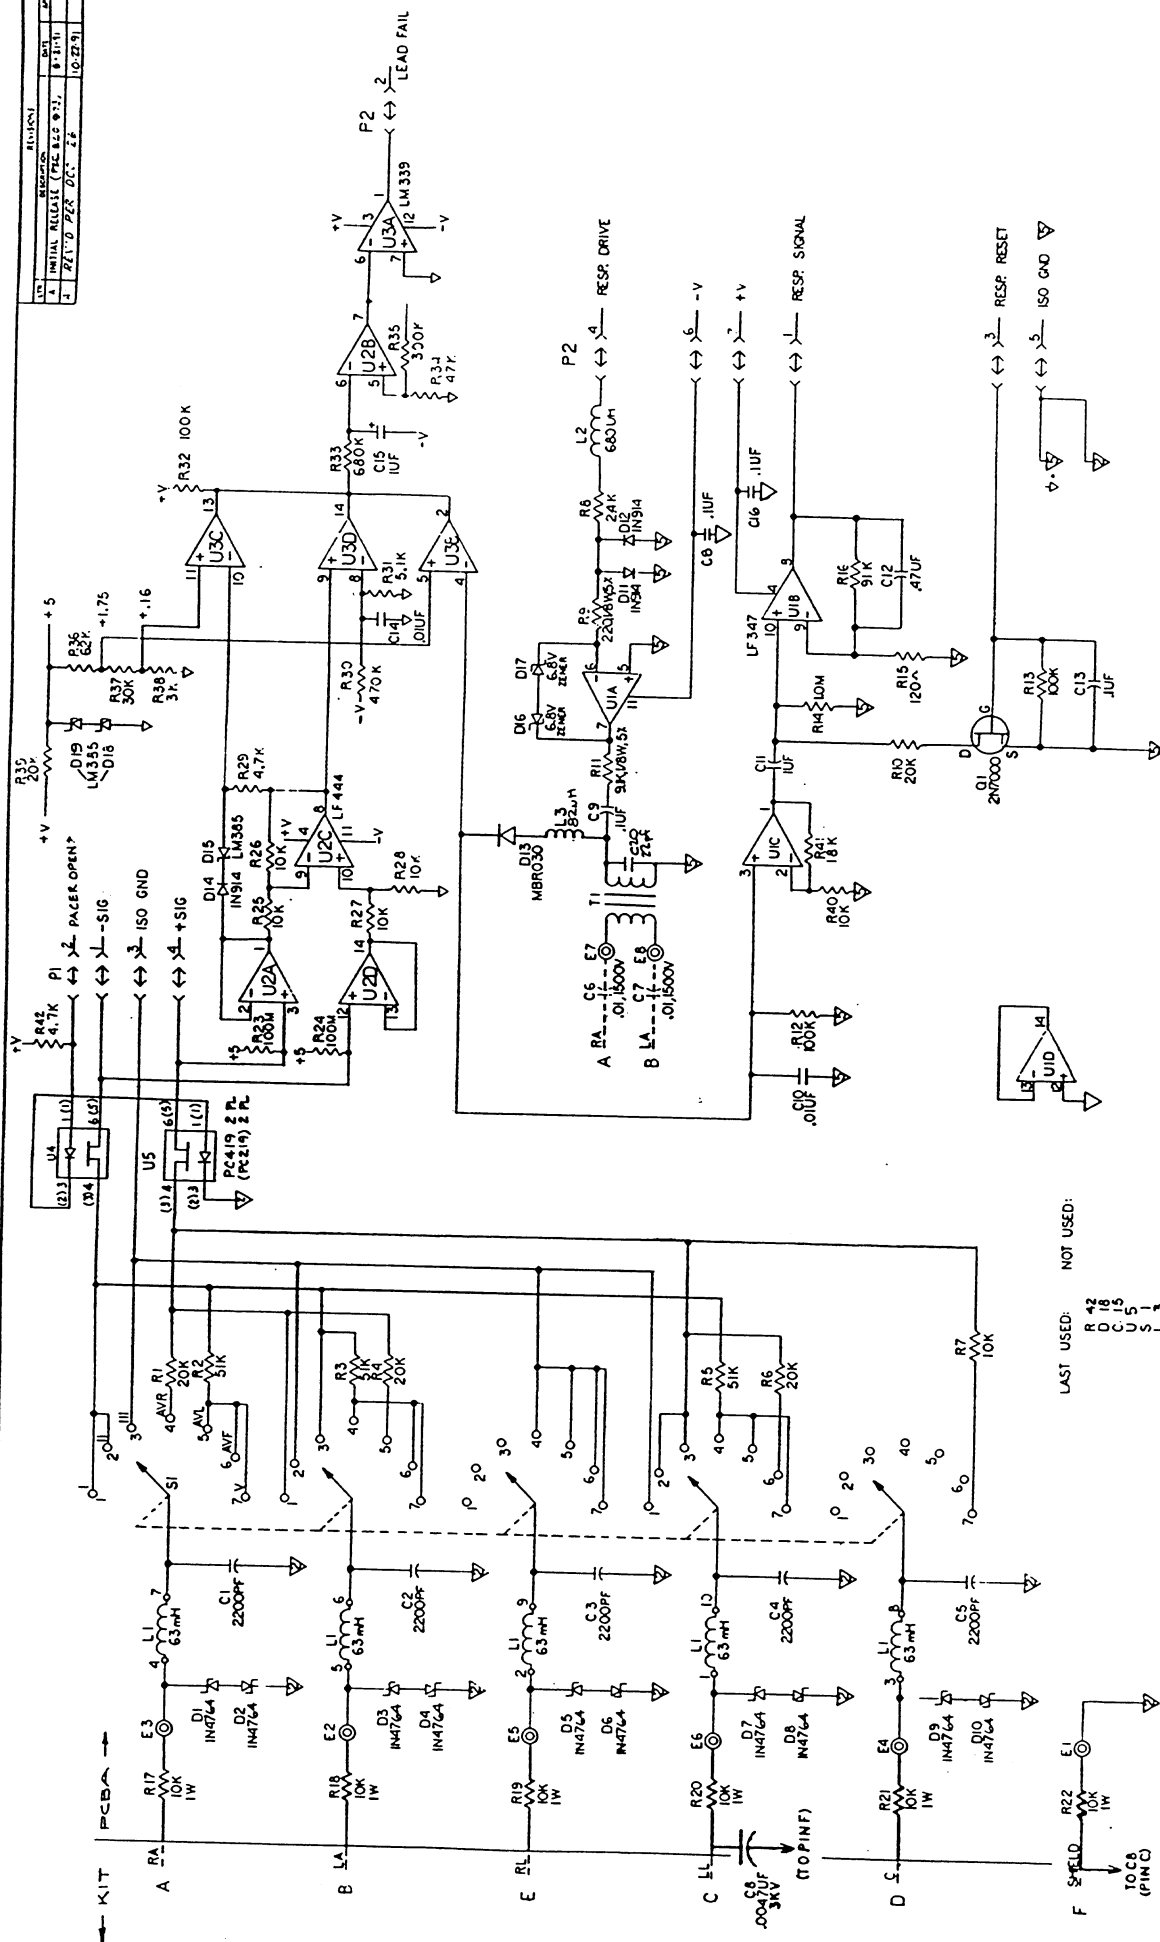

REV 1 A

NOTE: COMPONENTS DRAWN WITH DASHED LINES ARE PART OF SUBSEQUENT ASSEMBLIES AND NOT LISTED AS PART OF 401596 D.O.M.


LAST USED: NOT USED:

- R 42
- D 18
- C 15
- U 3
- Q 1

ALL RESISTORS 1/8 W UNLESS NOTED
 © FEED THROUGH SOLDER PLUG
 — () — HEADER PIN CONN. J7025

SPARES


PROJECT NAME	ECG W/RESP DAUGHTER BOARD
PROJECT NO.	401596
DATE	10-22-78
BY	
DO NOT SCALE DRAWING	1/1

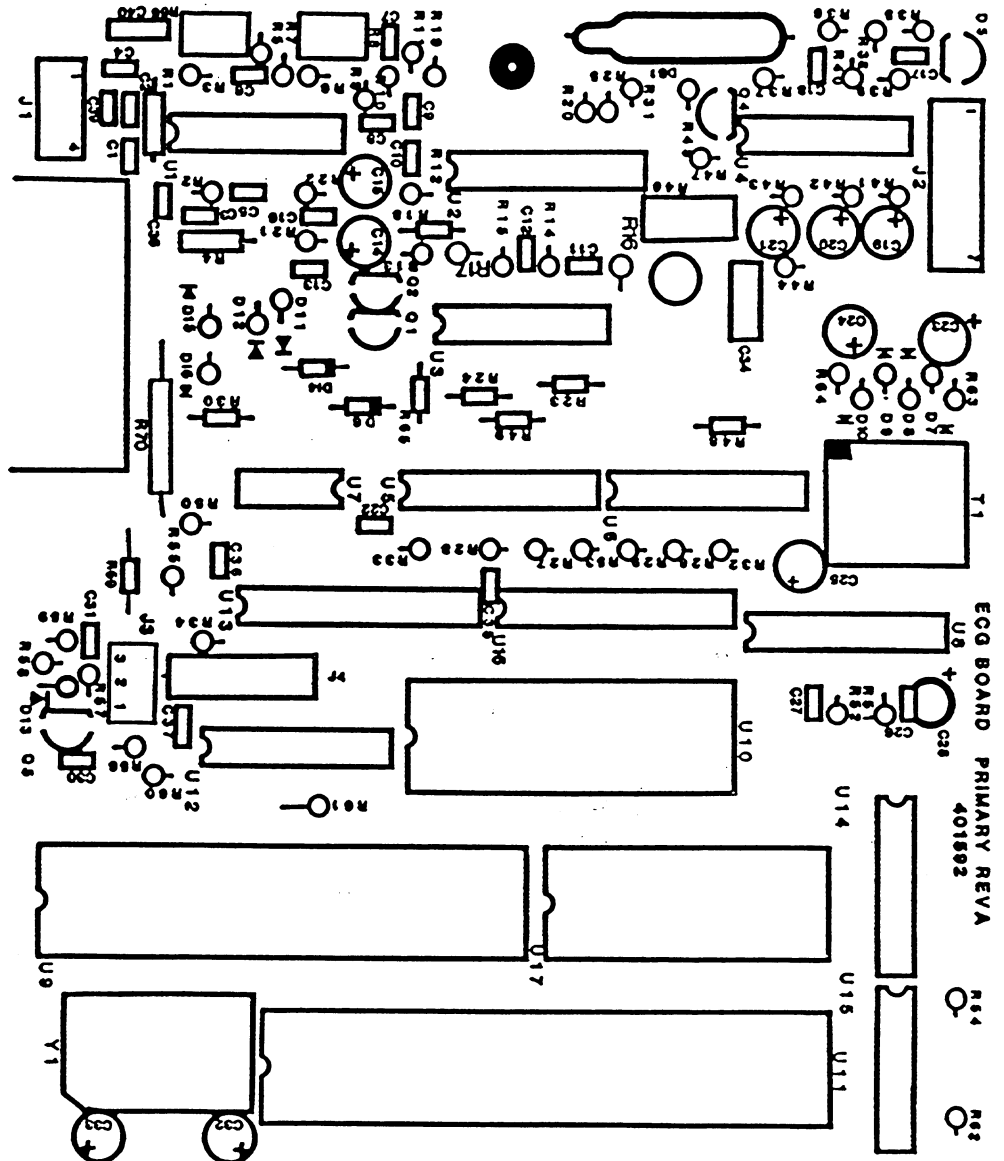

ECG BOARD



REVISIONS		
LTR	DESCRIPTION	DATE
A	INITIAL RELEASE	12.
		APPROVED

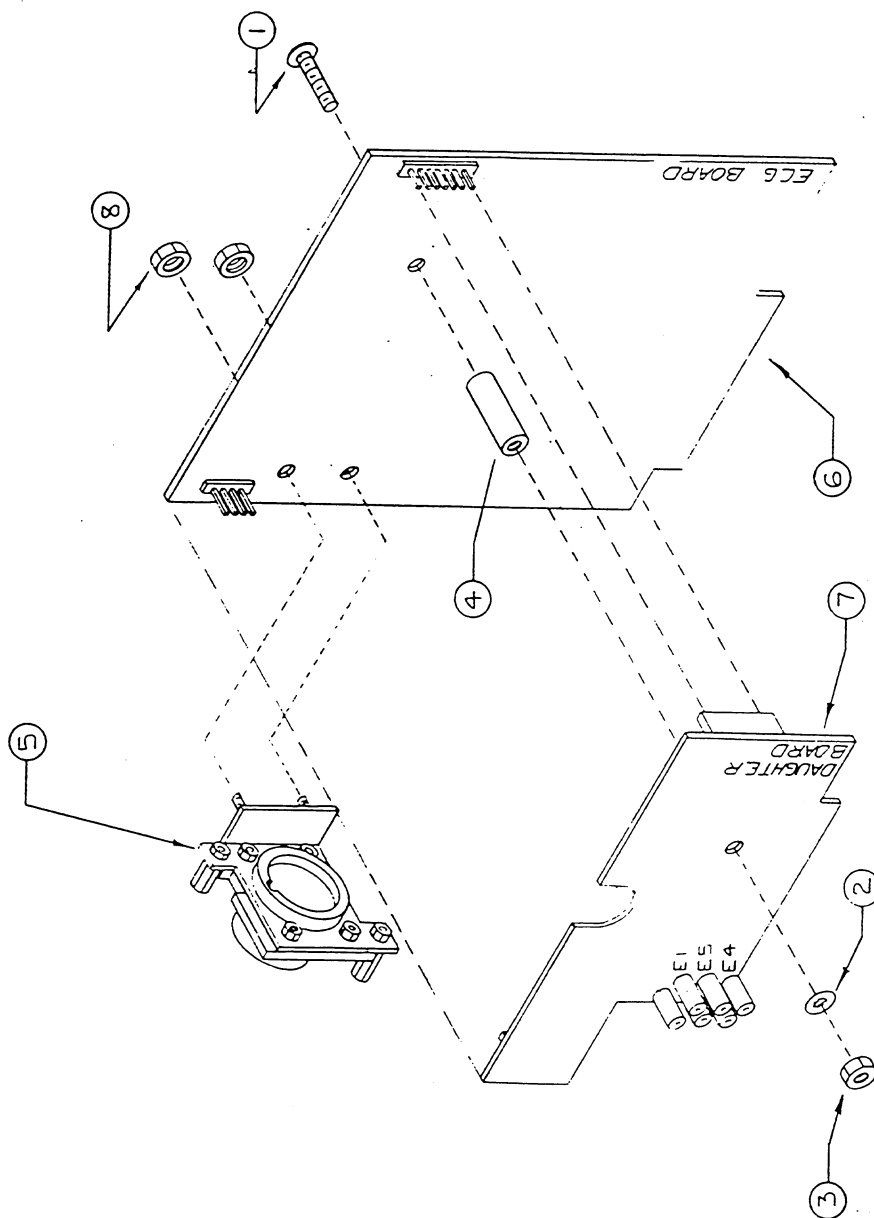

A	ORG	E3
B	RED	E7
C	BLU	E8
F	BRN	E6
E	GRN	E1
D	YEL	E5

oE3 oE1
 oE2 oE5
 oE6 oE4


NO.	QTY	DESCRIPTION	PART NO.
8	2	4-40 LOCK NUTS	360500-0037
7	1	ECG 5 LD DGTR PCBA	SEE NOTE 1
6	1	ECG MOTHER BD ASSY #2	400608-0000
5	1	ECG BRKT ASSY	400650-0000
4	1	#4 ROUND ALU SPACER	360500-0035
3	1	# HEX NUT SM. PATTERN	360500-0021
2	1	#4 STAR WASHER	358200-0007
1	1	4-40 x 3/4 PHIL1 SCREW	358100-0022

3 C6 AND C7 USED ON 400585-0000 (RESP) ONLY.
 USE DGTR BD. 400610.
 2 FOR 5 LEAD WITH RESP (400585)
 DGTR BD. ASSY. 400609.
 NOTES: 1. FOR 5 LD ONLY (400584) USE

TOLERANCES UNLESS OTHERWISE SPECIFIED		FRACTIONS DEC ANGLES	
1	1	1	1
APPROVALS	DATE	DRAWN BY	
APPROVED	2/22/87	KRAUSE	
SCALE		FULL C	
SIZE		4-00000	
DO NOT SCALE DRAWING		SHEET 1/1	

YOKE ASSEMBLY

3 LEAD

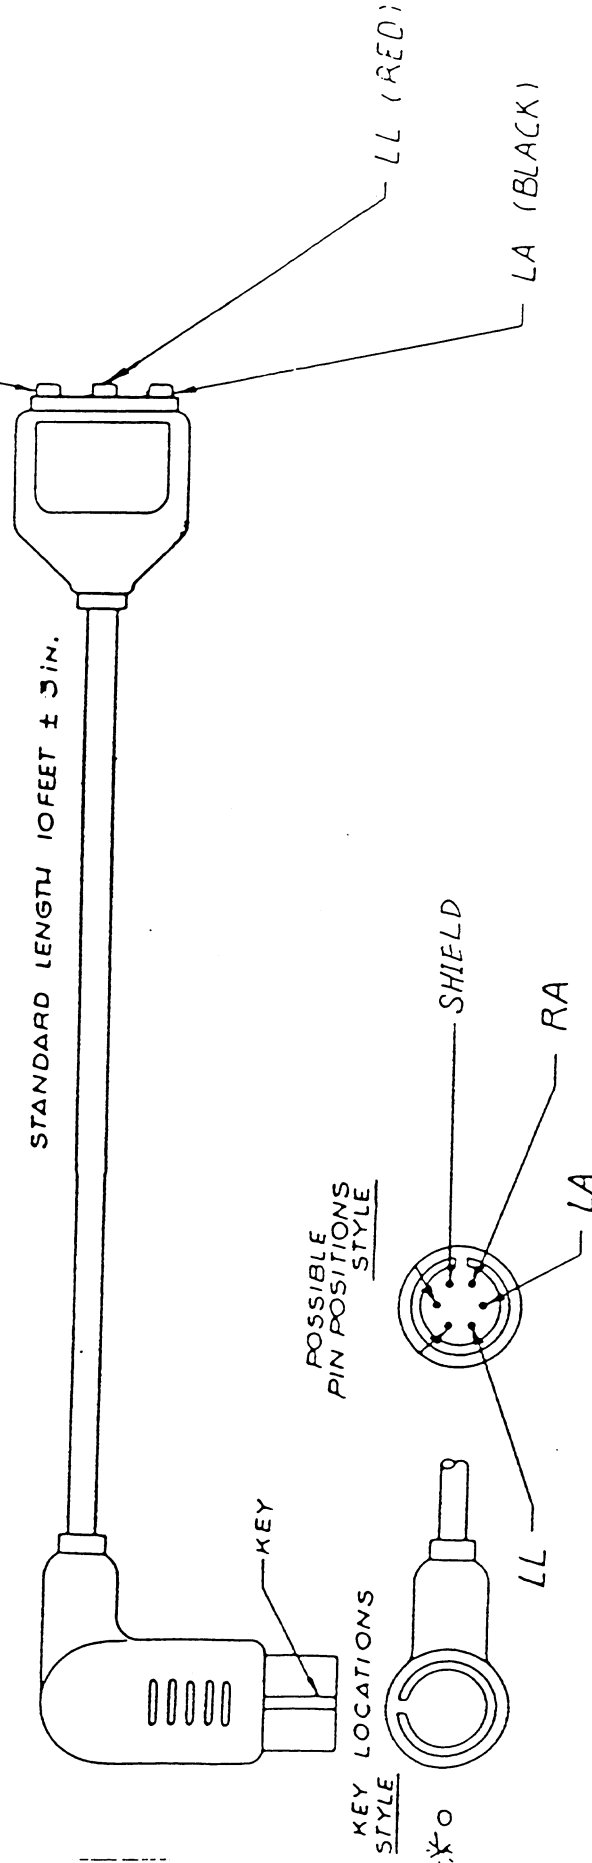


ASSEMBLY MAY BE GAS STERILIZED.
LEAD RETAINER WITH BEDSHEET CLIP
IS P/N K-2148.
UNLESS OTHERWISE NOTED, STANDARD
COLOR OF ASSEMBLY IS GRAY.

MOLD NO. T-102
SHEET 5 A
4-79-A

MOLD NO T-103-5
SHEET 2
4-79-A

YOKE ASSEMBLY

5 LEAD

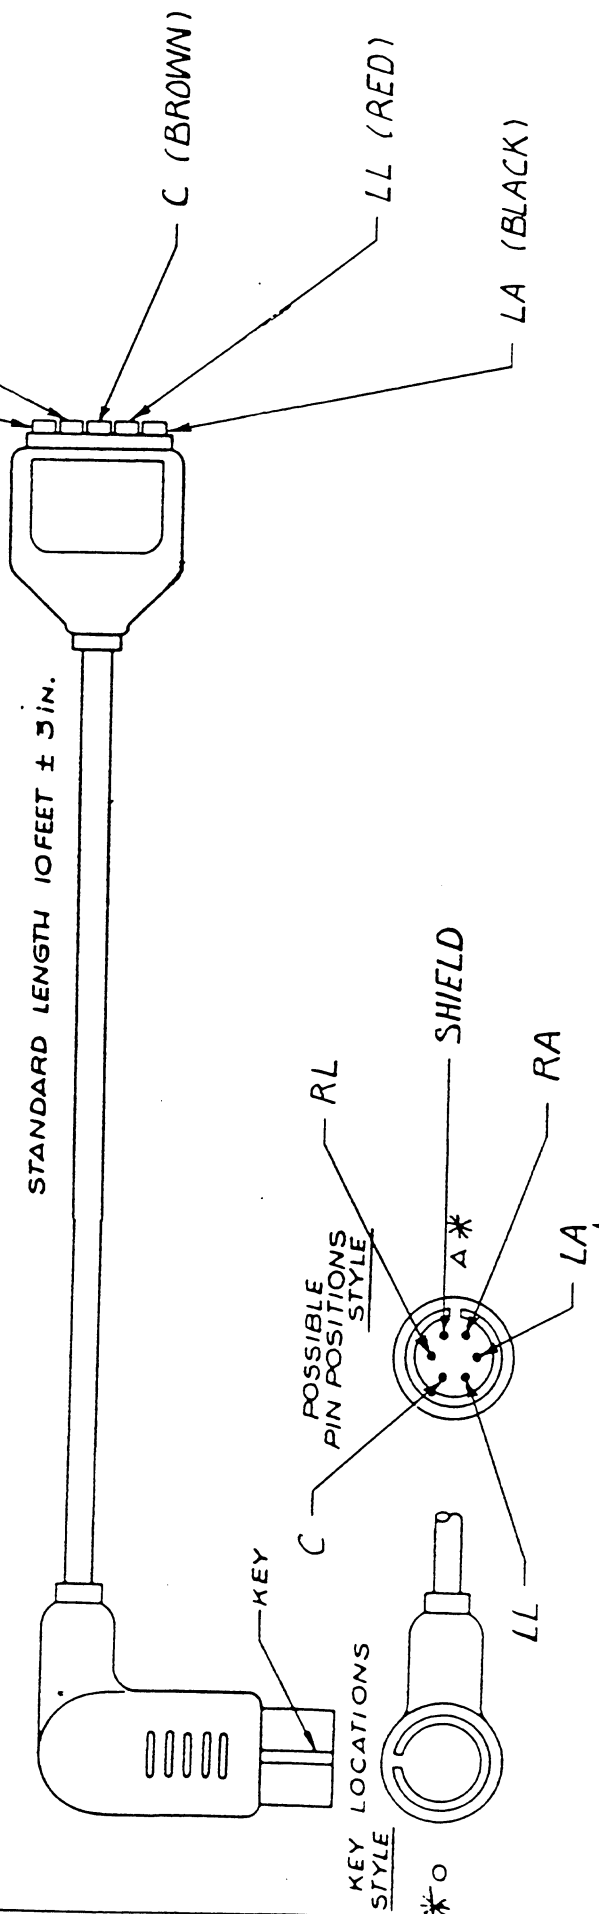

ASSEMBLY MAY BE GAS STERILIZED.
LEAD RETAINER WITH BEDSHEET CLIP
IS P/N K-2148.
UNLESS OTHERWISE NOTED, STANDARD
COLOR OF ASSEMBLY IS GRAY.

MOLD NO. T-102

SHEET 5A
4-79-A

MOLD NO. T-103-5

SHEET 2
4-79-A

REVISIONS		
LTR	DESCRIPTION	DATE
		APPROVED

RESP.CAPS	H.P.CONN.	EII DAUGHTER BD.	(REF)
	H GRN/WHT		LL
	F BROWN		C
	J BLUE		RL
X	AORANGE		RA
X	B RED		LA
	D YELLOW		SHIELD

TOLERANCES UNLESS OTHERWISE SPECIFIED		MEDICAL DATA ELECTRONICS	
FRACTIONS	DEC	ANGLES	
±	±	±	±
APPROVALS	DATE	SCALE	SIZE
<u>E. DAVIS</u>	<u>10/26/88</u>	NONE	A
CHECKED		DRAWING NO.	
DO NOT SCALE DRAWING		SHEET 1 OF 1	

REVISIONS			
LTR	DESCRIPTION	DATE	APPROVED

RESPCAPS	MERLIN H.P. CONN	EII DAUGHTER BD.	(REF)
	6 GRN/WHT		LL
	5 BROWN		C
	2 BLUE		RL
X	1 ORANGE		RA
X	7 RED		LA
	C YELLOW		SHIELD

TOLERANCES UNLESS OTHERWISE SPECIFIED		
FRACTIONS	DEC	ANGLES
±	±	±
APPROVALS	DATE	
DRAWN E. DAVIS 2/10/89		
CHECKED		



H.P. MERLIN ECG WIRING
FOR ESCORT II

SCALE NONE SIZE A DRAWING NO.

DO NOT SCALE DRAWING SHEET

REVIEWS

DESCRIPTION

DATE

APPROVED


LTR

A INITIAL RELEASE

2-10-89

B ECO 393 REDRAWN

2-22-89

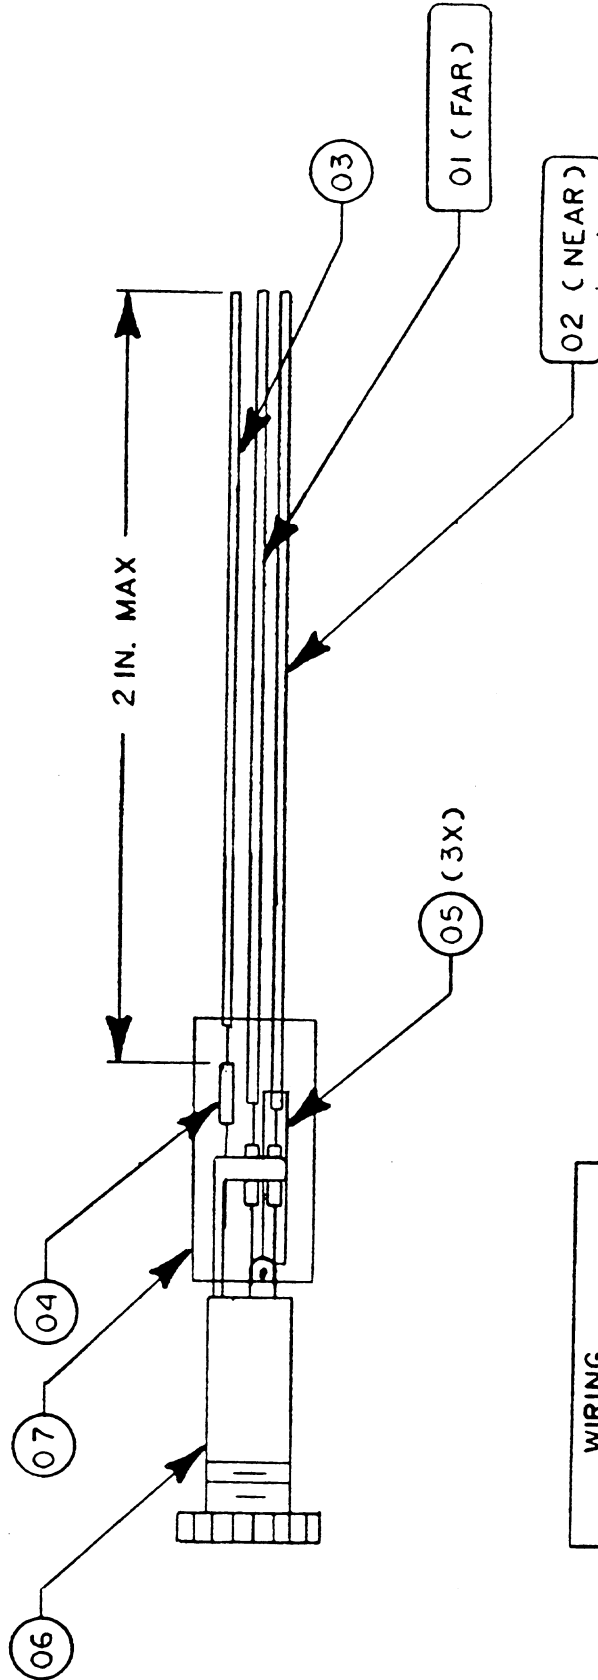

WIRING	
PIN 1	BROWN
PIN 2	RED
PIN 3	ORANGE

4-18

REV: B

NO.	QTY.	DESCRIPTION	PART NO.	TOLERANCES UNLESS OTHERWISE SPECIFIED			APPROVALS	DATE	DRAWN A. KRAUSE	CHECKED	2-22-89
				±	±	±					
07	1	1/4" DIA. HT. SHRINK 1/2" LENGTH	385000-0005A								
06	1	CONN. MINI STEREO	354000-0144A								
05	3	1/16" SHRINK TUBING 1/2" LENGTH	385000-0003A								
04	3	RESISTOR 1K, 1/4W, 5%	370100-0102A								
03	1	WIRE ORANGE 24GA STRD. 1.5"	399100-0003A								
02	1	WIRE RED 24GA STRD. 1.5"	399100-0002A								
01	1	WIRE BROWN 24 GA STRD 1.5"	399100-0001A								
				SCALE 2X							
				SIZE A							
				DRAWING NO. 400903-0000							
				DEFIB SYNC CONNECTOR HARNESS ASSY.							
				MEDICAL DATA ELECTRONICS							
				DO NOT SCALE DRAWING							
				SHEET 1 OF 1							

Assembly	Description	Group	PFC	Commodity Class	Planner	Buyer	Drawing	Rev	LT
401596-0000	PCBA, ECG W/RESP 5LD DAUGHTER REV. A1 (D126)			A				A1	22
Shrinkage Factor: 0.000									

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
401594-0000	*1	1	PCB, ECG 5LD DAUGHTER REV A . A (E973)	R		22	1.000	EA		Yes		
354000-0142A	*1	2	CONN, 7 SKT STRP,.1 SKT S P,.335 HT	R		22	1.000	EA		Yes		
354000-0143A	*1	3	CONN, 4 SKT STRP,.1 SKT S P,.335 HT.	R		22	1.000	EA		Yes		
370101-0103A	*1	4	RES, 10K,1/8W,5%,CF	R		11	6.000	EA	R7,25,26,27,28,40	Yes		
370101-0203A	*1	5	RES, 20K,1/8W,5%,CF	R		11	5.000	EA	R1,4,6,10,39	Yes		
370101-0513A	*1	6	RES, 51K,1/8W,5%,CF	R		11	3.000	EA	R2,3,5	Yes		
370402-0103A	*1	7	RES, 10K,1/2W,5%,CC (ALL N BRDLY ONLY)*BULK ONLY*	R		22	6.000	EA	R17-22	Yes		
100000	*1	8	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	ABOVE ALL MATCHED 1%	Yes		
378000-0054A	*1	9	DIO, 1N4764,100V,ZENER	R		22	10.000	EA	D1-10	Yes		
352100-0104A	*1	10	CAP, .1UF,50V,10%,RAD,X7R	R		11	3.000	EA	C13,8,16	Yes		
380000-0017A	*1	11	SW, MINI,PCB MOUNT,5 POLE ,7-POS	R		44	1.000	EA	S1	Yes		
352300-0222A	*1	12	CAP, 2200PF,50V OR 100V,1 %,MYLAR,.15L.S.	R		77	5.000	EA	C1-5	Yes		
400554-0000	*1	13	IDCTR, MULTI ESCORT II, R EV. '8' **(FIFO)**	R		22	1.000	EA	L1	Yes		
360600-0016A	*1	14	LUG, 1/4,INT TOOTH,13/16 INCH LENGTH	R		11	1.000	EA		Yes		
400738-0000	*1	15	5-LEAD SHIELD, REV. 'B', GOLD IRRID.FINISH	R		22	1.000	EA		Yes		
352300-0104A	*1	16	CAP, .1UF,50V,20%,RAD,MYL AR	R		22	1.000	EA	C9	Yes		
352300-0103A	*1	17	CAP, .01UF,50V,20%,RAD,MY LAR	R		22	2.000	EA	C10,14	Yes		
352301-0105A	*1	18	CAP, 1UF,63V,20%,MYLAR	R		66	1.000	EA	C11	Yes		
352600-0019A	*1	19	CAP, .01UF,1000V,20%,Z5U, CER DISC,.4 L.S.	R		11	2.000	EA	C6,7	Yes		
364000-0135A	*1	20	IC, LF347, SCREENED TO +/- -1.5mV OFFSET & LOW NOISE	A		22	1.000	EA	U1	Yes		
370101-0121A	*1	21	RES, 120,1/8W,5%,CF	R		11	1.000	EA	R15	Yes		
370101-0104A	*1	22	RES, 100K,1/8W,5%,CF	R		11	3.000	EA	R12,13,32	Yes		
364000-0132A	*1	23	IC, LF444 NATIONAL ONLY	R		22	1.000	EA	U2	Yes		
370101-0242A	*1	24	RES, 2.4K,1/8W,5%,CF	R		11	1.000	EA	R8	Yes		

Assembly Description
401596-0000 PCBA, ECG W/RESP 5LD DAUGHTER REV. A1 (D126)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
A1 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
370101-0221A	*1	25	RES, 220,1/8W,5%,CF	R		11	1.000	EA	R9	Yes		
370101-0105A	*1	26	RES, 1M,1/8W,5%,CF	R		11	1.000	EA	R14	Yes		
370101-0912A	*1	27	RES, 9.1K,1/8W,5%,CF	R		11	1.000	EA	R11	Yes		
376000-0019A	*1	28	XSTR, 2N7000,FET	R		11	1.000	EA	Q1	Yes		
378000-0005A	*1	29	DIO, 1N914,SIGNAL T&R	R		11	3.000	EA	D11,12,14	Yes		
378000-0009A	*1	30	DIO, 1N754A,6.8V,ZENER T&R ***HOT ONLY***	R		11	2.000	EA	D16,17	Yes		
400553-0000	*1	31	XFMR, ESC. II RESP DRIVE REV. A **(FIFO)**	R		22	1.000	EA	T1	Yes		
352300-0474A	*1	32	CAP, .47UF, 50V,20%,RAD,MYLAR(METALLIZED POLYESTR)	R		22	1.000	EA	C12	Yes		
365000-0014A	*1	33	SKT, 14-POS,DIP,TIN PLATE ,L.P.	R		11	1.000	EA	U1	Yes		
370101-0913A	*1	34	RES, 91K,1/8W,5%,CF	R		22	1.000	EA	R16	Yes		
378000-0037A	*1	35	DIO, MBR030,SCHOTTKY RCTF R	R		11	1.000	EA	D13	Yes		
382200-0015A	*1	36	CHOKE, 680 UH	R		11	1.000	EA	L2	Yes		
384000-0047A	*1	37	BUMPERS, .125 INCH, BLACK	R		22	1.000	EA		Yes		
352400-0105A	*1	38	CAP, 1UF,50V,20%,RAD,TANT , MAX: HT. .28; O.D. .16	R		11	1.000	EA	C15	Yes		
364000-0010A	*1	39	IC, LM339	R		11	1.000	EA	U3	Yes		
378000-0034A	*1	40	DIO, LM385,ZENER (XSTR NA TIONAL ONLY)	R		11	3.000	EA	D19,18,15	Yes		
370500-0107A	*1	41	RES, 100M,1/4W,5%,M.O. (O R M.G.)	R		33	2.000	EA	R23,24	Yes		
370101-0183A	*1	42	RES, 18K,1/8W,5%,CF	R		11	1.000	EA	R41	Yes		
370101-0302A	*1	43	RES, 3K,1/8W,5%,CF	R		11	1.000	EA	R38	Yes		
370101-0303A	*1	44	RES, 30K,1/8W,5%,CF	R		11	1.000	EA	R37	Yes		
370101-0304A	*1	45	RES, 300K,1/8W,5%,CF	R		11	1.000	EA	R35	Yes		
370101-0472A	*1	46	RES, 4.7K,1/8W,5%,CF	R		11	1.000	EA	R29	Yes		
370101-0473A	*1	47	RES, 47K,1/8W,5%,CF	R		11	1.000	EA	R34	Yes		
370101-0474A	*1	48	RES, 470K,1/8W,5%,CF	R		11	1.000	EA	R30	Yes		

Assembly Description
401596-0000 PCBA, ECG W/RESP 5LD DAUGHTER REV. A1 (D126)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing Rev LT
A 1 A1 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
370101-0512A	*1	49	RES, 5.1K,1/8W,5%,CF	R		11	1.000	EA	R31	Yes		
370101-0623A	*1	50	RES, 62K,1/8W,5%,CF	R		11	1.000	EA	R36	Yes		
370101-0684A	*1	51	RES, 680K,1/8W,5%,CF	R		11	1.000	EA	R33	Yes		
382200-0027A	*1	52	IDCTR, 82uH,SHIELDED,ISOLATED	R		22	1.000	EA	L3 IN SERIES WITH D13	Yes		
352100-0220A	*1	53	CAP, 22PF,50V,10%,RAD,NPO EDPT	R		22	1.000	EA	ACROSS PRIMARY OF T1	Yes		
352100-0220A	*1	54	CAP, 22PF,50V,10%,RAD,NPO EDPT	R		22	0.000	EA	FLY ON SOLDER SIDE	Yes		
100000	*1	55	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	FOR ASSEMBLY	Yes		
100000	*1	56	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	FOR RESISTORS CHECK	Yes		
100000	*1	57	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	BIN - FILL IF REQUIRE	Yes		
352101-0472A	*1	58	CAP, 4700PF,20%,3KV, Z5U, CERAMIC DISC (5000PF OK)	R		22	1.000	EA	C17	Yes		
364000-0175A	*1	59	IC, PC219,PHOTOCOUPLER,MI NI-FLAT PKG.	R		22	2.000	EA	U4-5	Yes		
370100-0472A	*1	60	RES, 4.7K,1/4W,5%,CF	R		11	1.000	EA	R42	Yes		
900000	*1	99	ASSEMBLY LABOR & BURDEN	L		0	0.910	HR		Yes		

Cumulative Lead Time for 401596-0000 = 99

Assembly Description
401593-0000 PCBA, ECG 5LD MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
D 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
401592-0000	*1	1	PCB, ECG 5LD MOTHER REV. A (E973)	R		22	1.000	EA		Yes		
352300-0102A	*1	2	CAP, 1000PF,50V,20%,RAD,M YLAR	R		66	1.000	EA	C18	Yes		
352300-0103A	*1	3	CAP, .01UF,50V,20%,RAD,MY LAR	R		22	2.000	EA	C17,22	Yes		
352300-0104A	*1	4	CAP, .1UF,50V,20%,RAD,MYL AR	R		22	6.000	EA	C5,6,30,36,37,31	Yes		
352301-0104A	*1	5	CAP, .1UF,5%,MYLAR	R		66	1.000	EA	C10	Yes		
354000-0084A	*1	6	CONN, 3-P,M,STRT LCK,.1 C TR	R		11	1.000	EA	J3	Yes		
352100-0471A	*1	7	CAP, 470PF,25V,10%,RAD,X7 R	R		22	1.000	EA	C11	Yes		
352300-0007A	*1	8	CAP, .001UF,10%, MYLAR	R		66	2.000	EA	C26,27	Yes		
352100-0223A	*1	9	CAP, .022UF,50V,10%,RAD,X 7R	R		22	1.000	EA	C7	Yes		
352300-0018A	*1	10	CAP, .47UF,10%,MYLAR	R		66	1.000	EA	C13	Yes		
352301-0103A	*1	11	CAP, .01UF,100V,20%,POLYC ARB,.2 L.S.	R		66	1.000	EA	C34	Yes		
352401-0106A	*1	12	CAP, 10UF,35V,20%,RAD,TAN T	R		11	6.000	EA	C19,20,21,25,32,33	Yes		
352400-0226A	*1	13	CAP, 22UF,25V,20%,TANT	R		11	2.000	EA	C23,24	Yes		
352401-0476A	*1	14	CAP, 47UF,10V,20%,RAD,TAN T (10V ONLY)	R		11	2.000	EA	C14,15	Yes		
354000-0104A	*1	15	CONN, SGL ROW,STRT,SGL PI NS,SNAP-AWAY	R		11	4.000	PIN	1 PC. OF 4 PINS	Yes		
354000-0104A	*1	16	CONN, SGL ROW,STRT,SGL PI NS,SNAP-AWAY	R		11	7.000	PIN	1 PC. OF 7 PINS	Yes		
356000-0008A	*1	17	REF OSCILLATOR, 4.0MHZ,CM OS HIGH SPEED	R		22	1.000	EA	Y1	Yes		
360500-0048A	*1	18	SPCR, 1/4 X 1/4,SWAGE TYP E	R		11	1.000	EA	DO NOT ISSUE	Yes		
364000-0008A	*1	19	IC, DG212CJ	R		11	1.000	EA	U2	Yes		
364000-0114A	*1	20	IC, TL064 ACN	R		11	1.000	EA	U4	Yes		
364000-0010A	*1	21	IC, LM339	R		11	1.000	EA	U3	Yes		
364000-0027A	*1	22	IC, 74HC32	R		11	2.000	EA	U14,15	Yes		
364000-0029A	*1	23	IC, 74HC138	R		11	1.000	EA	U12	Yes		
364000-0038A	*1	24	IC, 27C256,CMOS,EPROM,200 NS	R		11	1.000	EA	U10	Yes		

Assembly Description
401593-0000 PCBA, ECG SLD MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
D 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
364000-0132A	*1	25	IC, LF444 NATIONAL ONLY	R		22	1.000	EA	U1	Yes		
364000-0080A	*1	26	IC, TMP284C00P (Z80A, CM OS VERSION)	R		11	1.000	EA	U9	Yes		
364000-0091A	*1	27	IC, SG 3525	R		44	1.000	EA	U8	Yes		
364000-0093A	*1	28	IC, ILQ5 QUAD OPTO ISOLAT OR	R		22	2.000	EA	U5,6	Yes		
364000-0094A	*1	29	IC, HP2630, OPTO ISOLATOR	R		11	1.000	EA	U7	Yes		
364000-0095A	*1	30	IC, MS6132, DUAL PORT RAM, 8 X 2K, 48-PIN (OR MS7132)	R		11	1.000	EA	U11	Yes		
364000-0096A	*1	31	IC, 74HC240	R		11	1.000	EA	U13	Yes		
364000-0097A	*1	32	IC, 74HC374	R		11	1.000	EA	U16	Yes		
364000-0098A	*1	33	IC, 82C54, CTC	R		11	1.000	EA	U17	Yes		
370100-0010A	*1	34	RES, 1, 1/4W, 5%, CF	R		11	2.000	EA	R63,64	Yes		
370100-0101A	*1	35	RES, 100, 1/4W, 5%, CF	R		11	1.000	EA	R47	Yes		
370100-0102A	*1	36	RES, 1K, 1/4W, 5%, CF	R		11	4.000	EA	R27-29,32	Yes		
370100-0102A	*1	37	RES, 1K, 1/4W, 5%, CF	R		11	1.000	EA	R53	Yes		
370100-0103A	*1	38	RES, 10K, 1/4W, 5%, CF	R		11	6.000	EA	R20,35,54,60-62	Yes		
370100-0104A	*1	39	RES, 100K, 1/4W, 5%, CF	R		11	2.000	EA	R55,56	Yes		
370100-0121A	*1	40	RES, 120, 1/4W, 5%, CF	R		11	2.000	EA	R9,10	Yes		
370100-0153A	*1	41	RES, 15K, 1/4W, 5%, CF	R		11	1.000	EA	R40	Yes		
370100-0204A	*1	43	RES, 200K, 1/4W, 5%, CF	R		11	1.000	EA	R19	Yes		
370100-0221A	*1	44	RES, 220, 1/4W, 5%, CF	R		11	2.000	EA	R57,59	Yes		
370100-0222A	*1	45	RES, 2.2K, 1/4W, 5%, CF	R		11	1.000	EA	R45	Yes		
370100-0334A	*1	46	RES, 330K, 1/4W, 5%, CF	R		11	1.000	EA	R58	Yes		
370100-0243A	*1	47	RES, 24K, 1/4W, 5%, CF	R		11	1.000	EA	R15	Yes		
370100-0333A	*1	48	RES, 33K, 1/4W, 5%, CF	R		11	1.000	EA	R12	Yes		
370100-0622A	*1	49	RES, 6.2K, 1/4W, 5%, CF	R		11	1.000	EA	R51	Yes		

Assembly Description
401593-0000 PCBA, ECG SLD MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
D 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
370100-0473A	*1	50	RES, 47K,1/4W,5%,CF	R		11	3.000	EA	R17,25,31	Yes		
370100-0620A	*1	51	RES, 62,1/4W,5%,CF	R		11	1.000	EA	R11	Yes		
370200-6342A	*1	52	RES, 63.4K,1/4W,1%,MF	R		11	1.000	EA	R7	Yes		
370101-0153A	*1	53	RES, 15K,1/8W,5%,CF	R		11	1.000	EA	R48	Yes		
370101-0104A	*1	54	RES, 100K,1/8W,5%,CF	R		11	3.000	EA	R23,24,34	Yes		
370200-3011A	*1	55	RES, 3.01K,1/4W,1%,MF	R		11	1.000	EA	R1	Yes		
370101-0222A	*1	56	RES, 2.2K,1/8W,5%,CF	R		11	1.000	EA	R18	Yes		
370101-0332A	*1	57	RES, 3.3K,1/8W,5%,CF	R		22	1.000	EA	R49	Yes		
370200-1183A	*1	58	RES, 118K,1/4W,1%,MF	R		11	1.000	EA	R36	Yes		
370200-1210A	*1	59	RES, 121,1/4W,1%,MF	R		11	1.000	EA	R44	Yes		
370200-2002A	*1	60	RES, 20K,1/4W,1%,MF	R		11	1.000	EA	R38	Yes		
370200-3322A	*1	61	RES, 33.2K,1/4W,1%,MF	R		11	1.000	EA	R22	Yes		
370200-4990A	*1	62	RES, 499,1/4W,1%,MF	R		11	2.000	EA	R41,42	Yes		
370200-5492A	*1	63	RES, 54.9K,1/4W,1%,MF	R		11	1.000	EA	R14	Yes		
370200-6812A	*1	64	RES, 68.1K,1/4W,1%,MF	R		11	5.000	EA	R2-6	Yes		
370200-8872A	*1	65	RES, 88.7K,1/4W,1%,MF	R		11	1.000	EA	R39	Yes		
370200-9761A	*1	66	RES, 9.76K,1/4W,1%,MF	R		11	1.000	EA	R43	Yes		
374300-0202A	*1	67	POT, 2K,TRIM,SIDE ADJ,CER MET,3/8 SQR,.15LS	R		11	1.000	EA	R46	Yes		
374401-0103A	*1	68	POT, 10K,TRIM,MULTI-TURN ,CERMET FILM (860X)	R		11	2.000	EA	R8,66	Yes		
376000-0019A	*1	69	XSTR, 2N7000,FET	R		11	2.000	EA	Q4,5	Yes		
376000-0020A	*1	70	XSTR, J201,FET	R		11	2.000	EA	Q1,2	Yes		
378000-0005A	*1	71	DIO, 1N914,SIGNAL T&R	R		11	6.000	EA	D6,7,8,9,10,14	Yes		
378000-0005A	*1	72	DIO, 1N914,SIGNAL T&R	R		11	2.000	EA	D11,12	Yes		
378000-0034A	*1	73	DIO, LM385,ZENER (XSTR NA TIONAL ONLY)	R		11	1.000	EA	D5	Yes		

Assembly Description
401593-0000 PCBA, ECG 5LD MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
D 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
400552-0000	*1	75	ESCORT II ISO-TRANSFORMER , REV. 'A' **(FIFO)**	R		22	1.000	EA	T1	Yes		
352100-0003A	*1	76	CAP, 3.3PF,50V,+/- .5PF,RA D,NPO EDPT	R		11	1.000	EA	C16	Yes		
370100-0332A	*1	77	RES, 3.3K,1/4W,5%,CF	R		11	1.000	EA	R13	Yes		
365000-0024A	*1	82	SKT, 24-POS,DIP,TIN PLATE ,L.P.	R		11	1.000	EA		Yes		
365000-0028A	*1	83	SKT, 28-POS,DIP,TIN PLATE ,L.P.	R		11	1.000	EA		Yes		
365000-0040A	*1	84	SKT, 40-POS,DIP,TIN PLATE ,L.P.	R		11	1.000	EA		Yes		
370200-6191A	*1	86	RES, 6.19K, 1/4W 1%, MF	R		11	1.000	EA	R37	Yes		
378000-0009A	*1	87	DIO, 1N754A,6.8V,ZENER T& R ***MOT ONLY***	R		11	1.000	EA	D13	Yes		
370200-1001A	*1	88	RES, 1K,1/4W,1%,MF	R		11	1.000	EA	R21	Yes		
352300-0222A	*1	89	CAP, 2200PF,50V OR 100V,1 %,MYLAR,.15L.S.	R		77	1.000	EA	C40	Yes		
370101-0163A	*1	90	RES, 16K,1/8W,5%,CF	R		11	1.000	EA	R30	Yes		
370100-0392A	*1	91	RES, 3.9K,1/4W,5%,CF	R		11	1.000	EA	R50	Yes		
370100-0271A	*1	92	RES, 270,1/4W,5%,CF	R		11	1.000	EA	R26	Yes		
370101-0202A	*1	93	RES, 2K,1/8W,5%,CF	R		11	1.000	EA	R65	Yes		
352101-0471A	*1	95	CAP, 470pF,10%,50V,RAD,NP O	R		22	2.000	EA	C3,4	Yes		
352300-0008A	*1	96	CAP, .01UF,5%,MYLAR	R		66	2.000	EA	C8,9	Yes		
352400-0105A	*1	97	CAP, 1UF,50V,20%,RAD,TANT , MAX: HT. .28; O.D. .16	R		11	1.000	EA	C28	Yes		
370102-0010A	*1	98	RES, 1,1/2W,5%,CF	R		11	1.000	EA	R52	Yes		
900000	*1	99	ASSEMBLY LABOR & BURDEN	L		0	0.990	HR		Yes		
384000-0061A	*1	100	GAS TUBE (SURGE ARRESTER)	R		33	1.000	EA	DS1	Yes		
352100-0104A	*1	101	CAP, .1UF,50V,10%,RAD,X7R	R		11	1.000	EA	C35	Yes		
352100-0220A	*1	102	CAP, 22PF,50V,10%,RAD,NPO EDPT	R		22	4.000	EA	C38,39,1,2	Yes		
352300-0015A	*1	103	CAP, .22UF,10%,MYLAR	R		66	1.000	EA	C12	Yes		
370100-0273A	*1	104	RES, 27K,1/4W,5%,CF	R		11	1.000	EA	R69	Yes		

Assembly Description
401593-0000 PCBA, ECG SLD MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
D 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
370401-0108A	*1	105	RES, 1000M,1W,5%,2500V	R		66	1.000	EA	R70	Yes		
378000-0011A	*1	106	DIO, 1N4741A,11V,ZENER T&R ***MOTOROLA ONLY***	R		11	2.000	EA	D15,16	Yes		
365000-0148A	*1	107	SOCKET, 48 PIN DIP	R		22	1.000	EA	U11	Yes		
100000	*1	108	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	FOR ASSEMBLY	No		
100000	*1	109	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	FOR RESISTORS CHECK	No		
100000	*1	110	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	BIN - FILL IF REQUIRE	No		
370100-0511A	*1	111	RES, 510,1/4W,5%,CF	R		11	1.000	EA	R33	Yes		
370200-1402A	*1	112	RES, 14K,1/4W,1%,MF	R		11	1.000	EA	R16	No		

Cumulative Lead Time for 401593-0000 = 99

TEMPERATURE PRESSURE BOARD

CHAPTER 5

5.0.0 TEMPERATURE-PRESSURE BOARD

5.1.0 OVERVIEW

Another optional processor board in the ESCORT 300A is the TEMP-PRESS BOARD. Whether the monitor is configured for temperature or blood pressure, the circuitry to implement the configuration is on the TEMP-PRESS board.

The two main functions of the board are: (1) To detect temperature and display on the screen the value in degrees C or degrees F (selectable by user), and (2) To receive a signal from a pressure transducer, interpret, and reproduce the pressure waveform on the screen, while calculating the mean, systolic and diastolic values. All information is received in analog and converted to a digital format that is stored in RAM on the CPU Board.

The TEMP-PRESS board also provides an excitation voltage of +5VDC for use by the pressure transducer.

As on the ECG Board, an ISOLATION BARRIER is also utilized to protect the patient from line current. The barrier is created by the use of opto couplers. The isolated section has its own power supply to complete the barrier.

5.2.0 ISOLATION SECTION

5.2.1 TEMPERATURE INPUTS

The temperature input connector to the ESCORT 300A is a 1/4 inch stereo phone jack. 700 series temperature probes are used by the ESCORT 300A. There is an option that can provide 400 series temperature probe input. Temperature is detected by measuring the resistance from the probe and interpreting that resistance to a temperature value.

The temperature inputs for T1 at J5 are protected by zener diodes D10 and D11. Capacitors C40, C41 and C44 are for noise reduction. U10 pin 14 is a constant current source of 2.5uA to the temperature probes. The resistance change that occurs in the probe parallels the temperature change. This will produce a voltage across R50 and R51. The signal HALFREF (2.5V) goes to U10 pin 12. R52 is adjusted to offset and to equal U10 pin 12, so only the difference is seen at the output. This difference is equal to the temperature. R50 and R51 will divide the signal to a level that is usable by the multiplexer, creating the signals TPOS1 and TNEG1. These signals go directly to MUX, U11 and U14.

The input circuit for T2 is functionally identical to that of T1.

5.2.2 PRESSURE INPUTS

The pressure inputs are on J3 (BP1) and J2 (BP2). The inputs are protected by zener diodes D14-D18. The +5VDC excitation goes to the transducer through pin 13 on J2 and J3. The +SIG and -SIG are filtered by LC circuits to reduce noise. L1, C19 and C20 filter BP1 and L2, C21 and C22 filter BP2. The filtered signal PPOS1, PNEG1 and PPOS2, PNEG2 also go to MUX, U11 and U14.

5.2.3 MULTIPLEXERS

U11 and U14 are 8 to 1 multiplexers that are addressed by the microprocessor. The address lines E0, E1, and E2 are used by the processor to walk through the inputs one at a time and send the appropriate signal on to the A to D circuit.

Along with temperature and pressure signals, other signals that the processor walks through at the MUX are the GROUND and the REFERENCE VOLTAGE. Information from the ground signal is used by software to determine what ground will look like when it is sent through the A to D circuit, and will use that as a zero reference. The reference voltage generated by metal film resistors R47, R48, and R49 is used by software as a calibration standard, and will adjust all other readings appropriately. R47 is adjusted for a reading of 100mmHg by the monitor when a calibrated 100mmHg is input to it.

5.2.4 ANALOG TO DIGITAL

The positive and negative signals are passed on to the differential amplifier which begins the A to D conversion. As on the ECG Board, a ramp waveform is compared to the signal input; when both are equal, the sample voltage is turned into a digital data point to be used by the digital portion of the board. Here again, reference voltages are used to initiate timing cycles. A 900us time limit is set by the CTC (U5) to retrieve and calculate one data point.

U12 is a high impedance differential amplifier that subtracts and amplifies the input signals. The output at U12 pin 7 has a gain of 770. R30 adjusts to compensate for common mode offset, and to give the circuit more precision.

SAMPLE RST is used to begin a new "fetch datapoint" cycle by driving U13 pins 8 and 11 to -11.7V. As the voltage from U12 pin 8 ramps up, the counter (U5) will start and the square wave (SAMPLE) will go high. The ramp will continue up until its voltage is equal to the signal at U13 pin 9. Since pins 13 and 14 are wired OR'd together, U13 pin 14 will pull the outputs low, completing the square wave and stopping the counter. Q1 is used as a current source to drive the opto-coupler, U17.

5.2.5 EXCITATION VOLTAGE

The excitation voltage provided by the ESCORT 300A is +5VDC. D8 and D20 are 2.5V reference diodes that put +5V at U10 pin 5. Q2 is used to give the +5V a higher current capability. VREF becomes + excitation voltage to the transducer.

5.2.6 ISOLATION POWER SUPPLY

Plus and minus voltages for the isolated section of the board are supplied by U15 and T1. PS SYNC drives the pulse width modulator, U15, and synchronizes it with all other supply voltages in the monitor. T1 furnishes isolation to complete the barrier. D4-D7 rectify the AC to DC; L3, L4, C9 and C10 filter out the ripple. +V is equal to +15V and -V is equal to -15V.

5.3.0 NON-ISOLATED

5.3.1 TEMP-PRESS DIGITAL

The digital portion of the TEMP-PRESS board is identical to the ECG Board.

The microprocessor chip is a Z-80 type microprocessor. Y1 clocks U1 at 4MHz. I/O reads and writes (IORD, IOWR) and memory reads and writes (MRD, MWR) are decoded by U8 from the signals at pins 19-22. The TEMP-PRESS data address bus directs information to and from the EPROM, Dual Port RAM, CTC and address decoders. The microprocessor is reset by the CPU Board signal RSTOUT*. WAIT at pin 24 inserts wait cycles to the CPU from the Dual Port RAM. The interrupt on pin 16 will indicate to the microprocessor that 900 microseconds have elapsed since the start of the sampling cycle and will request the processor to terminate this cycle. Pin 17 is the signal TIMETIC* which synchronizes the sampling cycle so that each TIMETIC* denotes getting and decoding one data point.

The EPROM (U2) stores software for the TEMP-PRESS board and is enabled by U4 and the MRD signal.

The Dual Port RAM (U3) is a 2K x 8 bit CMOS RAM MS6132. It provides two ports with separate controls, address and I/O that permit separate access to memory reads and writes. The Dual Port RAM interfaces the CPU board data address bus to the TEMP-PRESS board. U3 is enabled by U4.

U6 and U7 are input and output ports. U7 outputs control signals to the isolated section of the board.

U5 is a Counter Timer Chip. It is programmable with four independent channels for counting and timing functions. It is enabled by IOWR, IORD, and A2, and it is clocked by Y1.

At SAMPLE RST the counter will start counting at the rate of 4MHz and will continue to count for 900 microseconds if it is not stopped before by the ramp voltage equaling the sample voltage in the A to D sample circuit.

5.4.0 SOFTWARE


Software for the TEMP-PRESS board is stored in the EPROM, U2.

Software tasks:

PRESSURE WAVEFORM	Correction for gain drift and amplification offset Low Pass filter, 15Hz cutoff Correction for transducer offset Final scaling for screen
PRESSURE CALCULATIONS	Mean calculation Heart rate picking Systolic calculation Diastolic calculation
TEMPERATURE CALCULATIONS	Correction for amplification and gain drift Low pass filter Linearization Conversion to degrees F
AUTO CALIBRATION	Compute gain and offset drift correction factors


Partial list of disposable type pressure transducer adapter cables for use with **ESCORT 300A**.

COMPANY NAME	PART NUMBER
Cobe	CDX3 - 041709-012
Baxter Edwards	Super Cable 892019-001
Baxter Edwards (HP)	UNIFLO893208-001
SpectraMed (Gould)	TCVTK 072393-000-013
Sorenson (Abbott Critical Care)	47987-01 or 42655-04-14
Deseret	38-8505-1
Utah Medical	650-208
MEDEX	MX900-03
MECWX (Reusable Disposable)	MX800-03

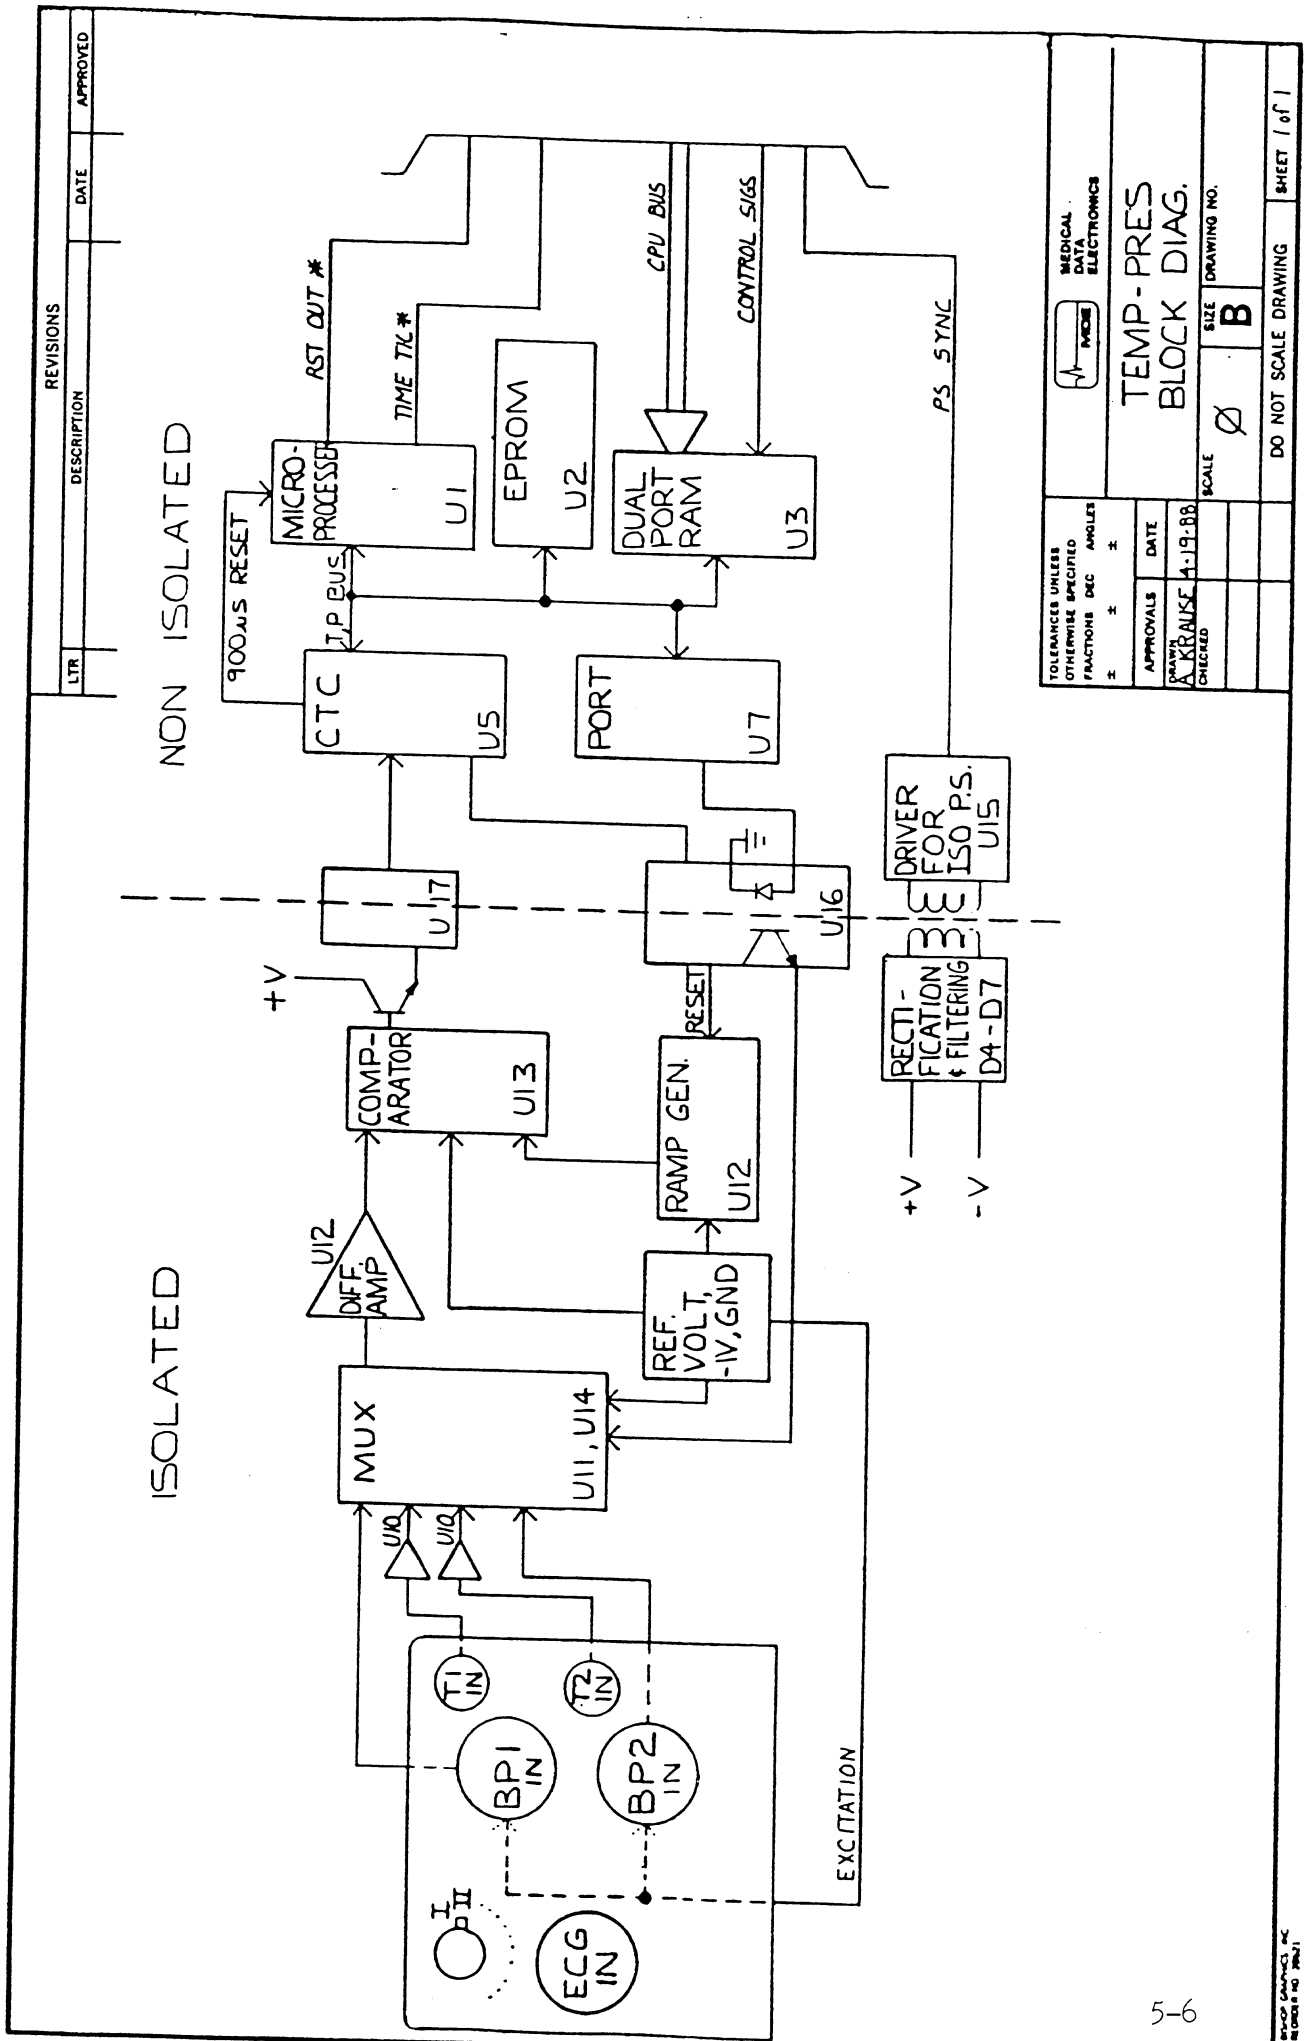

TOLERANCES UNLESS OTHERWISE SPECIFIED		FRACTIONS DEC ANGLES	
±	±	±	±
APPROVALS		DATE	
DRAWN BY A. KRAUSE		4-19-88	
CHECKED			


MEDICAL DATA ELECTRONICS		TEMP-PRES BLOCK DIAG.	
SCALE Ø		SIZE B	
DRAWING NO.		DO NOT SCALE DRAWING	
SHEET 1 of 1			

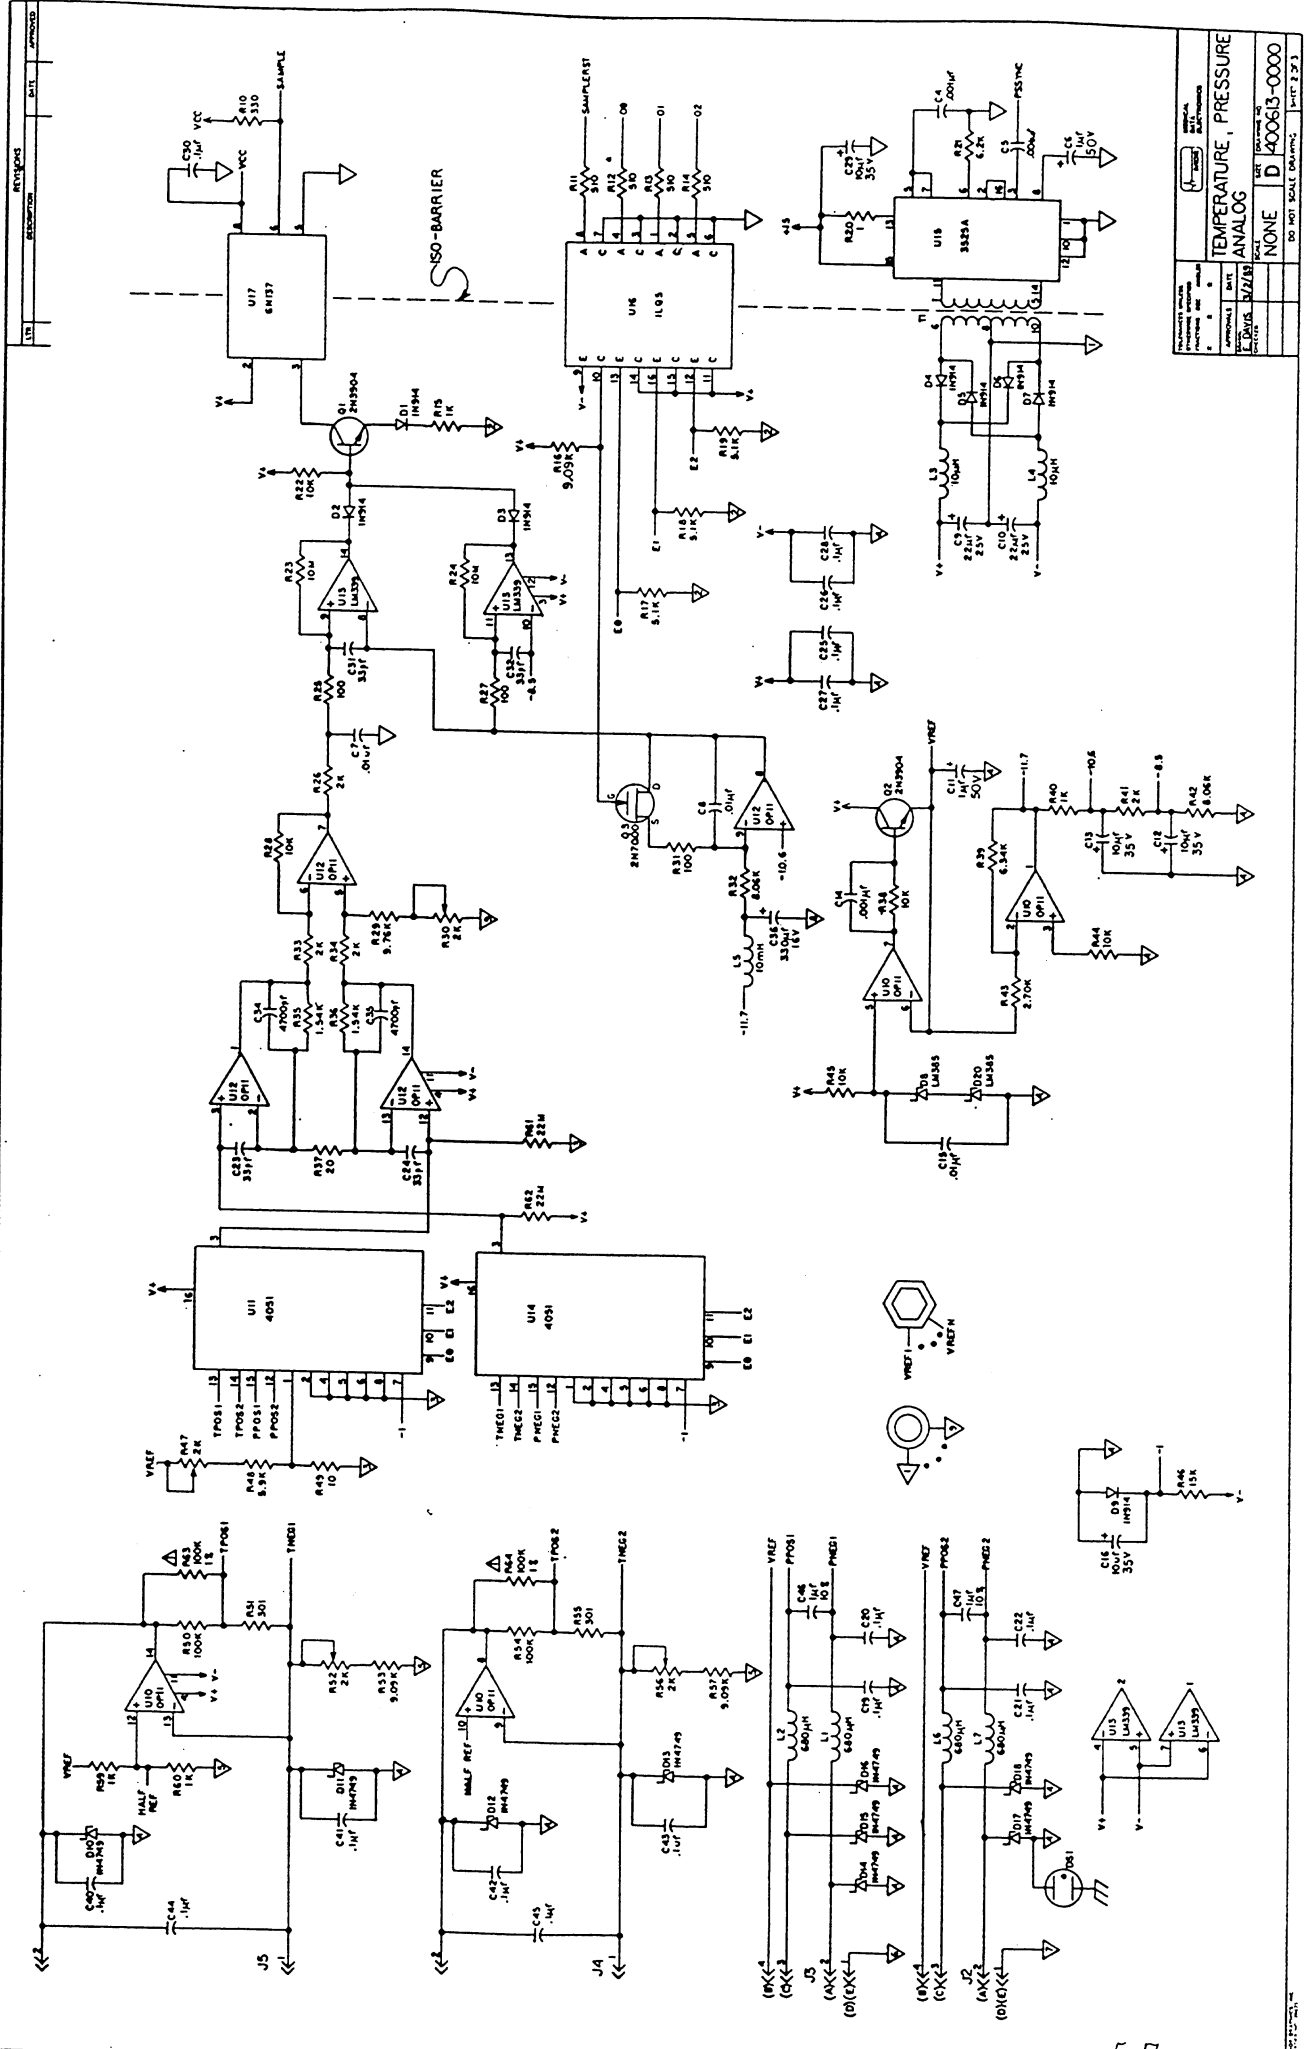

DESIGNER	DATE	REVISED	APPROVED
DAVIS	10/1/80		
TEMPERATURE, PRESSURE ANALOG			
NONE D 400613-0000			
DO NOT SCALE DRAWING			


REV	DESCRIPTION	REVISIONS	DATE	APPROVED
1	INITIAL RELEASE		1/17/87	
2	ECO 152		2/2/87	
3	ECO 158		2/2/87	
4	ECO 164		2/2/87	
5	ECO 193		3/10/88	
6	ECO 200		5/10/88	
7	ECO 201		5/10/88	
8	ECO 281		10/15/88	
9	ECO 285		10/15/88	
10	ECO 345		10/15/88	
11	ECO 421		2/2/89	
12	ECO 421		2/2/89	
13	ECO 614		8/1/89	
14	ECO 629		1/11/90	
15	ECO 707		10/26/90	
16	ECO 707		10/26/90	

LAAL USED	LAAL USED
Q47	T1
D20	U17
D81	T1
	PG.4
	NOT USED
D15	C5,17,18,33
	R38

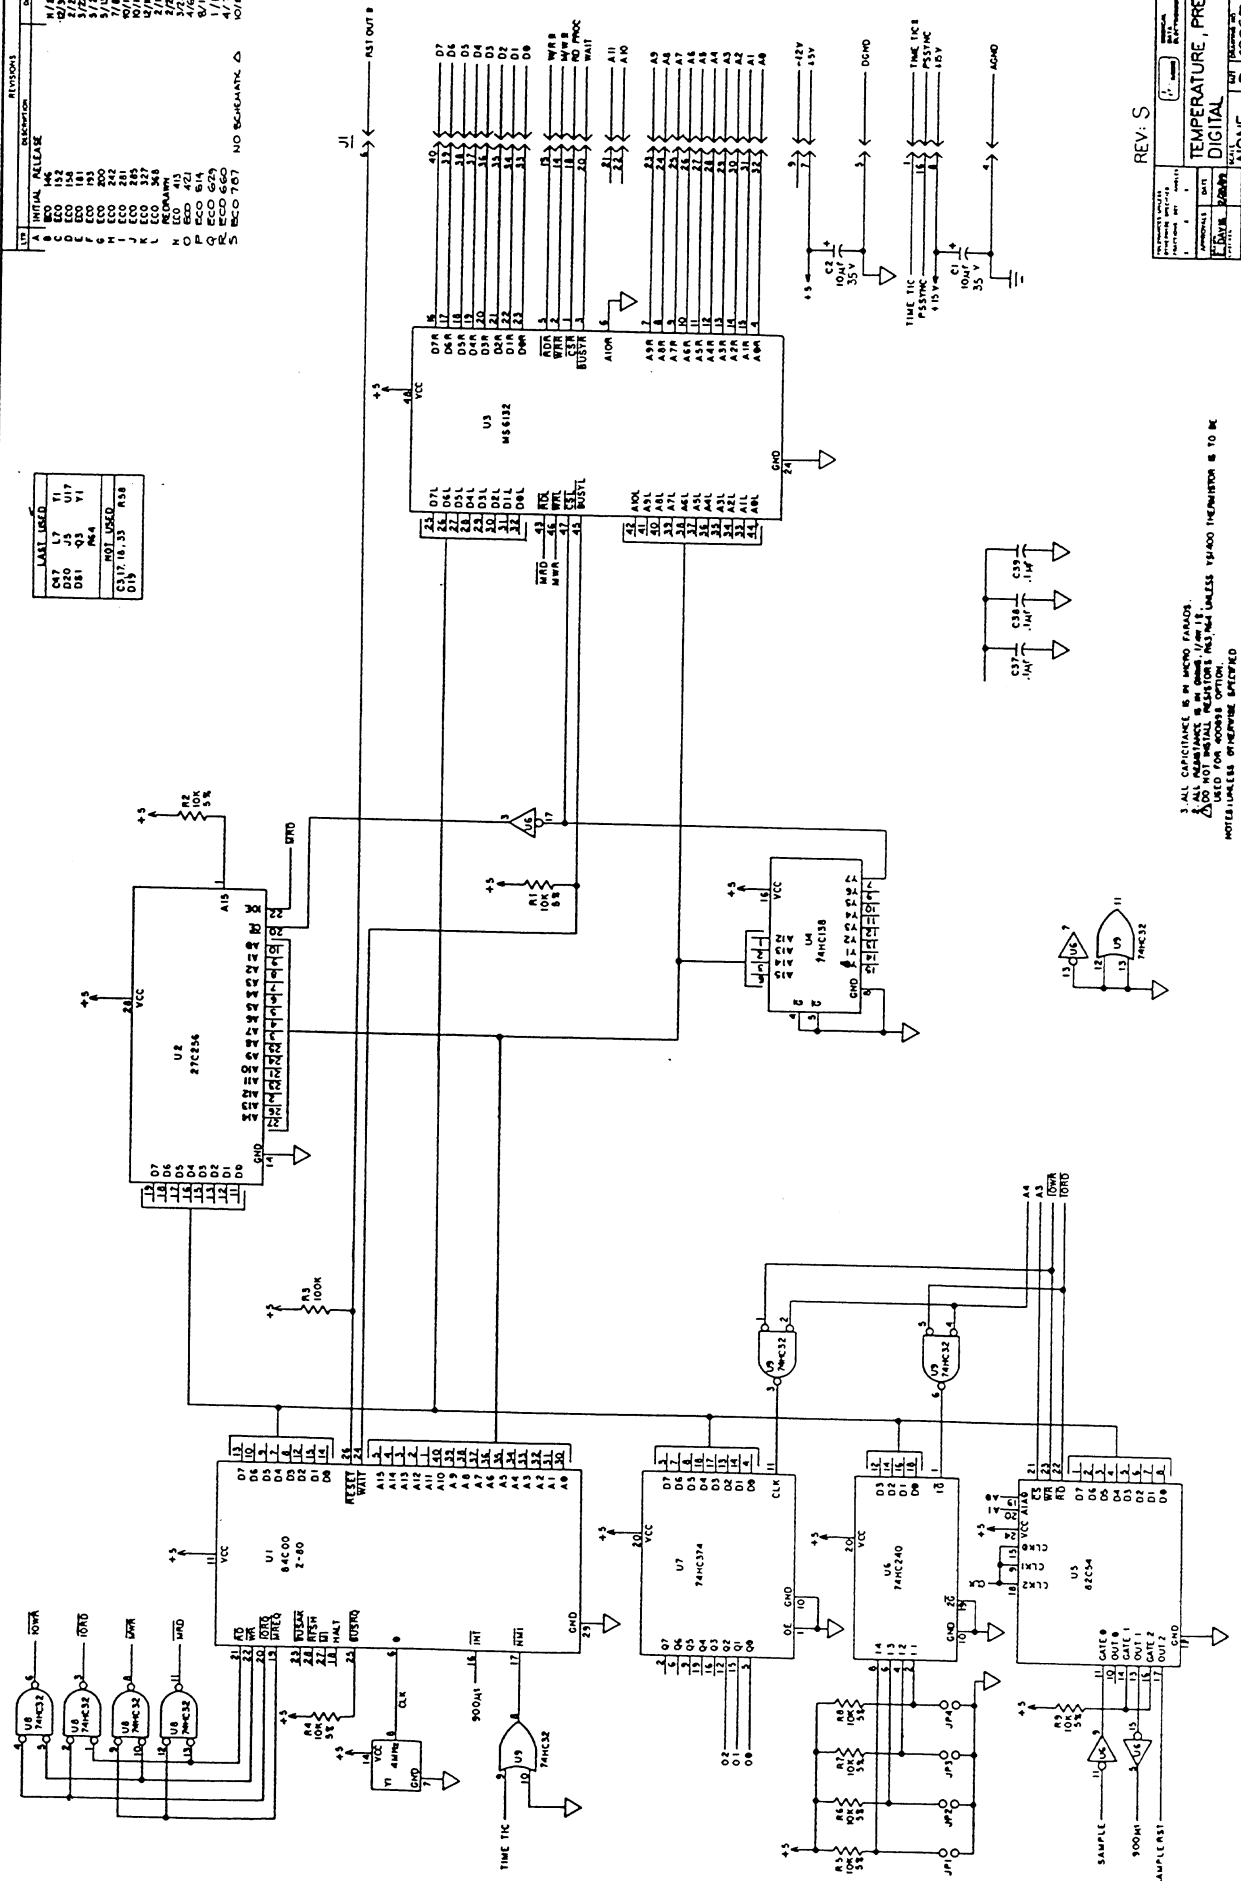


REV: S

3 ALL CAPACITANCE IS IN MICRO FARADS.
 4 ALL CAPACITANCE IS IN OHMS 1/1000.
 5 DO NOT INSTALL RESISTORS UNLESS THE OPTION IS TO BE
 6 UNLESS THE OPTION IS TO BE
 7 UNLESS THE OPTION IS TO BE

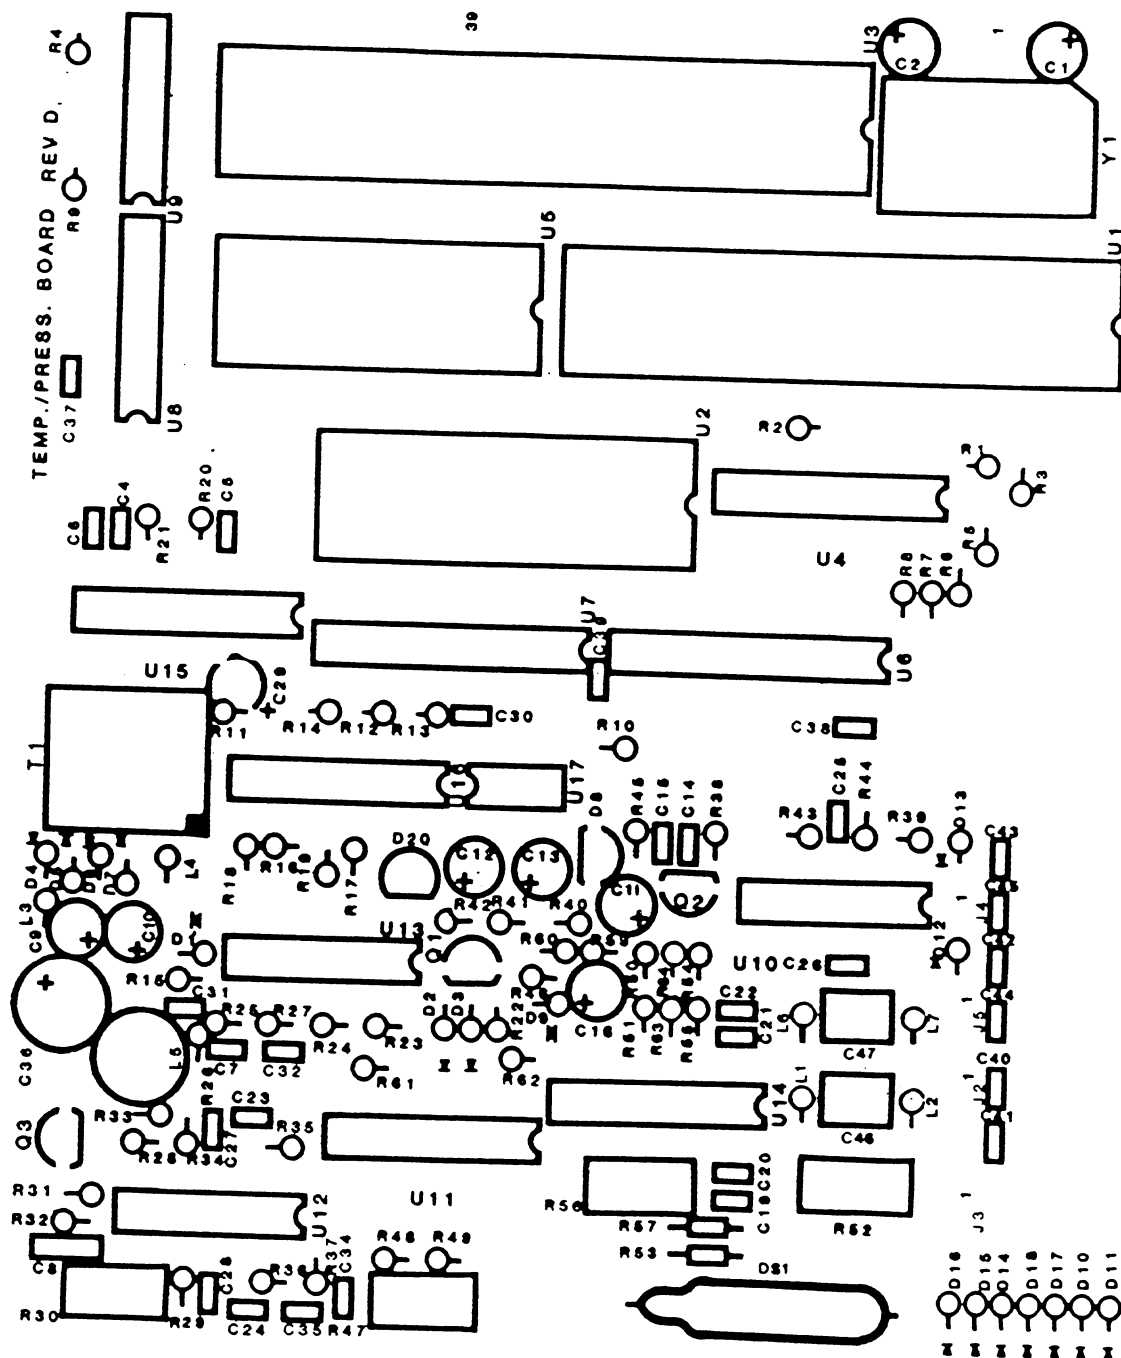

TEMP./PRESS. BOARD


MS 97-3102A14S-6S (639)



REAR VIEW

WIRING

VREF	B	YEL	4	VREF
+	C	ORG	3	+
-	A	RED	2	-
GND	D, E	BRN	1	GND



2.0"

TOLERANCES UNLESS OTHERWISE SPECIFIED		
FRACTIONS	DEC	ANGLES
±	±	±

APPROVALS	DATE
DRAWN A. KRAUSE	12-21-87
CHECKED	

--


MEDICAL DATA ELECTRONICS	
MDE	

PRESSURE CONN. HARNESS	
ESCORT 100/200 SERIES	
SCALE	DRAWING NO.
Ø	A 400698-0000

DO NOT SCALE DRAWING	SHEET 1 of 1
----------------------	--------------

REVISIONS

LTR	DESCRIPTION	DATE	APPROVED
A	INITIAL RELEASE	12-21-87	

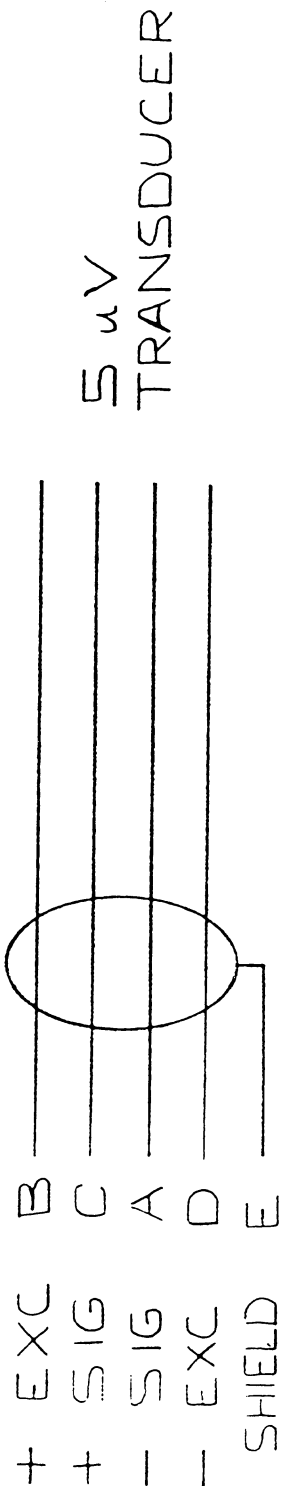


CABLE CONNECTOR
IS MS 3106E 14S-6P

REVISIONS

LTR	DESCRIPTION	DATE	APPROVED
A	INITIAL RELEASE	1-29-87	

TOLERANCES UNLESS OTHERWISE SPECIFIED		FRACTIONS DEC ANGLES		 MEDICAL DATA ELECTRONICS	
±	±	±	±		
APPROVALS	DATE				
DRAWN A. KRAUSE	1-29-88				
CHECKED					
PRESSURE XDUCER CABLE ESCORT 100 SERIES		SCALE Ø	SIZE A	DRAWING NO. REFERENCE ONLY	
		DO NOT SCALE DRAWING		SHEET / of /	

REVISIONS			
LTR	DESCRIPTION	DATE	APPROVED
A	INITIAL RELEASE	11/18/88	

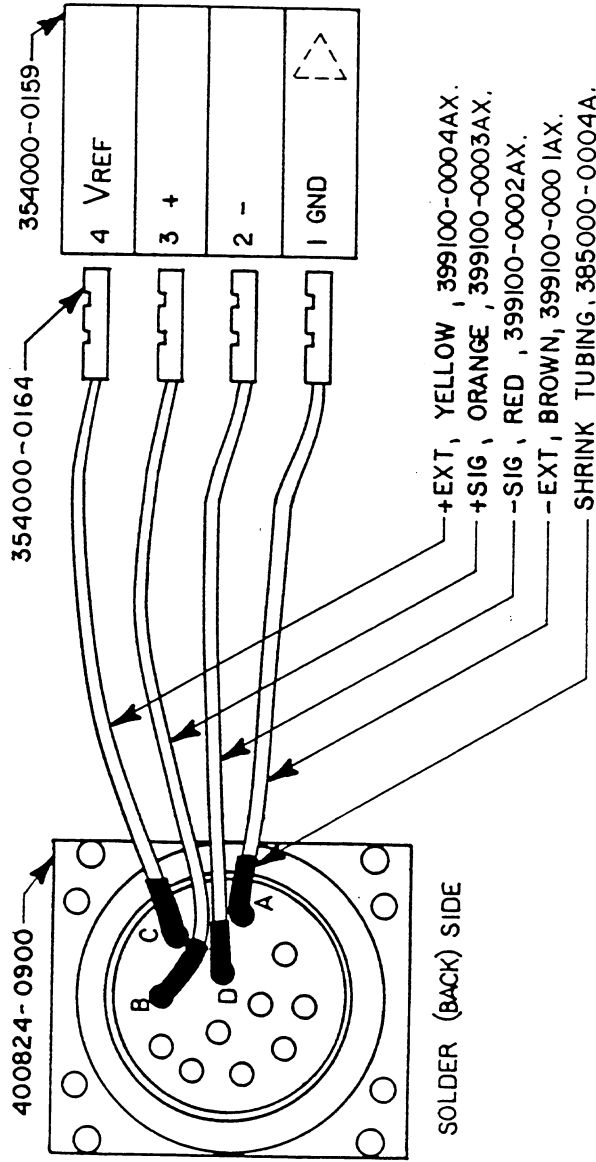

REV:A


TOLERANCES UNLESS OTHERWISE SPECIFIED		MEDICAL DATA ELECTRONICS	
FRACTIONS	DEC	ANGLES	
±	±	±	
APPROVALS	DATE	SCALE	DRAWING NO.
DAVIS	11/18/88	NONE	B 400819
CHECKED		DO NOT SCALE	DRAWING
			SHEET 1 OF 1

2: TRIM OFF NARROW END OF PINS ON NO. 354000-0176.
 1: ALL WIRE LENGTHS ARE 2.0 INCHES.

NOTES:

REVISIONS


LTR	DESCRIPTION	DATE	APPROVED
A	INITIAL RELEASE	12-14-87	

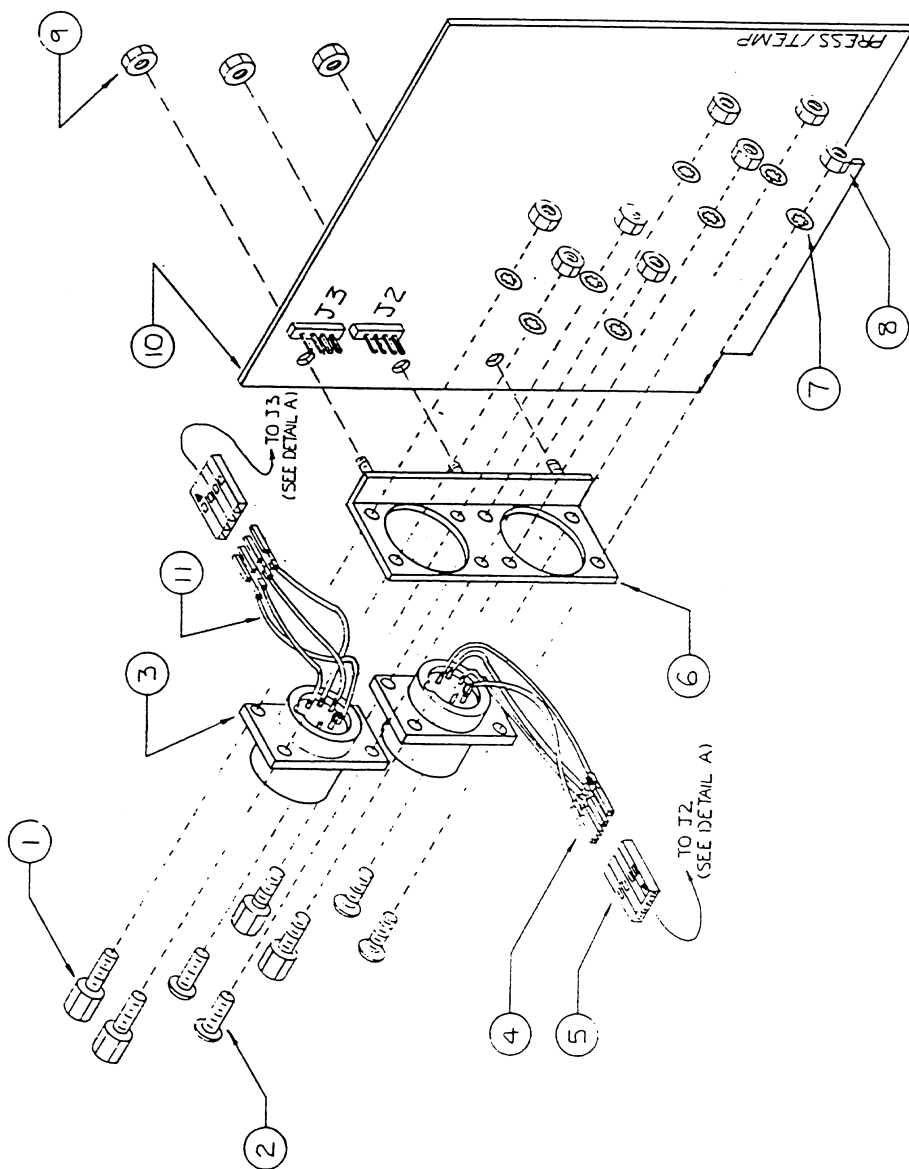

TOP VIEW

FRONT VIEW

NOTES: 1.



NO.	QTY.	DESCRIPTION	PART NO.
11	2	WHITE WIRE 24 GA STRANDED	399100-0009
10	1	PRESSURE/TEMP PCB A	400613-0000
9	3	#4 LOCK NUT THIN PATTERN	360500-0043
8	8	HEX NUT 2-56	360500-0020
7	8	#2 STAR WASHER	358200-0020
6	1	PRESSURE TEMP HSKT.	400578-0000
5	2	CONN. HOUSING 4 F	359000-0159
4	8	CRIMP PINS	354000-0160
3	2	PRESSURE CONNECTOR FAB	400665-0000
2	4	SCREW 2-56 X 3/8 PHILLIP	358100-0044
1	4	STANDOFF 2-56 X .187	360500-0020

TOLERANCES UNLESS
SPECIFIED
FRACTIONS DEC ANGLES

MEDICAL
DATA
ELECTRONICS

PRESS &/OR TEMP.
OPTION ASSY.

SCALE
FULL C 400587-0000

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400613-0000 PCBA, PRESS/TEMP, REV.'S' (E787) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
400612-0000	*1	1	PCB, PRESSURE/TEMP., REVISION 'P'	R		33	1.0	EA		Yes	
352300-0012A	*1	2	CAP, .01UF,10%,MYLAR	R		77	2.0	EA	C7,15	Yes	
352301-0105A	*1	4	CAP, 1UF,63V,20%,MYLAR	R		22	2.0	EA	C46,47	Yes	
352301-0104A	*1	5	CAP, .1UF,5%,MYLAR	R		66	4.0	EA	C19-22	Yes	
352300-0017A	*1	6	CAP, .0047UF,10%,MYLAR	R		77	2.0	EA	C34,35	Yes	
352101-0330A	*1	7	CAP, 33PF,100V,5%,RAD,NPO	R		22	4.0	EA	C23,24,31,32	Yes	
352201-0337A	*1	8	CAP, 330UF,16V,ELEC,RAD	R		22	1.0	EA	C36	Yes	
352301-0103A	*1	9	CAP, .01UF,100V,20%,POLYC ARB,.2 L.S.	R		66	1.0	EA	C8	Yes	
352400-0105A	*1	10	CAP, 1UF,50V,20%,RAD,TANT , MAX. HT. .28; O.D. .16	R		11	2.0	EA	C11,6	Yes	
352401-0106A	*1	11	CAP, 10UF,35V,20%,RAD,TAN T	R		11	6.0	EA	C1,2,12,13,16,29	Yes	
352400-0226A	*1	12	CAP, 22UF,25V,20%,TANT	R		11	2.0	EA	C9,10	Yes	
356000-0008A	*1	14	REF OSCILLATOR, CMOS 4.0M HZ,HIGH SPEED	R		22	1.0	EA	Y1	Yes	
364000-0010A	*1	15	IC, LM339	R		11	1.0	EA	U13	Yes	
364000-0027A	*1	16	IC, 74HC32	R		11	2.0	EA	U8,9	Yes	
364000-0029A	*1	17	IC, 74HC138	R		11	1.0	EA	U4	Yes	
364000-0038A	*1	18	IC, 27C256,CMOS,EPROM,200 NS	R		11	1.0	EA	U2	Yes	
364000-0040A	*1	19	IC, 4051	R		11	2.0	EA	U11,14	Yes	
364000-0065A	*1	20	IC, OP11FP,OP AMP	R		11	2.0	EA	U10,12	Yes	
364000-0080A	*1	21	IC, TMPZ84COOP (Z80A, CMOS VERSION)	R		11	1.0	EA	U1	Yes	
364000-0091A	*1	22	IC, SG 3525	R		44	1.0	EA	U15	Yes	
364000-0093A	*1	23	IC, ILQ5 QUAD OPTO ISOLAT OR	R		11	1.0	EA	U16	Yes	
364000-0095A	*1	24	IC, MS6132,DUAL PORT RAM, 8 X 2K,48-PIN (OR MS7132)	R		11	1.0	EA	U3	Yes	
364000-0096A	*1	25	IC, 74HC240	R		11	1.0	EA	U6	Yes	
364000-0097A	*1	26	IC, 74HC374	R		11	1.0	EA	U7	Yes	
364000-0098A	*1	27	IC, 82C54,CTC	R		11	1.0	EA	U5	Yes	

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400613-0000 PCBA, PRESS/TEMP, REV.'S' (E787) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
364000-0099A	*1	28	IC, 6N137	R		11	1.0	EA	U17	Yes	
370100-0010A	*1	29	RES, 1,1/4W,5%,CF	R		11	1.0	EA	R20	Yes	
370100-0101A	*1	30	RES, 100,1/4W,5%,CF	R		11	3.0	EA	R25,27,31	Yes	
370100-0102A	*1	31	RES, 1K,1/4W,5%,CF	R		11	1.0	EA	R15	Yes	
370100-0103A	*1	32	RES, 10K,1/4W,5%,CF	R		11	8.0	EA	R1,2,4-9	Yes	
370100-0103A	*1	33	RES, 10K,1/4W,5%,CF	R		11	3.0	EA	R22,38,45	Yes	
370100-0104A	*1	34	RES, 100K,1/4W,5%,CF	R		11	1.0	EA	R3	Yes	
370100-0106A	*1	35	RES, 10M,1/4W,5%,CF	R		11	2.0	EA	R23,24	Yes	
370100-0153A	*1	36	RES, 15K,1/4W,5%,CF	R		11	1.0	EA	R46	Yes	
370100-0202A	*1	37	RES, 2K,1/4W,5%,CF	R		11	1.0	EA	R26	Yes	
370100-0226A	*1	38	RES, 22M,1/4W,5%,CF	R		11	2.0	EA	R61,62	Yes	
370100-0622A	*1	39	RES, 6.2K,1/4W,5%,CF	R		11	1.0	EA	R21	Yes	
370100-0511A	*1	40	RES, 510,1/4W,5%,CF	R		11	4.0	EA	R11-14	Yes	
370100-0512A	*1	41	RES, 5.1K,1/4W,5%,CF	R		11	3.0	EA	R17-19	Yes	
370100-0331A	*1	42	RES, 330,1/4W,5%,CF	R		11	1.0	EA	R10	Yes	
370200-0200A	*1	43	RES, 20,1/4W,1%,MF	R		11	1.0	EA	R37	Yes	
370200-0100A	*1	44	RES, 10,1/4W,1%,MF	R		11	1.0	EA	R49	Yes	
370200-1001A	*1	45	RES, 1K,1/4W,1%,MF	R		11	3.0	EA	R40,59,60	Yes	
370200-1002A	*1	46	RES, 10K,1/4W,1%,MF	R		11	2.0	EA	R28,44	Yes	
370200-1003A	*1	47	RES, 100K,1/4W,1%,MF	R		11	2.0	EA	R50,54	Yes	
370200-1541A	*1	48	RES, 1.54K,1/4W,1%,MF	R		11	2.0	EA	R35,36	Yes	
370200-3010A	*1	49	RES, 301,1/4W,1%,MF	R		11	2.0	EA	R51,55	Yes	
370200-2001A	*1	50	RES, 2K,1/4W,1%,MF	R		11	3.0	EA	R33,34,41	Yes	
370200-2701A	*1	51	RES, 2.7K,1/4W,1%,MF	R		11	1.0	EA	R43	Yes	
370200-5901A	*1	52	RES, 5.9K,1/4W,1%,MF	R		11	1.0	EA	R48	Yes	

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400613-0000 PCBA, PRESS/TEMP, REV.'S' (K787) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
370200-6341A	*1	53	RES, 6.34K,1/4W,1%,MF	R		11	1.0	EA	R39	Yes	
370200-8061A	*1	54	RES, 8.06K,1/4W,1%,MF (8 .05K N/A :OK PER KR)	R		11	2.0	EA	R32,42	Yes	
370200-9091A	*1	55	RES, 9.09K,1/4W,1%,MF	R		11	3.0	EA	R16,53,57	Yes	
370200-9761A	*1	56	RES, 9.76K,1/4W,1%,MF	R		11	1.0	EA	R29	Yes	
374300-0202A	*1	57	POT, 2K,TRIM,SIDE ADJ,CER MET,3/8 SQR,.15LS	R		11	4.0	EA	R30,47,52,56	Yes	
376000-0003A	*1	58	ISTR, 2N3904	R		11	2.0	EA	Q1,2	Yes	
376000-0019A	*1	59	ISTR, 2N7000,PET	R		11	1.0	EA	Q3	Yes	
378000-0005A	*1	60	DIO, 1N914,SIGNAL	R		11	8.0	EA	D1-7,9	Yes	
378000-0012A	*1	61	DIO, 1N4749A,24V,ZENER ** *NOT ONLY**	R		11	5.0	EA	D10-14	Yes	
378000-0012A	*1	62	DIO, 1N4749A,24V,ZENER ** *NOT ONLY**	R		11	4.0	EA	D15-18	Yes	
378000-0034A	*1	63	DIO, 1N385,ZENER (ISTR NA TIONAL ONLY)	R		11	2.0	EA	D8,20	Yes	
382200-0005A	*1	64	CHOKE, 10UH,MOLDED	R		11	2.0	EA	L3,4	Yes	
382200-0018A	*1	65	CHOKE, 10,000UH MS75089-35	R		11	1.0	EA	L5	Yes	
382200-0015A	*1	66	CHOKE, 680 UH	R		11	4.0	EA	L1,2,6,7	Yes	
352300-0007A	*1	67	CAP, .001UF,10%, MYLAR	R		66	3.0	EA	C4,5,14	Yes	
365000-0016A	*1	70	SKT, 16-POS,DIP,TIN PLATE ,L.P.	R		11	2.0	EA	U11,14	Yes	
365000-0028A	*1	73	SKT, 28-POS,DIP,TIN PLATE ,L.P.	R		11	1.0	EA	U2	Yes	
360500-0045A	*1	76	SPCR, #6 X 1.437 X 1/4,RO UND	R		22	1.0	EA		Yes	
400552-0000	*1	77	ESCORT II ISO-TRANSFORMER , REV. 'A' ** (FIFO)**	R		22	1.0	EA	T1	Yes	
354000-0103A	*1	78	CONN, SGL ROW,STRT,SGL PI NS,SNAP-AWAY	R		11	8.0	PIN	2 PCS. OF 4 PINS EACH	Yes	
354000-0103A	*1	79	CONN, SGL ROW,STRT,SGL PI NS,SNAP-AWAY	R		11	4.0	PIN	2 PCS. OF 2 PINS EACH	Yes	
352300-0104A	*1	80	CAP, .1UF,50V,20%,RAD,MYL AR	R		22	4.0	EA	C30,25,26,27	Yes	
352300-0104A	*1	81	CAP, .1UF,50V,20%,RAD,MYL AR	R		22	5.0	EA	C28,37,38,44,45	Yes	
352300-0104A	*1	82	CAP, .1UF,50V,20%,RAD,MYL AR	R		22	4.0	EA	C40,41,42,43	Yes	
352100-0104A	*1	83	CAP, .1UF,50V,10%,RAD,X7R	R		11	1.0	EA	C39	Yes	

MC Software, Inc.
BREP14

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400613-0000 PCBA, PRESS/TEMP, REV.'S' (E787) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
365000-0040A	*1	84	SKT, 40-POS,DIP,TIN PLATE ,L.P.	R		11	1.0	EA	U1		Yes
365000-0024A	*1	85	SKT, 24-POS,DIP,TIN PLATE ,L.P.	R		11	1.0	EA	U5		Yes
384000-0061A	*1	86	GAS TUBE (SURGE ARRESTER)	R		33	1.0	EA	DS1		Yes
365000-0148A	*1	87	SOCKET, 48 PIN DIP	R		22	1.0	EA	U3		Yes

Cumulative Lead Time for 400613-0000 = 77

NIBP BOARD

CHAPTER 6

6.0.0 NIBP

6.1.0 OVERVIEW

The NIBP option is separated into three major sections: Pneumatic, digital and analog. Included in the pneumatic section are: The pump itself, manifold, valve, check valve, and the interconnecting plumbing. The digital portion includes: EPROM, Dual Port RAM, and other circuitry for processing digital data. The analog section includes: The transducer, fail detect, AC and DC channels, reference voltage generation, A to D conversion, and pump and valve ON/OFF control.

6.1.1 AC/DC CHANNELS

The **ESCORT 300A** uses a two lumen hose to inflate and deflate the cuff. Cuff pressure is sensed through this hose. The DC channel represents actual cuff pressure. The AC element is used to calculate the systolic, mean, and diastolic values.

6.1.2 OVERPRESSURE PROTECTION AND DETECTION

There are three methods of overpressure detection to protect the patient from sustained or excessive cuff inflation. They are: 1) software, 2) hardware and 3) mechanical. The first method is software controlled. The algorithm checks cuff pressure every 4mS looking for a reading of over 240mmHg. If it reads a pressure higher than 240mmHg, the pump and valve will be turned off by the signals PUMP ON and VALVE ON. The cuff is deflated until pressure is below 240mmHg. The monitor will also display the message NIBP ERROR MAX LIMIT on the channel message line. The second method relies on analog hardware. A comparator detects cuff pressure over 275mmHg and turns the pump and valve off by the signal FAIL-INT, deflating the cuff completely. The channel message line will display NIBP FAIL MAX LIMIT. The third method is mechanical. A pressure switch, located in the pneumatics section, senses any pressure over 320mmHg. This switch will interrupt +V to the pump and valve, turning them off and deflating the cuff. No message is associated with this overpressure condition.

6.1.3 BLOOD PRESSURE OR TEMPERATURE OPTIONS

A Daughter Board is installed onto the NIBP option if invasive pressure or temperature options have been selected. The invasive pressure and temperature circuits are functionally identical to the circuits on the Pressure Temperature Board, P/N 400613. Please refer to section 5.0.0 for the Theory of Operation.

6.2.0 INPUT CIRCUIT

The transducer used in the NIBP option uses a +5VDC excitation and has internal amplification for an approximate output of 1V = 100mmHg at pin 2. R11 and R58 are to adjust gain and offset errors for a true reading of 1V = 100mmHg at U2 pin 8. This signal becomes the DC channel and is the input to the AC channel, the low pressure comparator and the high pressure comparator.

6.2.1 AC CHANNEL

The AC channel strips off the DC component with C9 and C18. U4 provides amplification for the AC signal.

BASELINE RESET resets the AC channel quickly in the event the signal is saturated: U7A discharges C9 by bringing U4 pin 8 to ground; U7B discharges C18.

The AC channel then goes into a gain stage that is software controlled. The signals 200N and 400N place R44 and R45 in parallel with R43, selecting one of 4 possible levels for U43.

The next stage biases the signal to half of the A to D converter's full scale. U4A uses a 1.25V reference to scale up the AC channel so the A to D converter can read both negative and positive signals. U10 selects either the AC or DC channel and converts it to a digital format. The A to D converter uses the 2.5 REF signal to set the scale. ADC DONE is a data available signal signifying that the conversion is complete.

6.2.2 VALVE AND PUMP CONTROL

The signal PUMP-ON is gated together with the signals FAIL-INT and RESET to drive Q2. Q2 turns the pump on by grounding its negative lead. The normally open valve is controlled by the signal VALVE ON which is also gated with FAIL-INT and RESET to drive Q1. When VALVE ON is low, the valve is open, releasing air out of the cuff. FAIL-INT or RESET inhibit the valve and pump. FAIL-INT occurs during any failure, and RESET is active during power up.

When cuff pressure exceeds 320mmHg $\pm$ 15mmHg, the overpressure switch interrupts +Vin, disabling the pump and valve.

6.2.3 FAIL DETECT

U6 and U2 comprise the Fail Detect circuit. U2A compares the DC pressure signal to a 31mmHg reference. The timer, U6, will time out after 5 minutes if not reset by the cuff pressure going below 31mmHg. If the timer does time out, the signal FAIL 5 - MINUTES will

be active. U2 compares 275mmHg with the DC pressure signal for overpressure. If cuff pressure exceeds 275mmHg, the signal FAIL OVER-PRESS will be active. Either signal will produce the FAIL-INT signal, turning off the pump and valve, and will go on to the Digital Section.

6.2.4 REFERENCE VOLTAGE

Reference Voltages are generated from +15V. The 2.5V zener reference diode, U20, generates the signal 2.5 REF. U2 pin 14 generates 5.0 REF. R6 and R7 form a voltage divider for the 1.25 REF signal.

6.3.0 DIGITAL

The digital section processes data and interfaces signals to and from the NIBP analog section, Blood Pressure or Temperature Daughter Boards, and the CPU Board. A Z-80 type microprocessor is clocked by a 4MHz crystal. RST OUT* from the CPU Board resets U11. TIME TIC* coordinates the fetching of data points. The ROM, U15, holds the microprocessor's program. U17 is an address decoder that decodes address BUS data to enable U15 or U18. U18, a dual Port RAM, passes data to and from the CPU Board. U12 and U13 are input and output ports. U12 outputs signals to the NIBP analog and invasive pressure or temperature sections. U13 receives signals from the NIBP analog section. U19 interfaces with the Invasive Pressure or Temperature Daughter Boards. J2 goes to the Daughter Board (Invasive Pressure or Temperature).

6.4.0 CALIBRATION CHECK PROCEDURE

Calibration of the monitor should be checked at least once a month or where there is doubt about the validity of the pressure readings. The test procedure is designed to confirm accuracy of the monitor as well as to diagnose pneumatic leaks.

CAUTION: Calibration tubing should always be kept dry and free of particulate matter. Moisture or foreign substances introduced into the pneumatic system can cause damage to the unit.

To perform a calibration check, follow these steps:

1. Obtain the calibration kit supplied with the unit.
2. Connect a mercury manometer to the monitor using the parts supplied with the calibration kit.

3. Press the NIBP TEST key and select CAL. Press PAGE HOME.
The following is displayed in trace 2 message field:
CAL NIBP
CUFF=XXX
4. Open manometer to air and verify the offset CUFF-XXX is between -3 and +10mmHg.
5. Using the inflation bulb, manually pump up the pressure to 100mmHg; monitor should read CUFF-XXX 100mmHg plus offset, ± 4 mmHg.
6. Using the inflation bulb, manually pump up the pressure to 200mmHg; monitor should read CUFF-XXX 200mmHg plus offset, ± 5 mmHg.
7. If indicated pressures are not within tolerance, the monitor must be calibrated. Refer to qualified service personnel.

NOTE

The ESCORT 300A also includes a backup automatic safety valve which, in the event of system failure, will automatically deflate the cuff if pressure exceeds 320mmHg.

6.4.1 LEAK TEST PROCEDURE

If a leak is suspected, use the cuff and hose in question.


1. Cuff should be wrapped tightly on itself.
2. Select the LEAK position of the NIBP TEST key.
3. Press NIBP key followed by the START key.
4. ESCORT 300A will inflate cuff and automatically check for a leak. If no leak is detected, a NO LEAK message is displayed. If a leak is detected, a LEAK message is displayed. If a leak is detected, replace or repair leak in cuff/hose before using to monitor a patient.
5. To exit the LEAK test mode, press STOP key.

6.4.2 OSCILLATION WAVEFORM RECORDING

If the ESCORT is configured with a recorder, the oscillation waveform can be recorded. The oscillation waveform can be recorded in the TEST mode. To record the waveform:


1. Select the WAVE position of the NIBP TEST key.
2. Press PAGE HOME followed by the NIBP setup key.
3. The oscillation waveform will automatically record for each determination.
4. To exit the waveform test mode, select the OFF position of the NIBP TEST key.

REV	DESCRIPTION	DATE	APPROVED

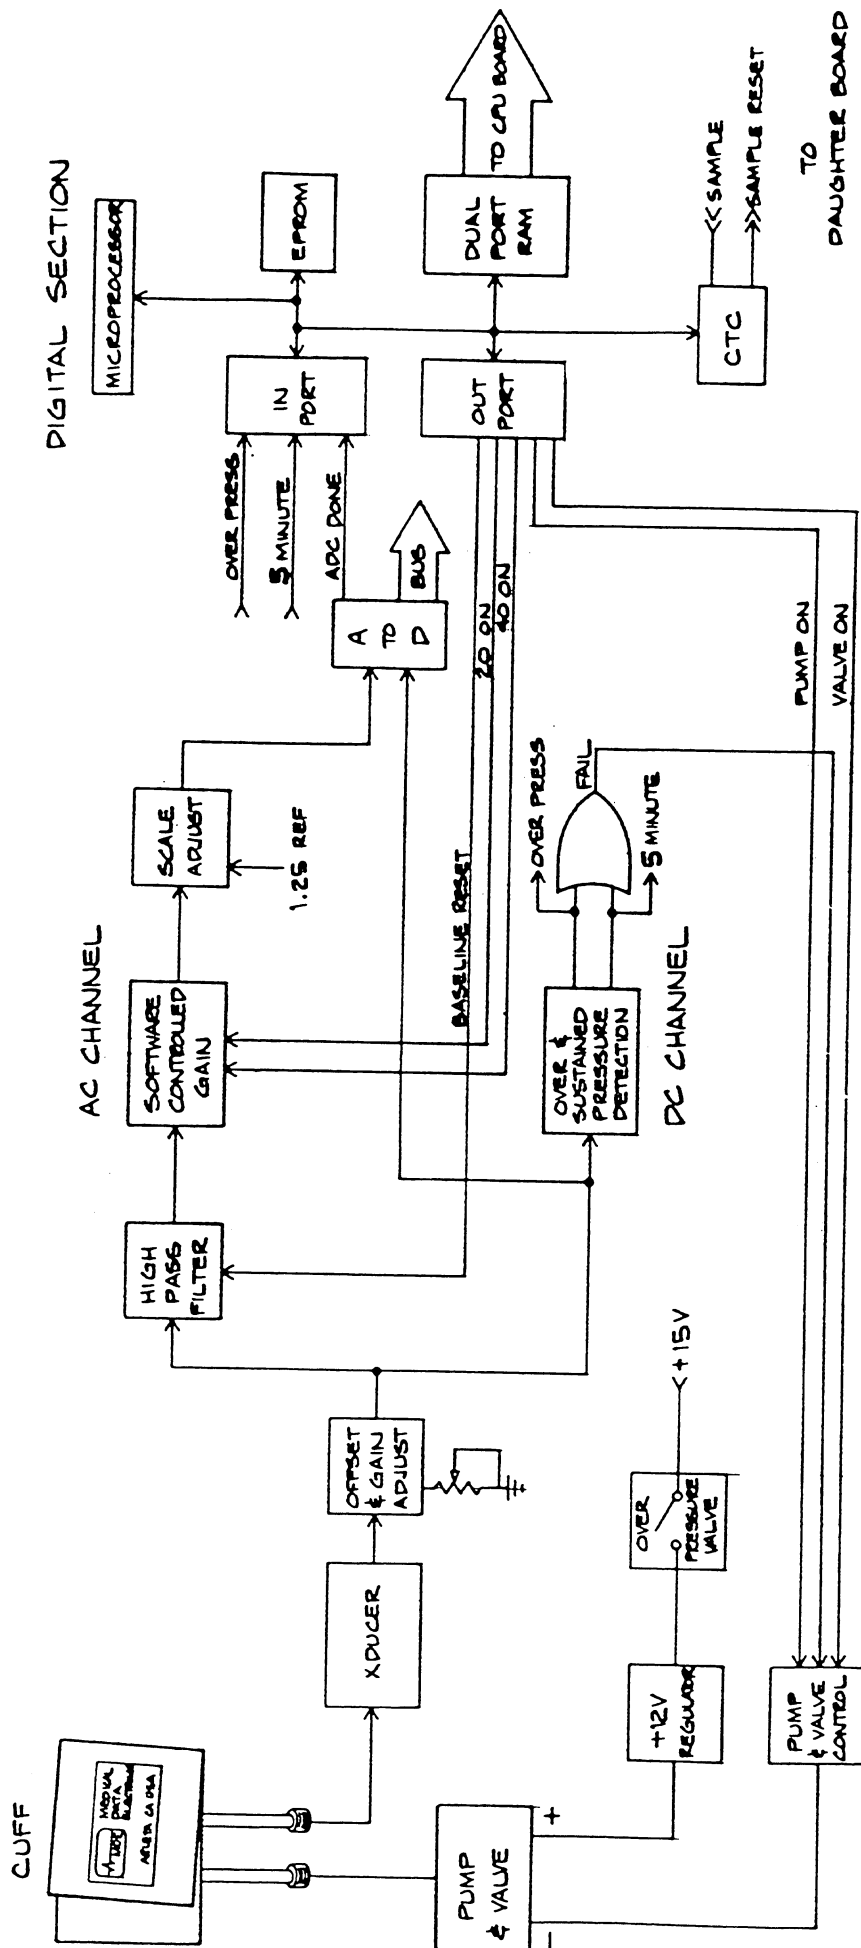


DESIGNED BY	DATE
APPROVED BY	DATE
FUNCTIONAL SPEC	DATE
REVISION	DATE

NIBP BLOCK DIAGRAM	
SCALE	NONE
SET	C
DO NOT SCALE DRAWING	SHEET 1 OF 1

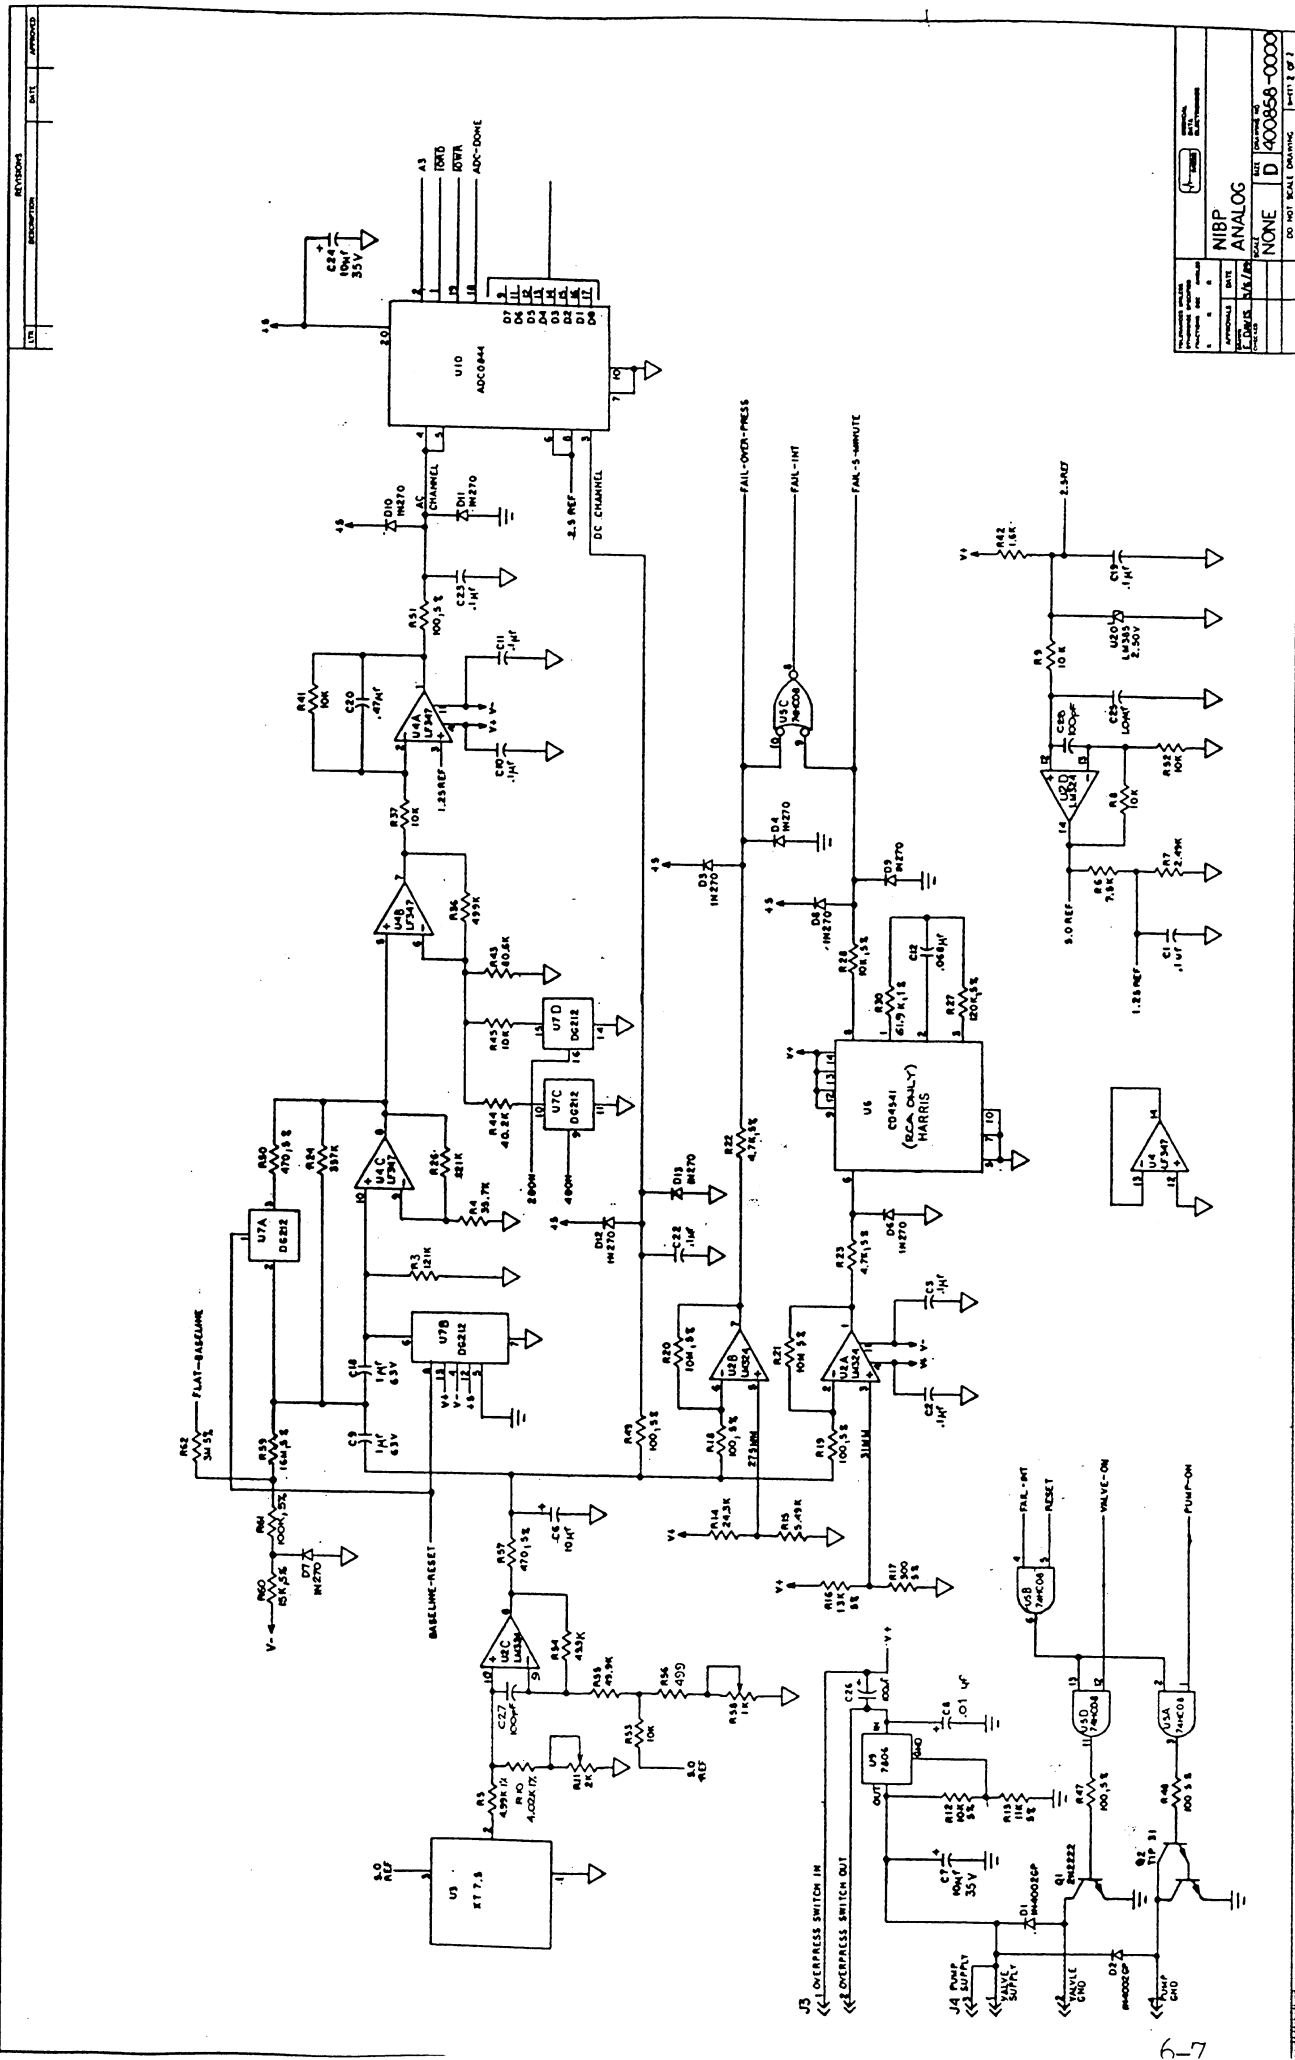


LAST USED	
C2D	J4 U20
D13	Q2 Y1
	M63

NOT USED	
C4, 9, 15, 21	U1, 8, D5
R1, 2, 29, 35, 38, 39, 40, 46	



APPROVALS DATE 3/3/89 DAYS 14	NIBP DIGITAL SCALE NONE	DO NOT SCALE

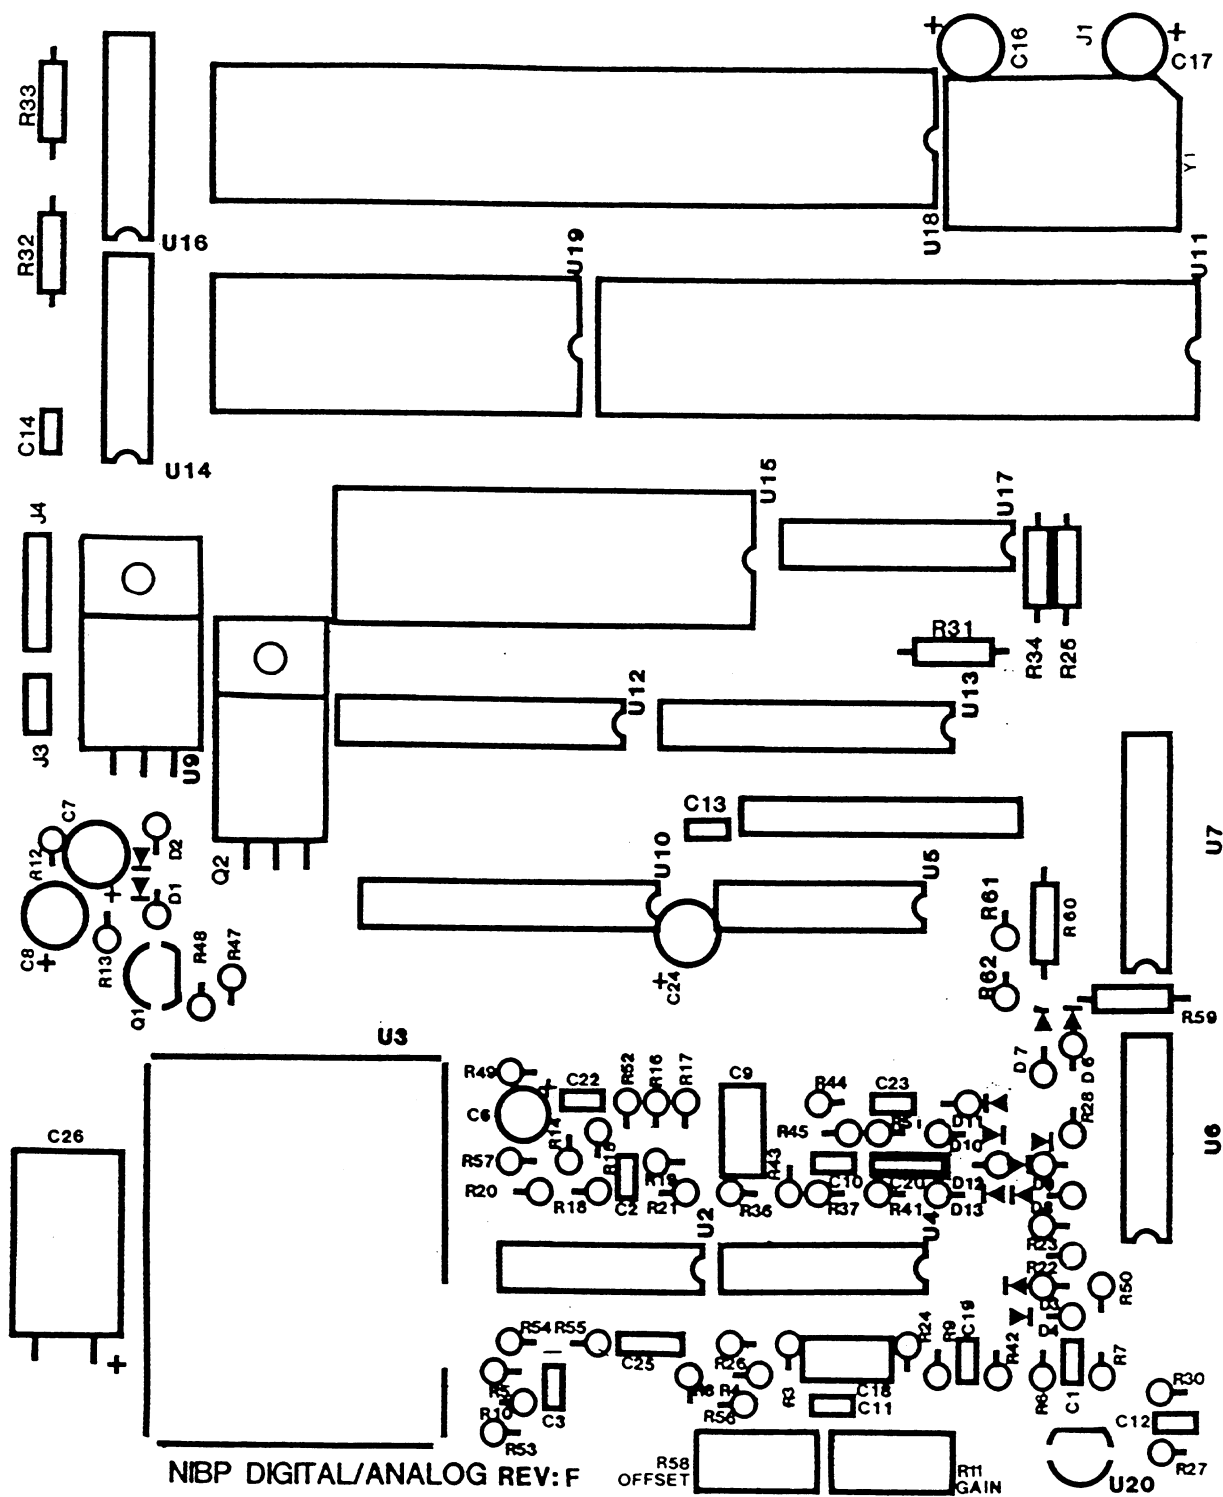

NIBP DIGITAL/ANALOG BOARD

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400858-0000 PCBA, NIBP, REV. "S" (E793) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
400857-0000	*1	1	PCB, NIBP, REVISION "G"	R		33	1.0	EA		Yes	
352100-0474A	*1	2	CAP, .47UF,50V,10%,RAD,X7R	R		22	1.0	EA	C20	Yes	
352100-0104A	*1	3	CAP, .1UF,50V,10%,RAD,X7R	R		11	1.0	EA	C13	Yes	
352300-0020A	*1	4	CAP., 1UF,63V,5%,MYLAR	R		77	2.0	EA	C9,18	Yes	
352300-0021A	*1	5	CAP., .068UF,50V,10%,MYLAR	R		66	1.0	EA	C12	Yes	
352300-0104A	*1	6	CAP, .1UF,50V,20%,RAD,MYLAR	R		22	7.0	EA	C1,2,3,10,11,14,19	Yes	
352300-0104A	*1	7	CAP, .1UF,50V,20%,RAD,MYLAR	R		22	2.0	EA	C22,23	Yes	
352300-0008A	*1	8	CAP, .01UF,5%,MYLAR	R		66	1.0	EA	C8	Yes	
352401-0106A	*1	9	CAP, 10UF,35V,20%,RAD,TANT	R		11	5.0	EA	C6,7,16,17,24	Yes	
356000-0008A	*1	10	REF OSCILLATOR, CMOS 4.0MHZ,HIGH SPEED	R		22	1.0	EA	Y1	Yes	
354000-0188A	*1	11	CONN, FEMALE, SNAP-AWAY, 20 PIN STRIP,INTERCONNECT	R		11	9.0	EA	J2 (CUT TO 9 PINS)	Yes	
364000-0008A	*1	12	IC, DG212CJ	R		11	1.0	EA	U7	Yes	
364000-0026A	*1	13	IC, 74HC08	R		11	1.0	EA	U5	Yes	
364000-0027A	*1	14	IC, 74HC32	R		11	2.0	EA	U14,16	Yes	
364000-0029A	*1	15	IC, 74HC138	R		11	1.0	EA	U17	Yes	
364000-0036A	*1	16	IC, 7806	R		11	1.0	EA	U9	Yes	
364000-0038A	*1	17	IC, 27C256,CMOS,EPROM,200NS	R		11	1.0	EA	U15	Yes	
364000-0057A	*1	18	IC, LM324, LINEAR	R		11	1.0	EA	U2	Yes	
364000-0080A	*1	19	IC, TMPZ84C00P (Z80A, CMOS VERSION)	R		11	1.0	EA	U11	Yes	
364000-0095A	*1	20	IC, MS6132,DUAL PORT RAM, 8 X 2K,48-PIN (OR MS7132)	R		11	1.0	EA	U18	Yes	
364000-0096A	*1	21	IC, 74HC240	R		11	1.0	EA	U13	Yes	
364000-0097A	*1	22	IC, 74HC374	R		11	1.0	EA	U12	Yes	
364000-0130A	*1	23	IC, LF347 (SCREENED TO +/- 1.5mV), NATIONAL ONLY	R		22	1.0	EA	U4	Yes	
384000-0067A	*1	24	PRESSURE TRANSDUCER XT7.5	R		22	1.0	EA	U3	Yes	
364000-0127A	*1	25	IC, CD4541 **RCA (HARRIS) ONLY**	R		22	1.0	EA	U6	Yes	

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400858-0000 PCBA, NIBP, REV. "S" (E793) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
364000-0128A	*1	26	IC, ADC844	R		22	1.0	EA	U10		Yes
370100-0101A	*1	27	RES, 100,1/4W,5%,CF	R		11	6.0	EA	R47,48,49,51,18,19		Yes
370100-0103A	*1	28	RES, 10K,1/4W,5%,CF	R		11	7.0	EA	R12,28,31,32,33,34,63		Yes
370100-0104A	*1	29	RES, 100K,1/4W,5%,CF	R		11	2.0	EA	R25,61		Yes
370100-0106A	*1	30	RES, 10M,1/4W,5%,CF	R		11	2.0	EA	R20,21		Yes
370100-0113A	*1	31	RES, 11K,1/4W,5%,CF	R		11	1.0	EA	R13		Yes
370100-0124A	*1	32	RES, 120K,1/4W,5%,CF	R		11	1.0	EA	R27		Yes
370100-0133A	*1	33	RES, 13K,1/4W,5%,CF	R		11	1.0	EA	R16		Yes
370100-0162A	*1	34	RES, 1.6K,1/4W,5%,CF	R		11	1.0	EA	R42		Yes
370100-0301A	*1	36	RES, 300,1/4W,5%,CF	R		11	1.0	EA	R17		Yes
370100-0471A	*1	37	RES, 470,1/4W,5%,CF	R		11	2.0	EA	R50,57		Yes
370100-0472A	*1	38	RES, 4.7K,1/4W,5%,CF	R		11	2.0	EA	R22,23		Yes
370200-6192A	*1	39	RES, 61.9K,1/4W,1%,MF	R		11	1.0	EA	R30		Yes
370200-1002A	*1	40	RES, 10K,1/4W,1%,MF	R		11	7.0	EA	R8,9,37,41,45,52,53		Yes
370200-1213A	*1	41	RES, 121K,1/4W,1%,MF	R		11	2.0	EA	R3,26		Yes
370200-2432A	*1	42	RES, 24.3K,1/4W,1%,MF	R		11	1.0	EA	R14		Yes
370200-2491A	*1	43	RES, 2.49K,1/4W,1%,MF	R		11	1.0	EA	R7		Yes
370200-3572A	*1	44	RES, 35.7K,1/4W,1%,MF	R		11	1.0	EA	R4		Yes
370200-3573A	*1	45	RES, 357K,1/4W,1%,MF	R		11	1.0	EA	R24		Yes
370200-4022A	*1	46	RES, 40.2K,1/4W,1%,MF	R		11	1.0	EA	R44		Yes
370200-4990A	*1	47	RES, 499,1/4W,1%,MF	R		11	1.0	EA	R56		Yes
370200-4992A	*1	48	RES, 49.9K,1/4W,1%,MF	R		11	2.0	EA	R54,55		Yes
370200-4993A	*1	49	RES, 499K,1/4W,1%,MF	R		11	1.0	EA	R36		Yes
370200-5491A	*1	50	RES, 5.49K,1/4W,1%,MF	R		11	1.0	EA	R15		Yes
370200-7501A	*1	51	RES, 7.5K,1/4W,1%,MF	R		11	1.0	EA	R6		Yes

Assembly	Description	Group	PFC	Commodity	Class	Planner	Buyer	Drawing			
400858-0000	PCBA, NIBP, REV. "S" (E793)				A						
ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
370200-8062A	*1	52	RES, 80.6K,1/4W,1%,MF	R		11	1.0	EA	R43	Yes	
370200-4021A	*1	53	RES, 4.02K,1/4W,1%,MF	R		11	1.0	EA	R10	Yes	
374300-0102A	*1	54	POT, 1K,TRIM,SIDE ADJ,CER MET,3/8 IN.QR,.15LS	R		11	1.0	EA	R58	Yes	
374300-0202A	*1	55	POT, 2K,TRIM,SIDE ADJ,CER MET,3/8 SQR,.15LS	R		11	1.0	EA	R11	Yes	
376000-0007A	*1	56	XSTR, TIP31	R		11	1.0	EA	Q2	Yes	
376000-0013A	*1	57	XSTR, PN2222,PLASTIC	R		11	1.0	EA	Q1	Yes	
378000-0001A	*1	58	DIO, 1N270	R		11	6.0	EA	D3,4,8,9,10,11,	Yes	
378000-0001A	*1	59	DIO, 1N270	R		11	4.0	EA	D12,13,6,7	Yes	
378000-0002A	*1	60	DIO, 1N4002GP,RCFTR, (MOT ONLY)	R		11	2.0	EA	D1,2	Yes	
378000-0034A	*1	61	DIO, LM385,ZENER (XSTR NA TIONAL ONLY)	R		11	1.0	EA	U20	Yes	
354000-0138A	*1	62	CONN, 2-P,M,STRT LOCK,.1 CTR,HDR	R		11	1.0	EA	J3	Yes	
354000-0148A	*1	63	CONN, 4-P,M,STRT,.1 CTR,L OCKING RAMP	R		11	1.0	EA	J4	Yes	
358100-0064A	*1	64	SCR, 4-24 X 3/8 ,PH.PNHD. ,SELF-TAP	R		11	2.0	EA	USED ON TRANSDUCER	Yes	
370100-0166A	*1	66	RES, 16K,1/4W,5%,CF	R		11	1.0	EA	R59	Yes	
370100-0153A	*1	67	RES, 15K,1/4W,5%,CF	R		11	1.0	EA	R60	Yes	
352400-0105A	*1	68	CAP, 1UF,50V,20%,RAD,TANT , MAX: HT. .28; O.D. .16	R		11	1.0	EA	C25	Yes	
365000-0014A	*1	69	SKT, 14-POS,DIP,TIN PLATE ,L.P.	R		11	3.0	EA	U2,4,6	Yes	
365000-0024A	*1	72	SKT, 24-POS,DIP,TIN PLATE ,L.P.	R		11	1.0	EA	U19	Yes	
365000-0228A	*1	73	SKT, 28-POS,LOW PROFILE,G OLD CNTCT W/TIN SHELL	R		22	1.0	EA	U15	Yes	
365000-0040A	*1	74	SKT, 40-POS,DIP,TIN PLATE ,L.P.	R		11	1.0	EA	U11	Yes	
360500-0062A	*1	75	STD OFF, #6,ALUM,1/4 RND X 1.375 LGTH	R		11	1.0	EA		Yes	
400712-0000	*1	76	FISH PAPER FAB, 23.26SQ"/ PC.(4.125" X 5.125")REV B	A		0	1.0	EA		Yes	
352200-0107A	*1	77	CAP, 100UF,50V,RAD,ELECT, LS TYPE	R		22	1.0	EA	C26	Yes	
370200-4991A	*1	78	RES, 4.99K,1/4W,1%,MF	R		11	1.0	EA	R5	Yes	
370100-0305A	*1	79	RES, 3K,1/4W,5%,CF	R		11	1.0	EA	R62	Yes	


Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400858-0000 PCBA, NIBP, REV. "S" (E793) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
352100-0101A	*1	80	CAP, 100PF, 25V, 10%, RAD, NP O	R		11	2.0	EA	C27,28	Yes	
100000	*1	84	NOTES & SPEC. INSTRUCTION S	P		0	0.0	EA	APPLY FOIL TAPE TO	Yes	
100000	*1	85	NOTES & SPEC. INSTRUCTION S	P		0	0.0	EA	BACK OF 384000-0067A	Yes	
100000	*1	86	NOTES & SPEC. INSTRUCTION S	P		0	0.0	EA	NIBP TRANSDUCER	Yes	
365000-0148A	*1	87	SOCKET, 48 PIN DIP	R		22	1.0	EA	U18	Yes	


Cumulative Lead Time for 400858-0000 = 77

REV	DESCRIPTION	DATE
1	INITIAL RELEASE	1/27/89
2	ECO 345	2/20/89
3	ECO 345	2/20/89
4	ECO 345	2/20/89
5	ECO 412	2/20/89
6	ECO 412	2/20/89
7	ECO 412	2/20/89
8	ECO 412	2/20/89
9	ECO 412	2/20/89
10	ECO 412	2/20/89
11	ECO 412	2/20/89
12	ECO 412	2/20/89
13	ECO 412	2/20/89
14	ECO 412	2/20/89
15	ECO 412	2/20/89
16	ECO 412	2/20/89
17	ECO 412	2/20/89
18	ECO 412	2/20/89
19	ECO 412	2/20/89
20	ECO 412	2/20/89

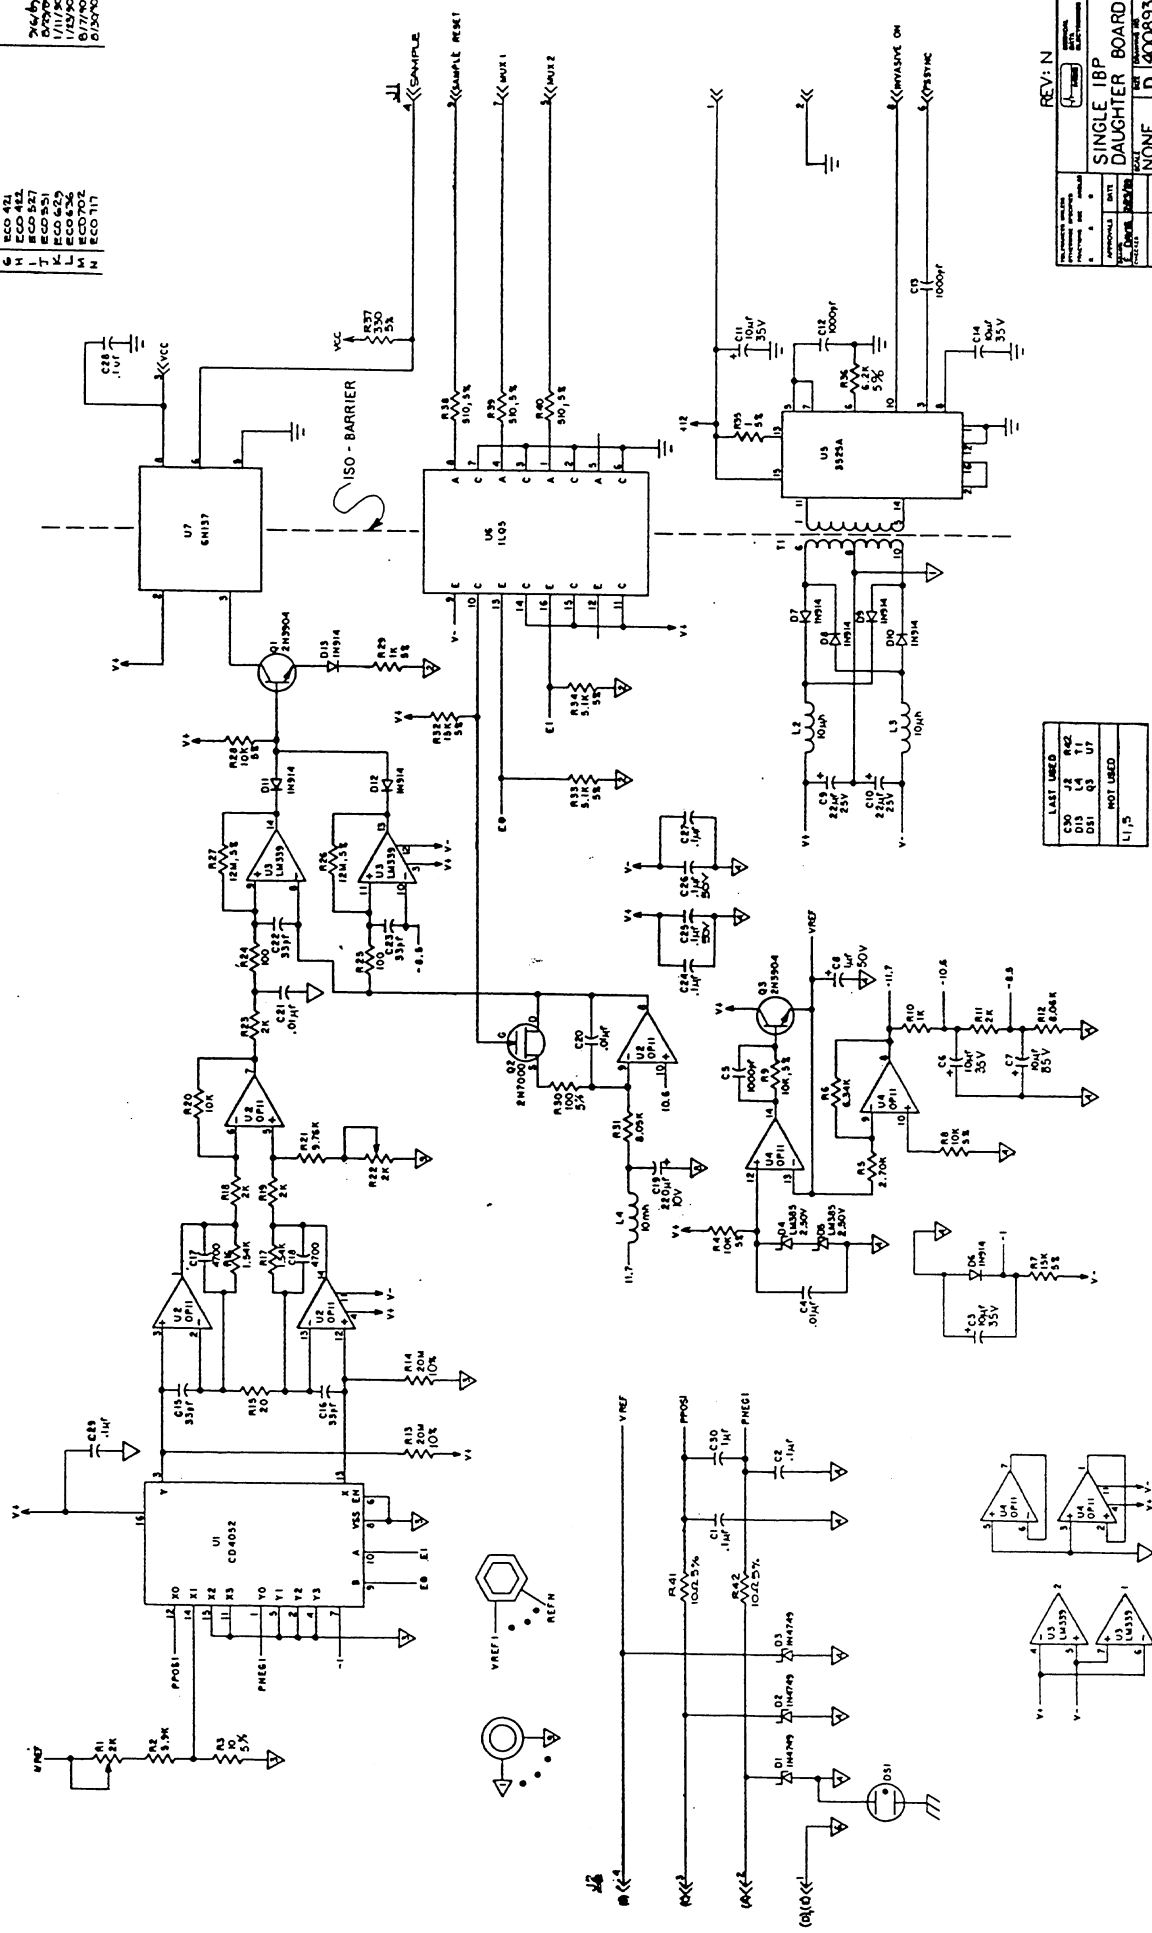

LAST USED	
C30	J2
D15	L4
D31	Q1
L1,5	U1

REV: N	
DATE	1/27/89
BY	W. J. B. / J. B. B.
DESCRIPTION	SINGLE 18P DAUGHTER BOARD
QTY	NONE
QTY	D 400893-0000
DO NOT SCALE DRAWING	PRINTED 1

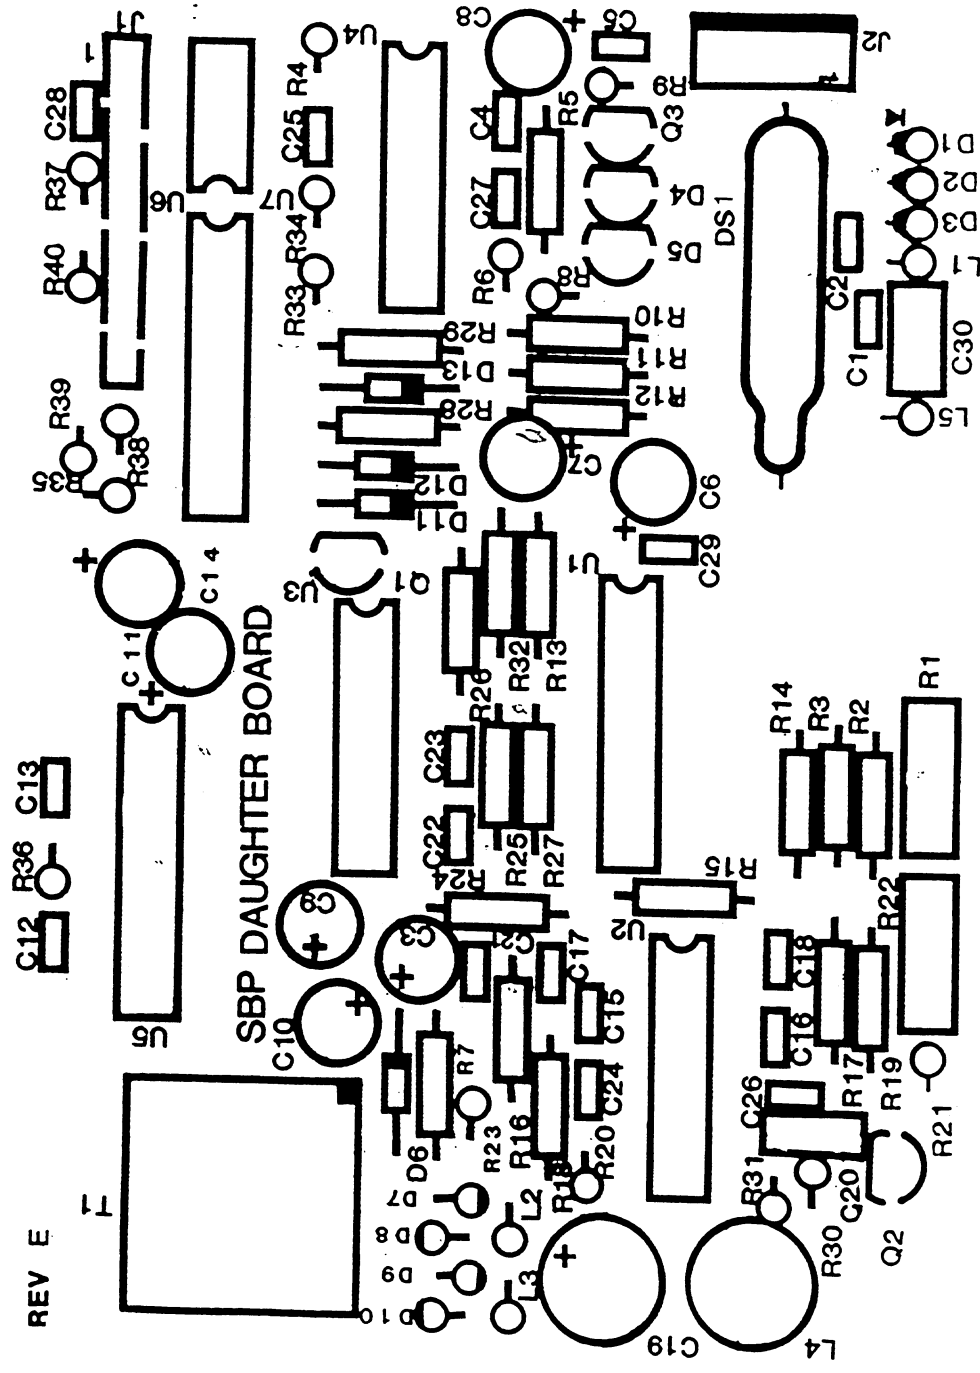

SBP DAUGHTER BOARD

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400893-0000 PCBA, SINGLE IBP DAUGHTER BOARD, REVISION "N" A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
400894-0000	*1	1	PCB, SINGLE IBP DAUGHTER BD., REVISION 'G'	R		33	1.0	EA	USE UP REV F PCB'S	Yes	
352100-0102A	*1	2	CAP, 1000PF, 50V, 10%, RAD, X 7R	R		11	2.0	EA	C5,13	Yes	
352100-0103A	*1	3	CAP, .01UF, 50V, 10%, RAD, X7 R	R		11	2.0	EA	C4,21	Yes	
352100-0472A	*1	4	CAP, .0047UF, 25V, 10%, RAD, X7R	R		22	2.0	EA	C17,18	Yes	
352101-0330A	*1	5	CAP, 33PF, 100V, 5%, RAD, NPO	R		22	4.0	EA	C15,16,22,23	Yes	
352201-0227A	*1	6	CAP, 220UF, 10V, RAD, ELECT, .248 X .433 CS	R		66	1.0	EA	C19	Yes	
352301-0103A	*1	7	CAP, .01UF, 100V, 20%, POLYC ARB, .2 L.S.	R		66	1.0	EA	C20	Yes	
352301-0104A	*1	8	CAP, .1UF, 5%, MYLAR	R		66	5.0	EA	C1,2,24,27,28	Yes	
352301-0104A	*1	9	CAP, .1UF, 5%, MYLAR	R		66	1.0	EA	C29	Yes	
352301-0105A	*1	10	CAP, 1UF, 63V, 20%, MYLAR	R		22	1.0	EA	C30	Yes	
352400-0105A	*1	11	CAP, 1UF, 50V, 20%, RAD, TANT , MAX: HT. .28; O.D. .16	R		11	1.0	EA	C8	Yes	
352401-0106A	*1	12	CAP, 10UF, 35V, 20%, RAD, TAN T	R		11	5.0	EA	C3,6,7,11,14	Yes	
352400-0226A	*1	13	CAP, 22UF, 25V, 20%, TANT	R		11	2.0	EA	C9,10	Yes	
364000-0010A	*1	14	IC, LM339	R		11	1.0	EA	U3	Yes	
364000-0055A	*1	15	IC, CD4052	R		11	1.0	EA	U1	Yes	
364000-0065A	*1	16	IC, OP11FP, OP AMP	R		11	2.0	EA	U2,4	Yes	
378000-0034A	*1	17	DIO, LM385, ZENER (XSTR NA TIONAL ONLY)	R		11	2.0	EA	D4,5	Yes	
364000-0091A	*1	18	IC, SG 3525	R		44	1.0	EA	U5	Yes	
364000-0093A	*1	19	IC, ILQ5 QUAD OPTO ISOLAT OR	R		11	1.0	EA	U6	Yes	
364000-0099A	*1	21	IC, 6N137	R		11	1.0	EA	U7	Yes	
354000-0103A	*1	22	CONN, SGL ROW, STRT, SGL PI NS, SNAP-AWAY	R		11	1.0	PIN	J2	Yes	
354000-0187A	*1	23	CONN, MALE, SNAP-AWAY, 2 0 PIN STRIP, INTERCONNECT	R		11	9.0	EA	J1-MALE; 9 PIN = 1 PC	Yes	
370100-0010A	*1	24	RES, 1, 1/4W, 5%, CF	R		11	1.0	EA	R35	Yes	
370100-0101A	*1	26	RES, 100, 1/4W, 5%, CF	R		11	3.0	EA	R24,25,30	Yes	
370100-0102A	*1	27	RES, 1K, 1/4W, 5%, CF	R		11	1.0	EA	R29	Yes	

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400893-0000 PCBA, SINGLE IBP DAUGHTER BOARD, REVISION "N" A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
370100-0103A	*1	28	RES, 10K,1/4W,5%,CF	R		11	4.0	EA	R4,8,9,28	Yes	
370100-0126A	*1	29	RES, 12M,1/4W,5%,CF	R		11	2.0	EA	R26,27	Yes	
370100-0153A	*1	30	RES, 15K,1/4W,5%,CF	R		11	2.0	EA	R7,32	Yes	
370100-0206A	*1	31	RES, 20M,1/4W,10%,CF	R		11	2.0	EA	R13,14	Yes	
370100-0331A	*1	32	RES, 330,1/4W,5%,CF	R		11	1.0	EA	R37	Yes	
370100-0511A	*1	33	RES, 510,1/4W,5%,CF	R		11	3.0	EA	R38,39,40	Yes	
370100-0512A	*1	34	RES, 5.1K,1/4W,5%,CF	R		11	2.0	EA	R33,34	Yes	
370100-0622A	*1	35	RES, 6.2K,1/4W,5%,CF	R		11	1.0	EA	R36	Yes	
370200-0200A	*1	36	RES, 20,1/4W,1%,MF	R		11	1.0	EA	R15	Yes	
370200-1001A	*1	37	RES, 1K,1/4W,1%,MF	R		11	1.0	EA	R10	Yes	
370200-1002A	*1	38	RES, 10K,1/4W,1%,MF	R		11	1.0	EA	R20	Yes	
370200-1541A	*1	39	RES, 1.54K,1/4W,1%,MF	R		11	2.0	EA	R16,17	Yes	
370200-2001A	*1	40	RES, 2K,1/4W,1%,MF	R		11	4.0	EA	R11,18,19,23	Yes	
370200-2701A	*1	41	RES, 2.7K,1/4W,1%,MF	R		11	1.0	EA	R5	Yes	
370200-5901A	*1	42	RES, 5.9K,1/4W,1%,MF	R		11	1.0	EA	R2	Yes	
370200-6341A	*1	43	RES, 6.34K,1/4W,1%,MF	R		11	1.0	EA	R6	Yes	
370200-8061A	*1	44	RES, 8.06K,1/4W,1%,MF (8 .05K W/A :OK PER KR)	R		11	2.0	EA	R31,12	Yes	
370200-9761A	*1	45	RES, 9.76K,1/4W,1%,MF	R		11	1.0	EA	R21	Yes	
374300-0202A	*1	46	POT, 2K,TRIM,SIDE ADJ,CER	R		11	2.0	EA	R1,22	Yes	
376000-0003A	*1	47	MET,3/8 SQR,.15LS XSTR, 2N3904	R		11	2.0	EA	Q1,3	Yes	
376000-0019A	*1	48	XSTR, 2N7000,PET	R		11	1.0	EA	Q2	Yes	
378000-0005A	*1	49	DIO, 1N914,SIGNAL	R		11	8.0	EA	D6,7,8,9,10,11,12,13	Yes	
378000-0012A	*1	50	DIO, 1N4749A,24V,ZENER ** *NOT ONLY***	R		11	3.0	EA	D1,2,3	Yes	
382200-0005A	*1	51	CHOKE, 10UH,MOLDED	R		11	2.0	EA	L2,3	Yes	
382200-0018A	*1	52	CHOKE, 10,000UH MS75089-35	R		11	1.0	EA	L4	Yes	


Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400893-0000 PCBA, SINGLE IBP DAUGHTER BOARD, REVISION "N" A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
384000-0061A	*1	54	GAS TUBE (SURGE ARRESTER)	R		33	1.0	EA	DS1	Yes	
400552-0000	*1	55	ESCORT II ISO-TRANSFORMER , REV. 'A' **(FIFO)**	R		22	1.0	EA	T1	Yes	
360500-0060A	*1	57	STNDOFF, NYLON, #4 THREADED	R		11	2.0	EA		Yes	
358100-0021A	*1	58	SCR, 4-40 X 1/4, PH FLTHD, 100 DEG, ZN	R		11	4.0	EA		Yes	
365000-0016A	*1	61	SKT, 16-POS, DIP, TIN PLATE , L.P.	R		11	1.0	EA	U1	Yes	
352100-0104A	*1	62	CAP, .1UF, 50V, 10%, RAD, X7R	R		11	2.0	EA	C25, 26	Yes	
358100-0066A	*1	64	SCR, 6-32 X 2.75, LONG-LAG	R		11	1.0	EA		Yes	
360500-0022A	*1	66	NUT, #4 HEX, LRG PTTRN	R		11	3.0	EA		Yes	
352300-0007A	*1	67	CAP, .001UF, 10%, MYLAR	R		66	1.0	EA	C12	Yes	
370100-0100A	*1	68	RES, 10, 1/4W, 5%, CF	R		11	3.0	EA	R3, 41, 42	Yes	
100000	*1	69	NOTES & SPEC. INSTRUCTION S	P		0	0.0	EA	ON REV E PCB & BEFORE	Yes	
100000	*1	70	NOTES & SPEC. INSTRUCTION S	P		0	0.0	EA	R41&R42 ARE L1&L5	Yes	


Cumulative Lead Time for 400893-0000 = 66

REV	DESCRIPTION	DATE	APPROVED
A	INITIAL RELEASE MCO 466	6-14-93	
B	REVISION	1-11-93	
C	ECO 427	1-13-93	
D	ECO 635		
E	ECO 783		

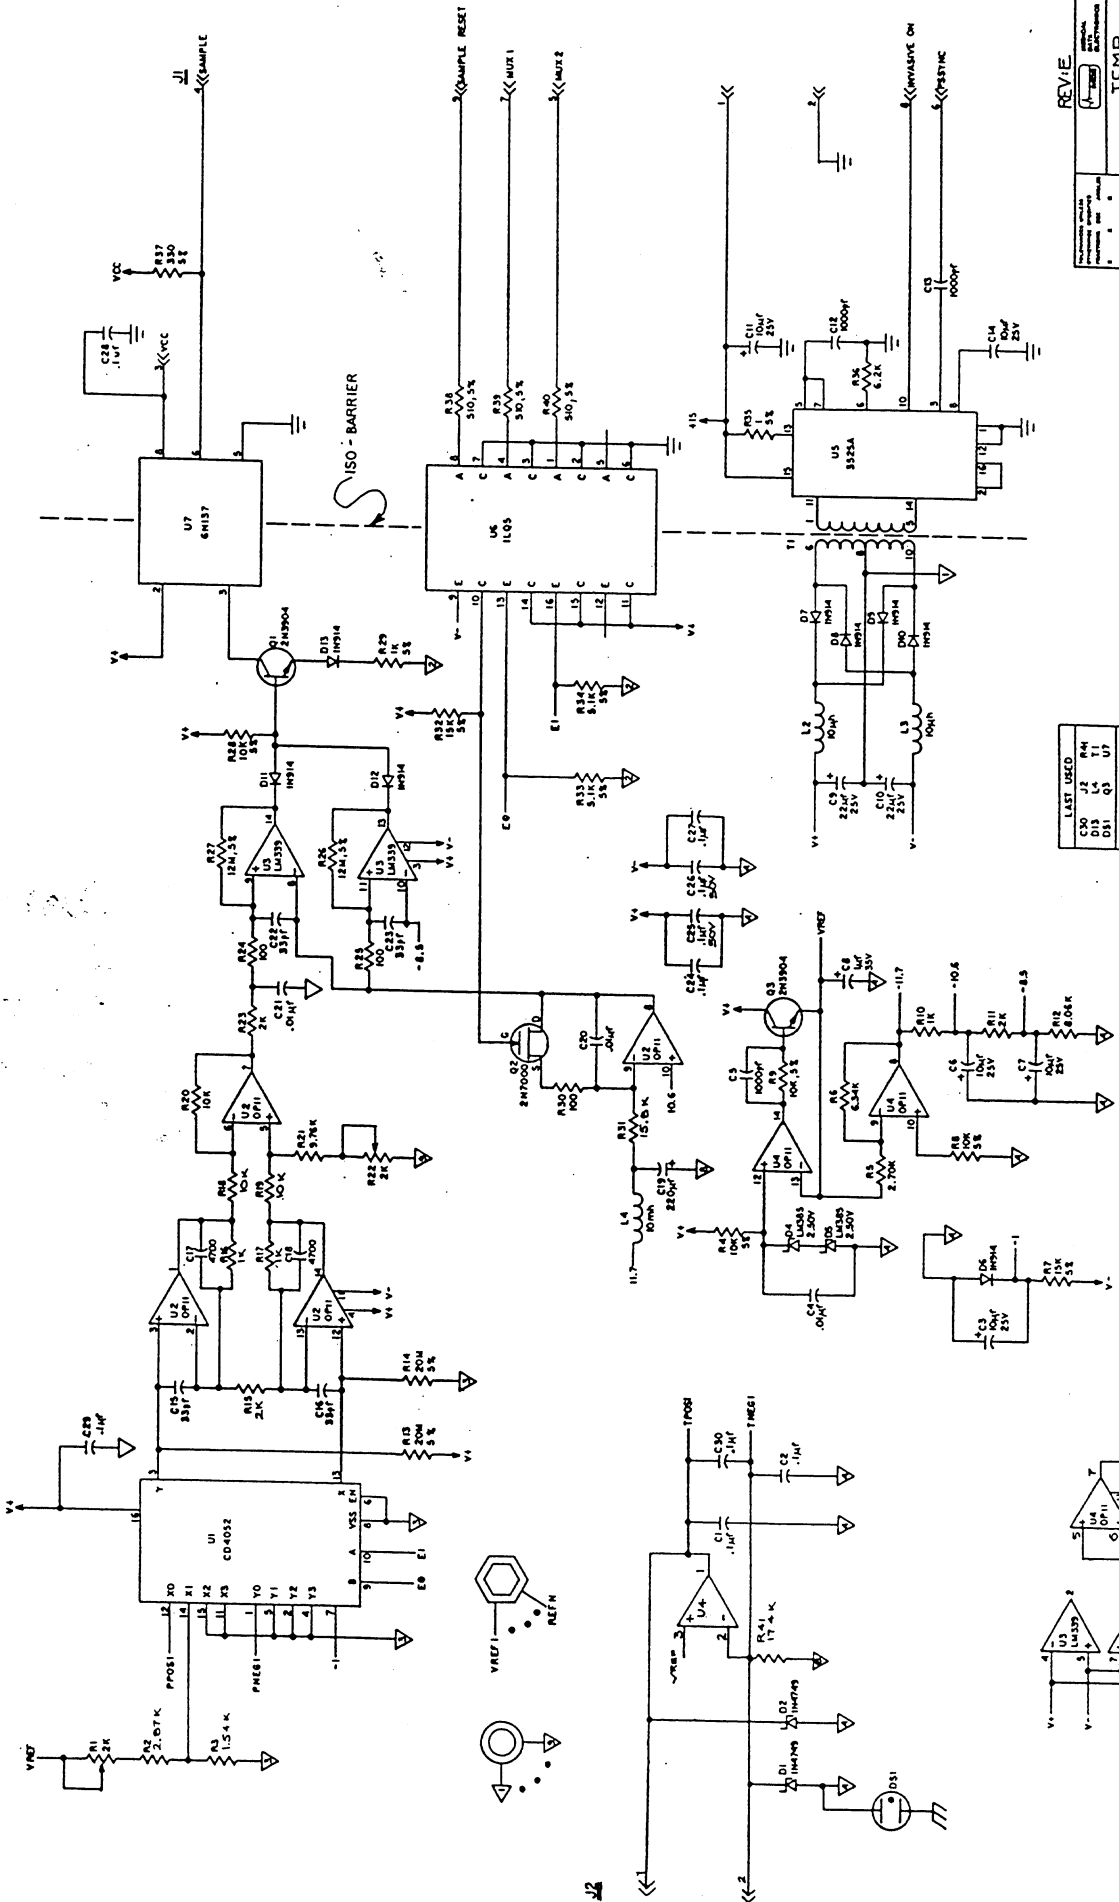

LAST USED		
C30	J2	R41
D13	L4	T1
D31	Q3	U7
NOT USED		
L1		
D3		

REV	DESCRIPTION	DATE	APPROVED
A	INITIAL RELEASE MCO 466	6-14-93	
B	REVISION	1-11-93	
C	ECO 427	1-13-93	
D	ECO 635		
E	ECO 783		

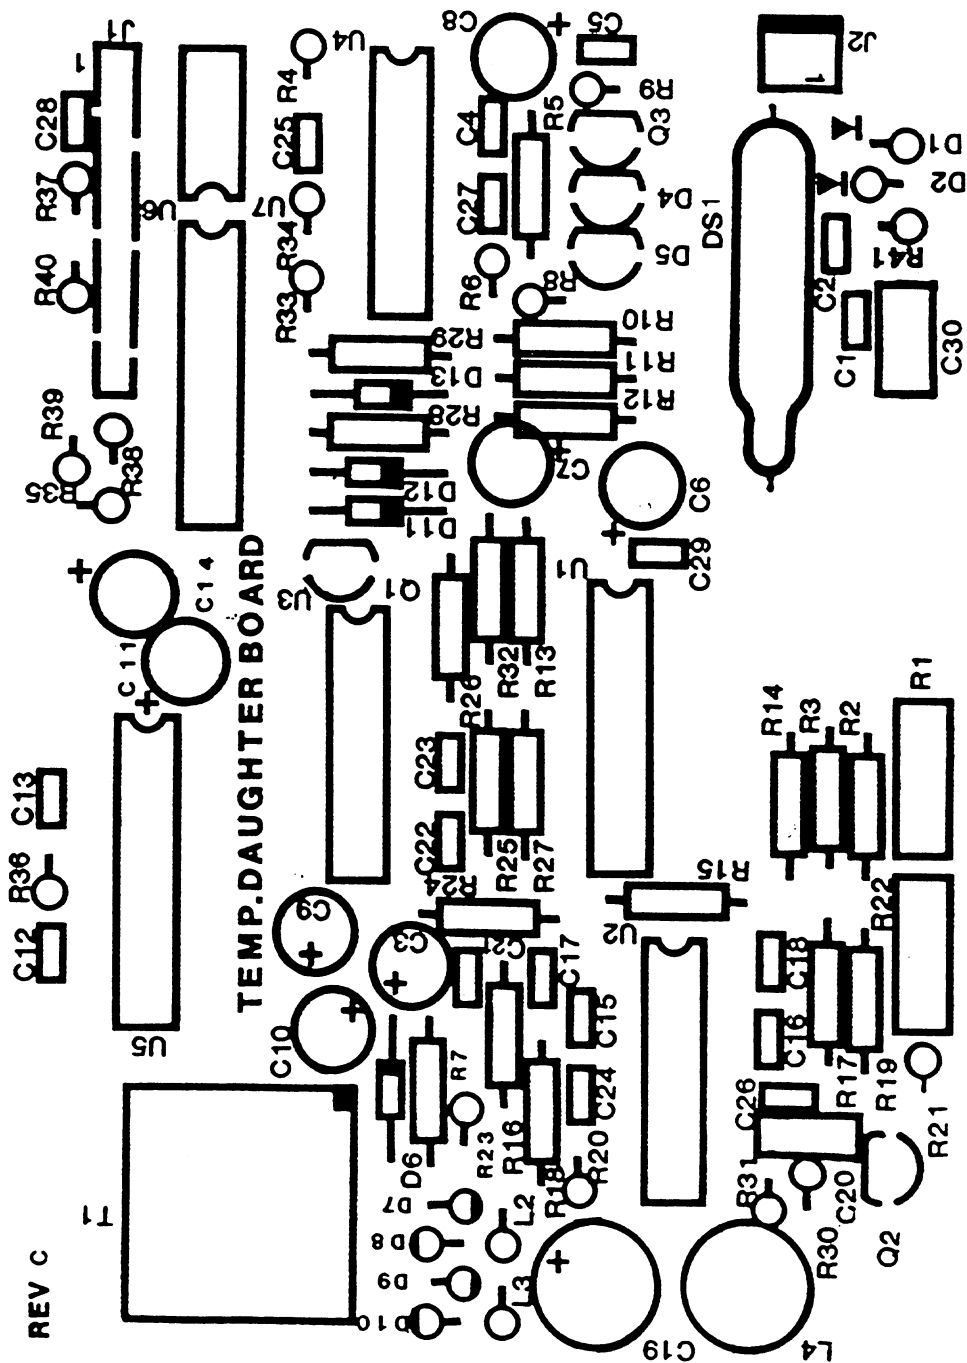

TEMP DAUGHTER BOARD

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400920-0000 PCBA, SINGLE TEMP. DGHTR. BOARD, REVISION "E" A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
400959-0000	*1	1	PCB, SGL.TEMP DGHTR. BD., RAW BOARD, REVISION 'D'	R		33	1.0	EA	USE UP REV. C PCB'S	Yes	
352100-0102A	*1	2	CAP, 1000PF,50V,10%,RAD,X 7R	R		11	2.0	EA	C5,13	Yes	
352100-0103A	*1	3	CAP, .01UF,50V,10%,RAD,X7 R	R		11	2.0	EA	C4,21	Yes	
352100-0472A	*1	4	CAP, .0047UF,25V,10%,RAD, X7R	R		22	2.0	EA	C17,18	Yes	
352101-0330A	*1	5	CAP, 33PF,100V,5%,RAD,NPO	R		22	4.0	EA	C15,16,22,23	Yes	
352201-0227A	*1	6	CAP, 220UF,10V,RAD,ELECT, .248 X .433 CS	R		66	1.0	EA	C19	Yes	
352301-0103A	*1	7	CAP, .01UF,100V,20%,POLYC ARB,.2 L.S.	R		66	1.0	EA	C20	Yes	
352301-0104A	*1	8	CAP, .1UF,5%,MYLAR	R		66	5.0	EA	C1,2,24,27,28	Yes	
352301-0104A	*1	9	CAP, .1UF,5%,MYLAR	R		66	2.0	EA	C29,30	Yes	
352400-0105A	*1	11	CAP, 1UF,50V,20%,RAD,TANT , MAX: HT. .28; O.D. .16	R		11	1.0	EA	C8	Yes	
352401-0106A	*1	12	CAP, 10UF,35V,20%,RAD,TAN T	R		11	5.0	EA	C3,6,7,11,14	Yes	
352400-0226A	*1	13	CAP, 22UF,25V,20%,TANT	R		11	2.0	EA	C9,10	Yes	
364000-0010A	*1	14	IC, LM339	R		11	1.0	EA	U3	Yes	
364000-0055A	*1	15	IC, CD4052	R		11	1.0	EA	U1	Yes	
364000-0065A	*1	16	IC, OP11FP,OP AMP	R		11	2.0	EA	U2,4	Yes	
378000-0034A	*1	17	DIO, LM385,ZENER (XSTR NA TIONAL ONLY)	R		11	2.0	EA	D4,5	Yes	
364000-0091A	*1	18	IC, SG 3525	R		44	1.0	EA	U5	Yes	
364000-0093A	*1	19	IC, ILQ5 QUAD OPTO ISOLAT OR	R		11	1.0	EA	U6	Yes	
364000-0099A	*1	21	IC, 6N137	R		11	1.0	EA	U7	Yes	
354000-0103A	*1	22	CONN, SGL ROW,STRT,SGL PI NS,SNAP-AWAY	R		11	1.0	PIN	J2	Yes	
354000-0187A	*1	23	CONN, MALE, SNAP-AWAY, 2 0 PIN STRIP, INTERCONNECT	R		11	9.0	EA	J1-MALE; 9 PIN = 1 PC	Yes	
370100-0010A	*1	24	RES, 1,1/4W,5%,CF	R		11	1.0	EA	R35	Yes	
370100-0101A	*1	26	RES, 100,1/4W,5%,CF	R		11	3.0	EA	R24,25,30	Yes	
370100-0102A	*1	27	RES, 1K,1/4W,5%,CF	R		11	1.0	EA	R29	Yes	
370100-0103A	*1	28	RES, 10K,1/4W,5%,CF	R		11	4.0	EA	R4,8,9,28	Yes	

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400920-0000 PCBA, SINGLE TEMP. DGHFR. BOARD, REVISION "E" A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
370100-0126A	*1	29	RES, 12K,1/4W,5%,CF	R		11	2.0	EA	R26,27		Yes
370100-0153A	*1	30	RES, 15K,1/4W,5%,CF	R		11	2.0	EA	R7,32		Yes
370100-0206A	*1	31	RES, 20K,1/4W,10%,CF	R		11	2.0	EA	R13,14		Yes
370100-0331A	*1	32	RES, 330,1/4W,5%,CF	R		11	1.0	EA	R37		Yes
370100-0511A	*1	33	RES, 510,1/4W,5%,CF	R		11	3.0	EA	R38,39,40		Yes
370100-0512A	*1	34	RES, 5.1K,1/4W,5%,CF	R		11	2.0	EA	R33,34		Yes
370100-0622A	*1	35	RES, 6.2K,1/4W,5%,CF	R		11	1.0	EA	R36		Yes
370200-1582A	*1	36	RES, 15.8K,1/4W,1%,MF	R		11	1.0	EA	R31		Yes
370200-1001A	*1	37	RES, 1K,1/4W,1%,MF	R		11	3.0	EA	R10,16,17		Yes
370200-1002A	*1	38	RES, 10K,1/4W,1%,MF	R		11	3.0	EA	R20,18,19		Yes
370200-1541A	*1	39	RES, 1.54K,1/4W,1%,MF	R		11	1.0	EA	R3		Yes
370200-2001A	*1	40	RES, 2K,1/4W,1%,MF	R		11	3.0	EA	R11,23,15		Yes
370200-2701A	*1	41	RES, 2.7K,1/4W,1%,MF	R		11	1.0	EA	R5		Yes
370200-2871A	*1	42	RES, 2.87K,1/4W,1%,MF	R		11	1.0	EA	R2		Yes
370200-6341A	*1	43	RES, 6.34K,1/4W,1%,MF	R		11	1.0	EA	R6		Yes
370200-8061A	*1	44	RES, 8.06K,1/4W,1%,MF (8 .05K N/A :0K PER KR)	R		11	1.0	EA	R12		Yes
370200-9761A	*1	45	RES, 9.76K,1/4W,1%,MF	R		11	1.0	EA	R21		Yes
374300-0202A	*1	46	POT, 2K,TRIM,SIDE ADJ,CER MET,3/8 SQR,.15LS	R		11	2.0	EA	R1,22		Yes
376000-0003A	*1	47	XSTR, 2N3904	R		11	2.0	EA	Q1,3		Yes
376000-0019A	*1	48	XSTR, 2N7000,PET	R		11	1.0	EA	Q2		Yes
378000-0005A	*1	49	DIO, 1N914,SIGNAL	R		11	8.0	EA	D6,7,8,9,10,11,12,13		Yes
378000-0012A	*1	50	DIO, 1N4749A,24V,ZENER ** *NOT ONLY***	R		11	2.0	EA	D1,2		Yes
382200-0005A	*1	51	CHOKE, 10UH,MOLDED	R		11	2.0	EA	L2,3		Yes
382200-0018A	*1	52	CHOKE, 10,000UH MS75089-35	R		11	1.0	EA	L4		Yes
100000	*1	53	NOTES & SPEC. INSTRUCTION S	P		0	0.0	EA	L1,5 - NOT USED		Yes

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400920-0000 PCBA, SINGLE TEMP. DGHTR. BOARD, REVISION "E" A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
384000-0061A	*1	54	GAS TUBE (SURGE ARRESTER)	R		33	1.0	EA	DS1	Yes	
400552-0000	*1	55	ESCORT II ISO-TRANSFORMER , REV. 'A' ** (FIFO) **	R		22	1.0	EA	T1	Yes	
360500-0060A	*1	57	STNDOFF, NYLON, #4 THREADE D	R		11	2.0	EA		Yes	
358100-0021A	*1	58	SCR, 4-40 X 1/4, PH FLTHD, 100 DEG, ZN	R		11	4.0	EA		Yes	
365000-0016A	*1	61	SKT, 16-POS, DIP, TIN PLATE , L.P.	R		11	1.0	EA	U1	Yes	
352100-0104A	*1	62	CAP, .1UF, 50V, 10%, RAD, X7R	R		11	2.0	EA	C25, 26	Yes	
360500-0063A	*1	63	STDOFF, #6, 1/4 RND X .75	R		11	1.0	EA		Yes	
358100-0066A	*1	64	SCR, 6-32 X 2.75, LONG-LAG	R		11	1.0	EA		Yes	
352300-0007A	*1	67	CAP, .001UF, 10%, MYLAR	R		66	1.0	EA	C12	Yes	
370200-1742A	*1	68	RES, 17.4K, 1/4W, 1%, MF	R		11	1.0	EA	R41	Yes	

Cumulative Lead Time for 400920-0000 = 66

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400859-0000 NIBP PNEUMATIC ASSEMBLY, REVISION 'I' A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
400849-0000	*1	1	NIBP PNEUMATICS BRACKET, REVISION 'B'	R		22	1.0	EA	1		Yes
400850-0000	*1	2	NIBP BULKHEAD CONNECTOR, REVISION 'D'	R		22	2.0	EA	2		Yes
360500-0057A	*1	3	NUT, 5/16 - 24	R		11	2.0	EA	3		Yes
360700-0001A	*1	4	VALVE, 12 VOLT	R		22	1.0	EA	4		Yes
400851-0000	*1	5	NIBP PNEUMATICS MANIFOLD REV. 'B'	R		22	1.0	EA	5		Yes
360700-0002A	*1	6	FITTING, HOSE NIPPLE 10-3 2,10-32	R		22	1.0	EA	6		Yes
360700-0003A	*1	7	FITTING, HOSE,10-32,1/8 I NCH	R		22	3.0	EA	7		Yes
360700-0004A	*1	8	FITTING, L HOSE,10-32,1/ 8 INCH	R		22	3.0	EA	8		Yes
400852-0000	*1	9	NIBP PRESS.SWITCH BRACKET , ZINC FINISH, REV. 'B'	R		22	1.0	EA	9		Yes
380000-0018A	*1	10	SWITCH, NIBP PRESSURE	R		22	1.0	EA	10		Yes
358100-0063A	*1	11	SCR, 2-56 X 5/8 PH PHHD	R		11	2.0	EA	11		Yes
360500-0020A	*1	12	NUT, 2-56 HEX	R		11	2.0	EA	12		Yes
358200-0020A	*1	13	WSHR, #2 INT TOOTH,CAD1 0 R NICKEL PLATING	R		11	2.0	EA	13		Yes
358200-0007A	*1	14	WSHR, #4 INT TOOTH	R		11	2.0	EA	14		Yes
360500-0022A	*1	15	NUT, #4 HEX,LRG PTTRN	R		11	2.0	EA	15		Yes
360500-0059A	*1	16	GROMMET, RUBBER #2185	R		11	3.0	EA	16		Yes
360500-0043A	*1	17	NUT, #4 LOCK,THIN PTTRN,W / NYLON INSERT	R		11	3.0	EA	17		Yes
400853-0000	*1	18	NIBP PUMP CAN AND LID (2 PCS. PER SET)	R		22	1.0	SET	18		Yes
400854-0000	*1	19	NIBP PUMP FOAM PACKING, REVISION 'B'	R		22	1.0	EA	20		Yes
400855-0000	*1	20	NIBP PUMP CAN FISH PAPER (1.7 SQ.IN. PER PC)	A		0	1.0	EA	21		Yes
360700-0009A	*1	21	PUMP, 12 VOLT NIBP, GLIA N	R		22	1.0	EA	22		Yes
360700-0005A	*1	22	FITTING, Y HOSE,1/8INCH	R		22	1.0	EA	23		Yes
385000-0020A	*1	23	TUBING, 1/8 INCH I.D.	R		11	16.1	IN	24		Yes
360700-0006A	*1	24	VALVE, PNEUMATIC CHECK	R		22	1.0	EA	25		Yes
360500-0058A	*1	25	STDOFF, #10 HEX,5/16 INCH	R		11	2.0	EA	26		Yes

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400859-0000 NIBP PNEUMATIC ASSEMBLY, REVISION 'I' A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
385000-0006A	*1	26	SHRINK TUBING, 3/8in BLAC K	R		11	0.3	IN.	19 (1PC = 1/4"	Yes	
360700-0008A	*1	27	MUFFLER, SINTERED METAL, 1 0-32	R		22	1.0	EA	27	Yes	
358100-0041A	*1	28	SCR, 6-32 X 1/4 PHL PHND	R		11	2.0	EA	28	Yes	
358200-0018A	*1	29	WSHR, #6 INT TOOTH STEEL	R		11	2.0	EA	29	Yes	
360700-0007A	*1	30	FITTING, L HOSE, 1/8 INCH	R		22	1.0	EA	30	Yes	
400890-0000	*1	33	NIBP VALVE/PUMP HARNESS, REVISION "D"	A		0	1.0	EA	33	Yes	
400891-0000	*1	34	NIBP PRESSURE SWITCH HARN G ESS, REVISION "G"	A		0	1.0	EA	34	Yes	
385000-0017A	*1	35	CABLE TIE MOUNT, ADHESIVE BACKED	R		11	2.0	EA	32,35	Yes	
385000-0000A	*1	36	TY-WRAPS, 3IN LENGTH (1000/BAG)	R		11	1.0	EA	36	Yes	
400958-0000	*1	37	CLIP, GROUND, REV. A	R		22	1.0	EA	37	Yes	
401005-0000	*1	38	WIRE ASSEMBLY, GROUND, REVISION 'B'	A		0	1.0	EA	38	Yes	

Cumulative Lead Time for 400859-0000 = 22

SAO₂ BOARD

CHAPTER 7

7.0.0 SAQ_i OPTION

7.1.0 OVERVIEW

The ESCORT 300A SAQ_i option provides an automatically calibrated measurement of blood oxygen content as well as deriving a pulse rate. The pulse oximeter employs spectrophotometric oximetry and plethysmography principles to obtain these readings.

The SAQ_i finger sensor has two low voltage LED light sources. One emits a red light (approximately 660nm) and the other emits an infrared light (approximately 920nm). The photo diode across from these two LED's senses the light that has passed through the sensor point. These values are then used by the pulse oximeter to calculate how much red and infrared light has been absorbed. With this information the percent of functional hemoglobin that is saturated with oxygen can be determined.

The ESCORT 300A SAQ_i option is packaged in two ways: 3 lead ECG SaO₂, slot 1 (SLOT1 SAQ_i); and 5 lead SAQ_i, slot 2 (SLOT2 SAQ_i). When configured with SLOT1 SAQ_i, 3 lead ECG and SAQ_i interface circuitry are both implemented on the same PCBA. When configured with SLOT2 SAQ_i, blood pressure or temperature as well as SAQ_i interface circuitry are all implemented on the same PCBA. These circuits are functionally identical to their original circuits with the exception of the interface circuitry for SAQ_i, isolated power supply, and the Nellcor OEM module. Please refer to Chapter 4 for the ECG and respiration theory of operation and to Chapter 5 for the blood pressure and temperature theory of operation.

7.1.1 NELLCOR OEM MODULE

A Nellcor OEM factory replaceable module is installed in all SAQ_i options. This module performs the SAQ_i functions of determining blood oxygen content, computing heart rate through pulse picking, and providing a pulse waveform. This information is transmitted from the module to the interface board by RS232 communications. In addition to the RS232 TX AND RX signals, an ECG SYNC signal goes to the Nellcor module for C-LOCK (tm) information. This ECG SYNC signal synchronizes the saturation measurements for the best time to perform an SAQ_i reading. If ECG SYNC is not present, C-LOCK (tm) will not be operational.

7.2.0 INTERFACE CIRCUITRY

Whether configured with SLOT1 or SLOT2 SAQ_i, the interface circuitry will be the same. J3 goes to the Nellcor module. The RS232 communications, RX, TX AND CTS* (clear to send), go to the opto-

couplers U13 and U14, as do RESET* and ECG SYNC. U13 and U14 provide isolation from line current for the patient. The signal RESET* comes from the CPU board and is active on power up and during hard resets. ECG SYNC signal information is pulled off the bus by U16 and outputted to U14 pin 8 for SLOT1 SAQ_i. For SLOT2 SAQ_i, the ECG SYNC signal information comes from the ECG board through the CPU board. The information is similarly pulled off the bus by U4 and fed to U14 pin 8. U4 and U16 are Z-80 compatible, 84 pin, serial/parallel/ counter/timer. U4 and U16 act as an I/O port between the digital and the isolated sections. This IC replaces the three I/O ports on the original ECG/RESP and BP/TEMP PCBA's.

The signal QRS OUT, at J1 pin 2, is a SAQ_i module generated ECG synchronizing signal that is routed to the AUX port, J8 pin 1, for the optional SAQ_i alarm.

7.3.0 ISOLATED SUPPLY

The isolation power supply circuits for SLOT1 and SLOT2 SAQ_i are functionally identical with the exception of the respiration drive that is exclusive to the SLOT1 SAQ_i. For convenience we shall refer to SLOT1 SAQ_i reference designators only. The pulse width modulator, U11, uses +15V as its Vin. PS SYNC keeps the supply voltages all switching on the same edge. The pulse width modulator uses the +5V as the sense line for voltage regulation. Q4 and Q5 drive T1. D19 and D14 are for spike protection. D8, D9, D10, and D13 form a bridge rectifier to turn the AC voltage to a DC voltage. L1 and C33-C34 filter the DC voltage.


The voltage regulation circuit uses D7 for a 2.5V reference input to the op-amp, U15. R58 and R59 divide the +5V in half and input it to U6. The difference is reflected at the output. It then goes to the opto-coupler U8, and on to the pulse width modulator.

3 LEAD-SAO2 (SLOT 1)


ISOLATED


NON-ISOLATED

EDGE CONNECTOR

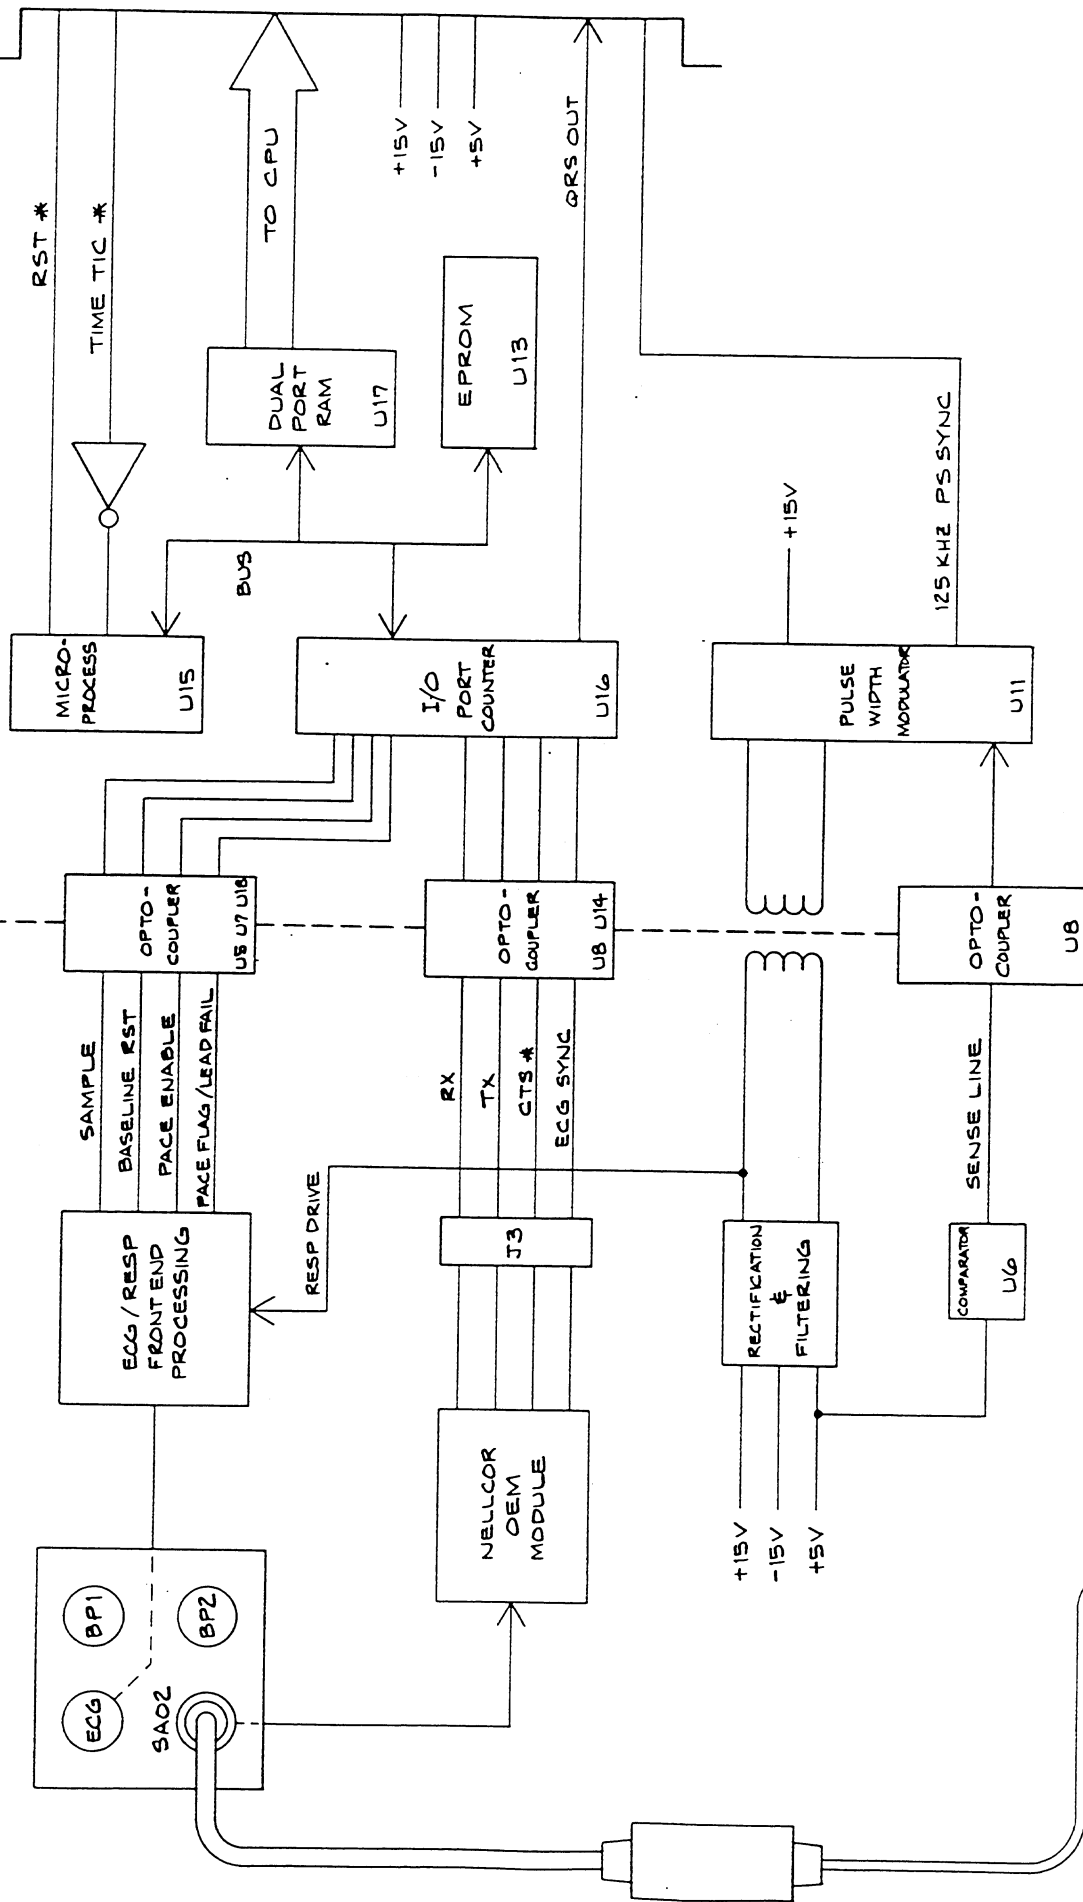


TOLERANCES UNLESS OTHERWISE SPECIFIED		FRACTIONS DEC ANGLES	
±	±	±	±
APPROVALS		DATE	
DRAWN: JAM		12-1-89	
CHECKED		SCALE	
		C	
MEDICAL ELECTRONICS		3 LEAD-SAO2 (SLOT 1) DIAGRAM	
DO NOT SCALE DRAWING		SHEET 1 OF 1	

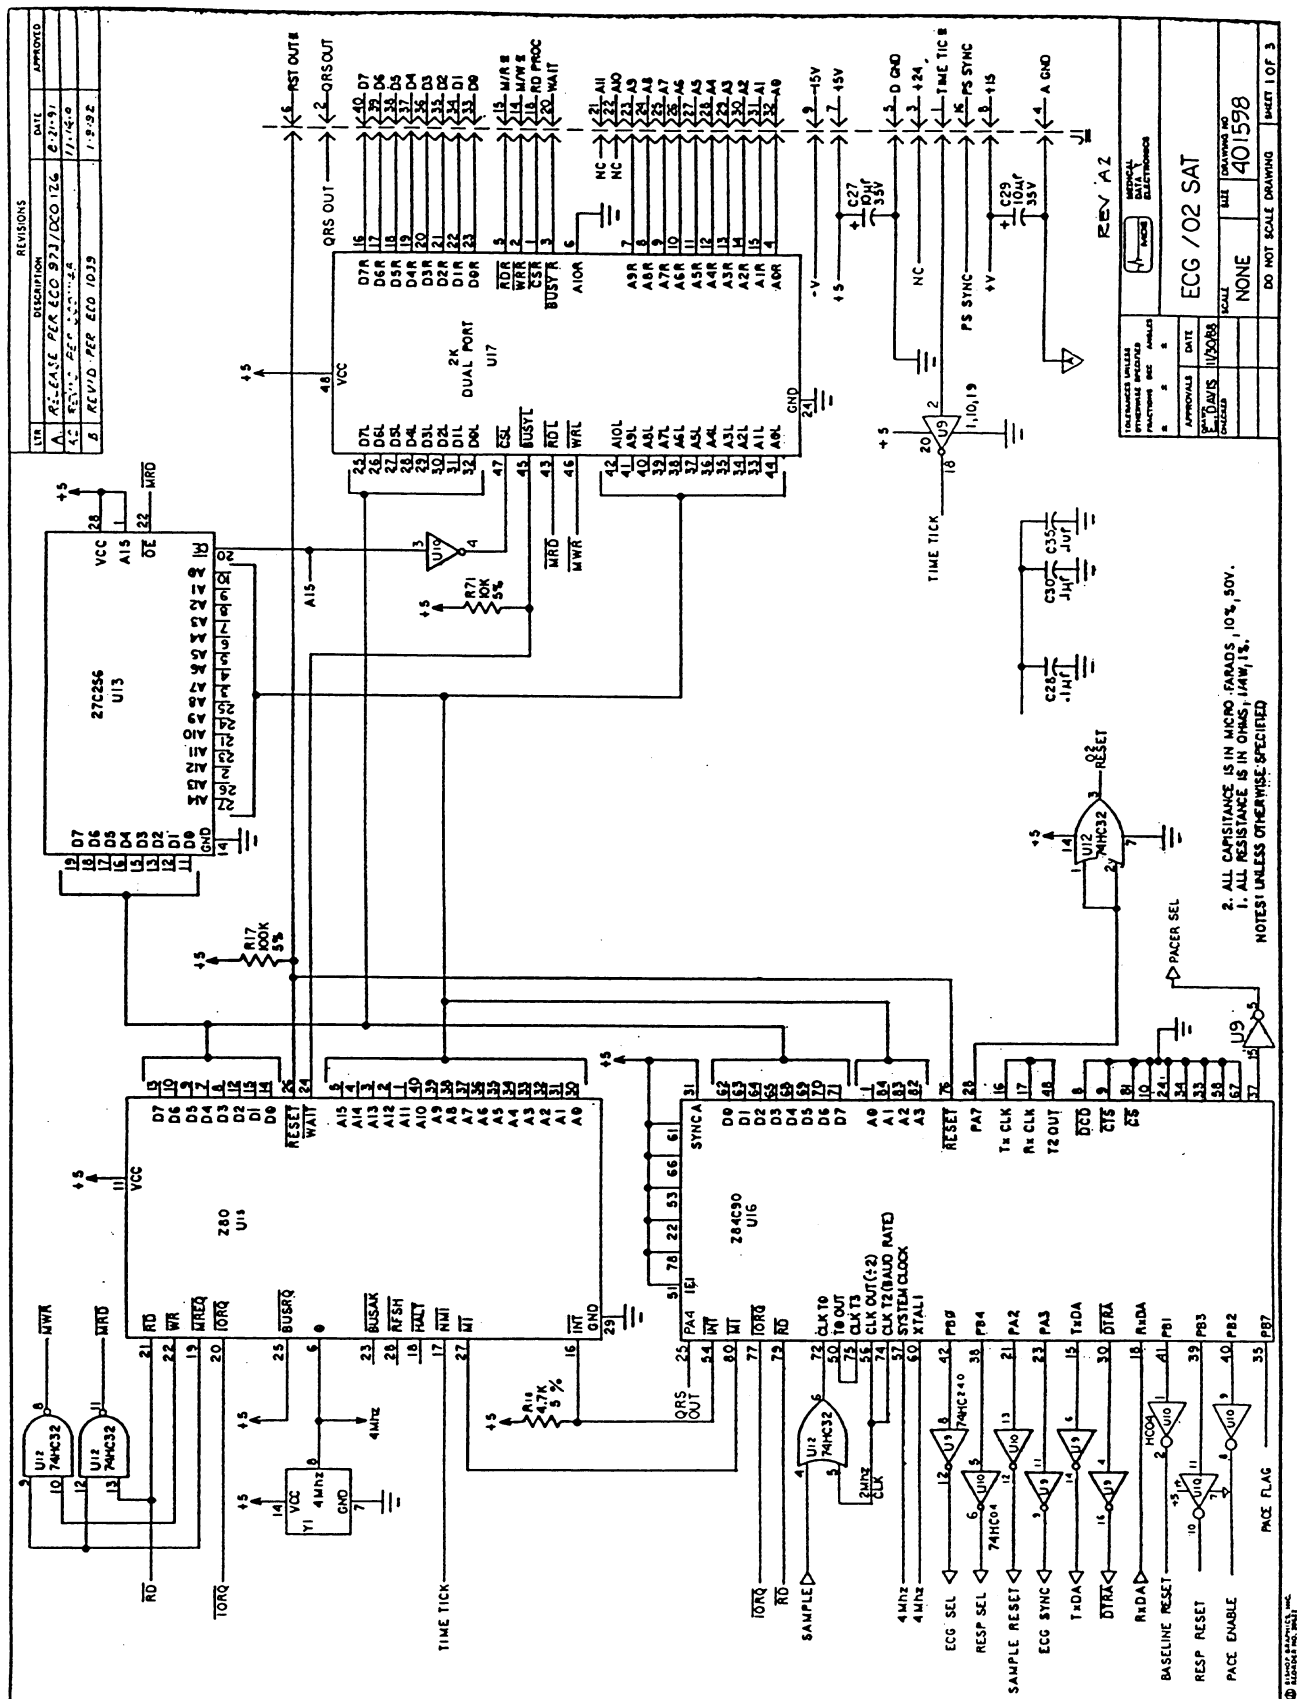

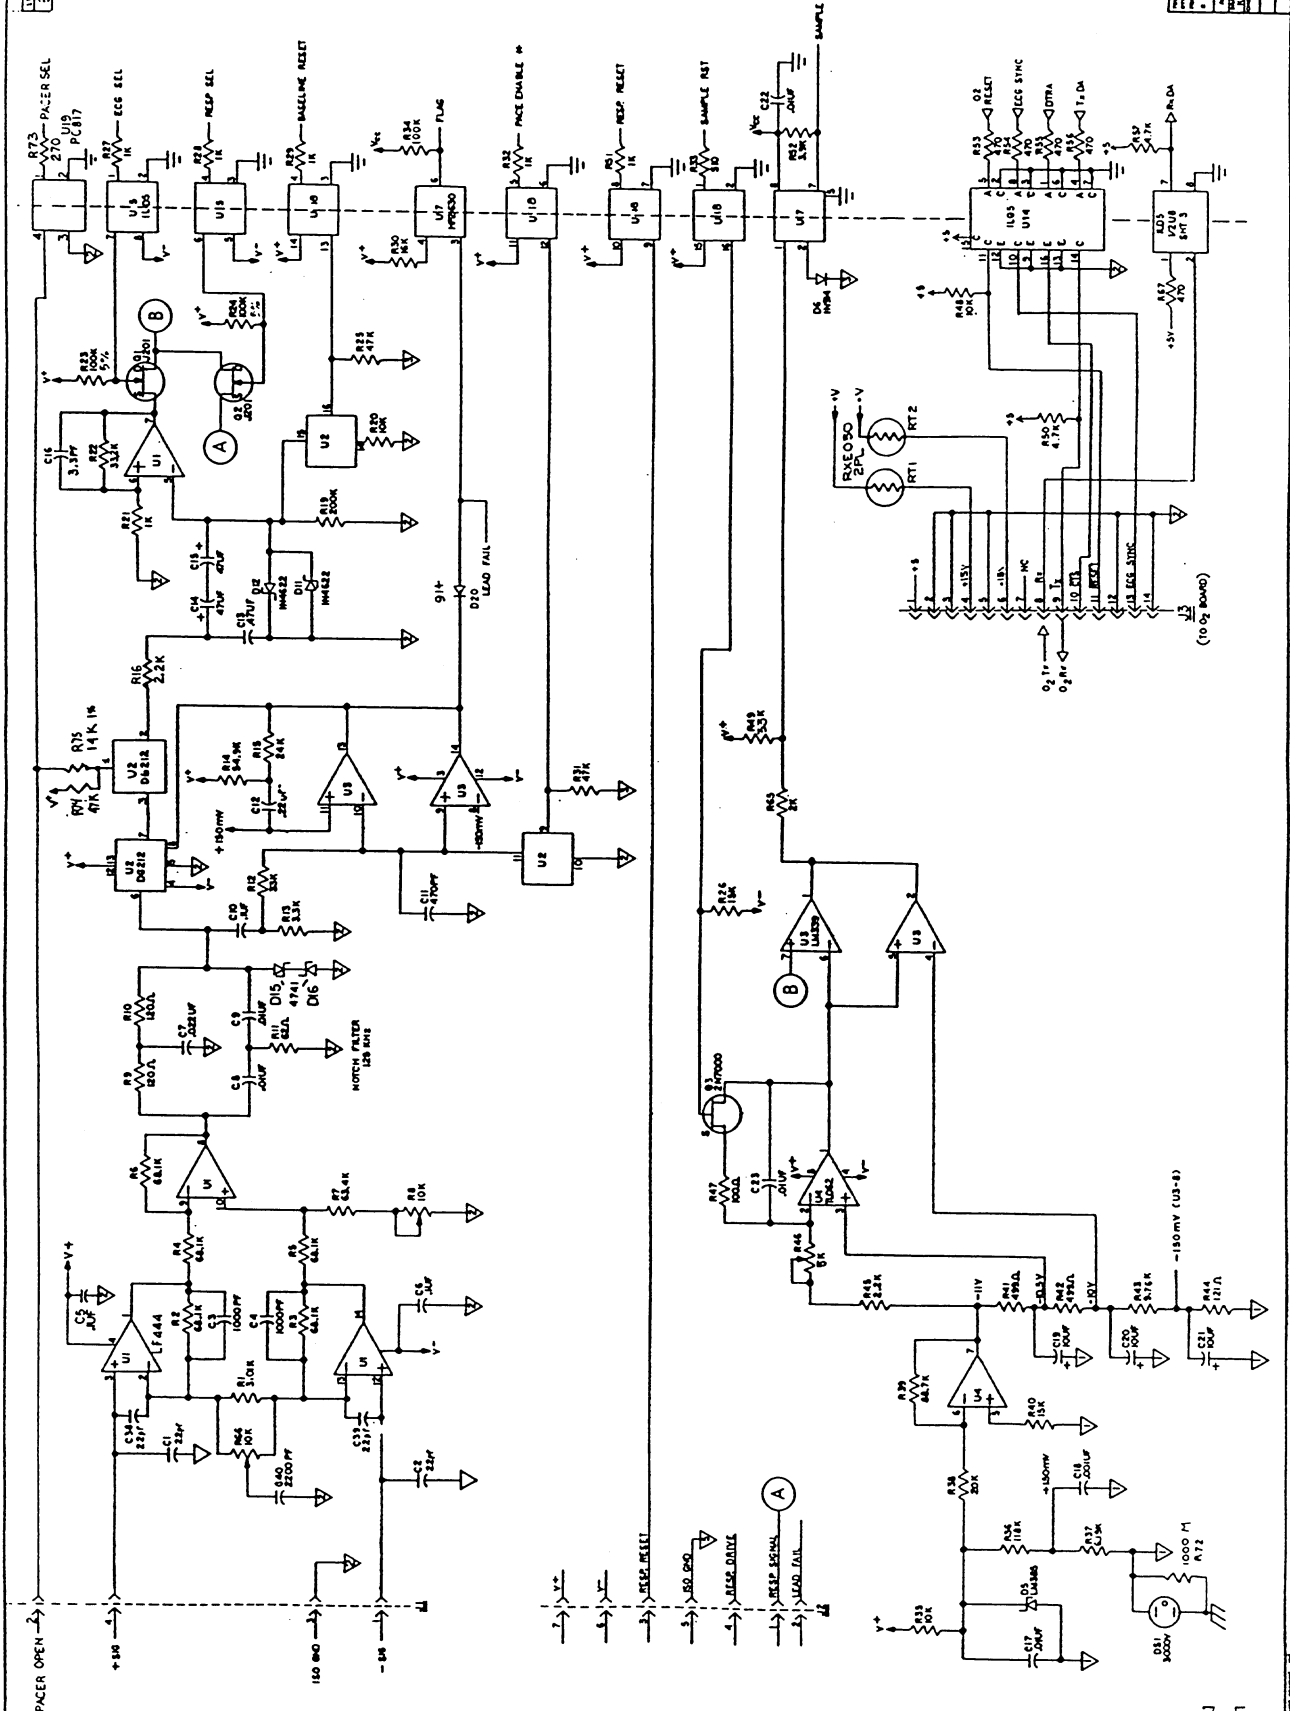


PROJECT	ECG/OC SAT
DATE	10/15/98
DESIGNER	NONE
CHECKED	
APPROVED	
REVISION	
DESCRIPTION	ECG/OC SAT
DATE	10/15/98
DESIGNER	NONE
CHECKED	
APPROVED	
REVISION	

REV	DESCRIPTION	DATE	BY
1	RELEASE PRE ECD 973	8-21-91	
2	AI CHANGE RES FOR DCO 122	10-15-93	

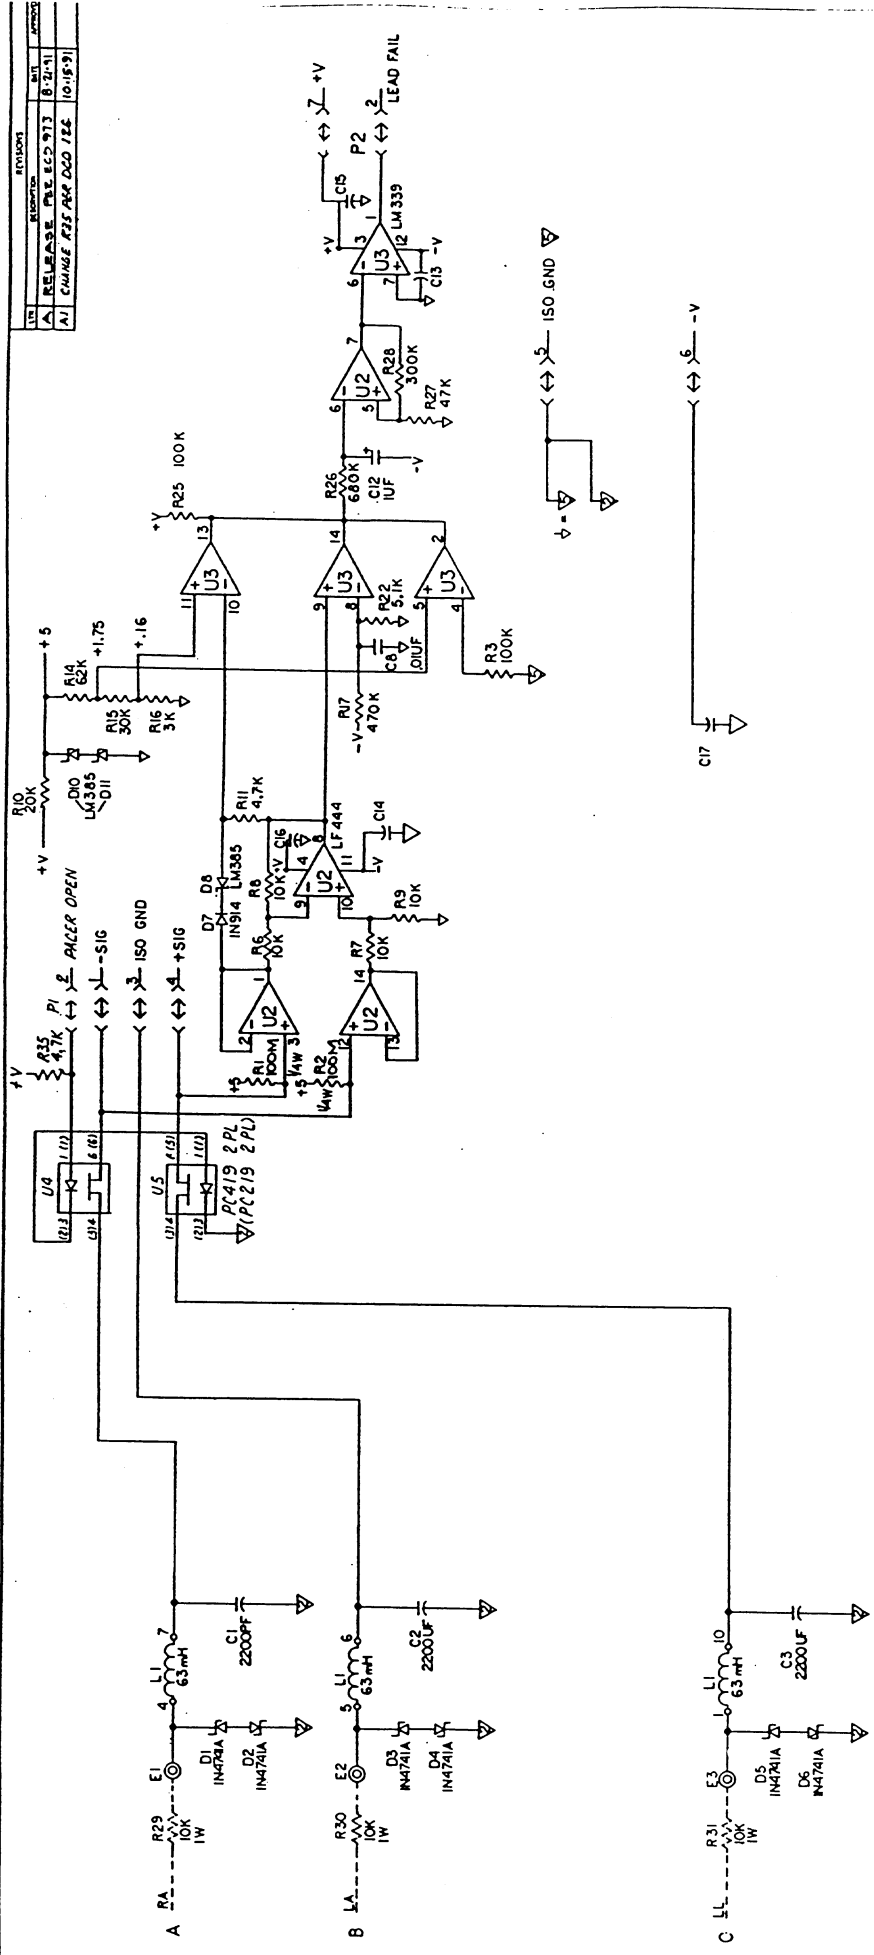


LAST USED: NOT USED:
 R 35
 C 20
 U 1
 Q 1

ALL RESISTORS 1/8 W UNLESS NOTED
 ◎ FEED THROUGH SOLDER PAUS
 -<->->- HEADER PIN CONN. 17/025



REV: AI	DATE: 10/15/93	BY: 10/15/93
ECG, SAO2	DAUGHTER BO	401601
SPARES	NONE	D


REV	DESCRIPTION	DATE	BY
1	RELEASED ESCD 913	8-21-91	...
2	ECO 126	15-7-91	...
3	ECO 1021 / 000 / 40	10-20-91	...

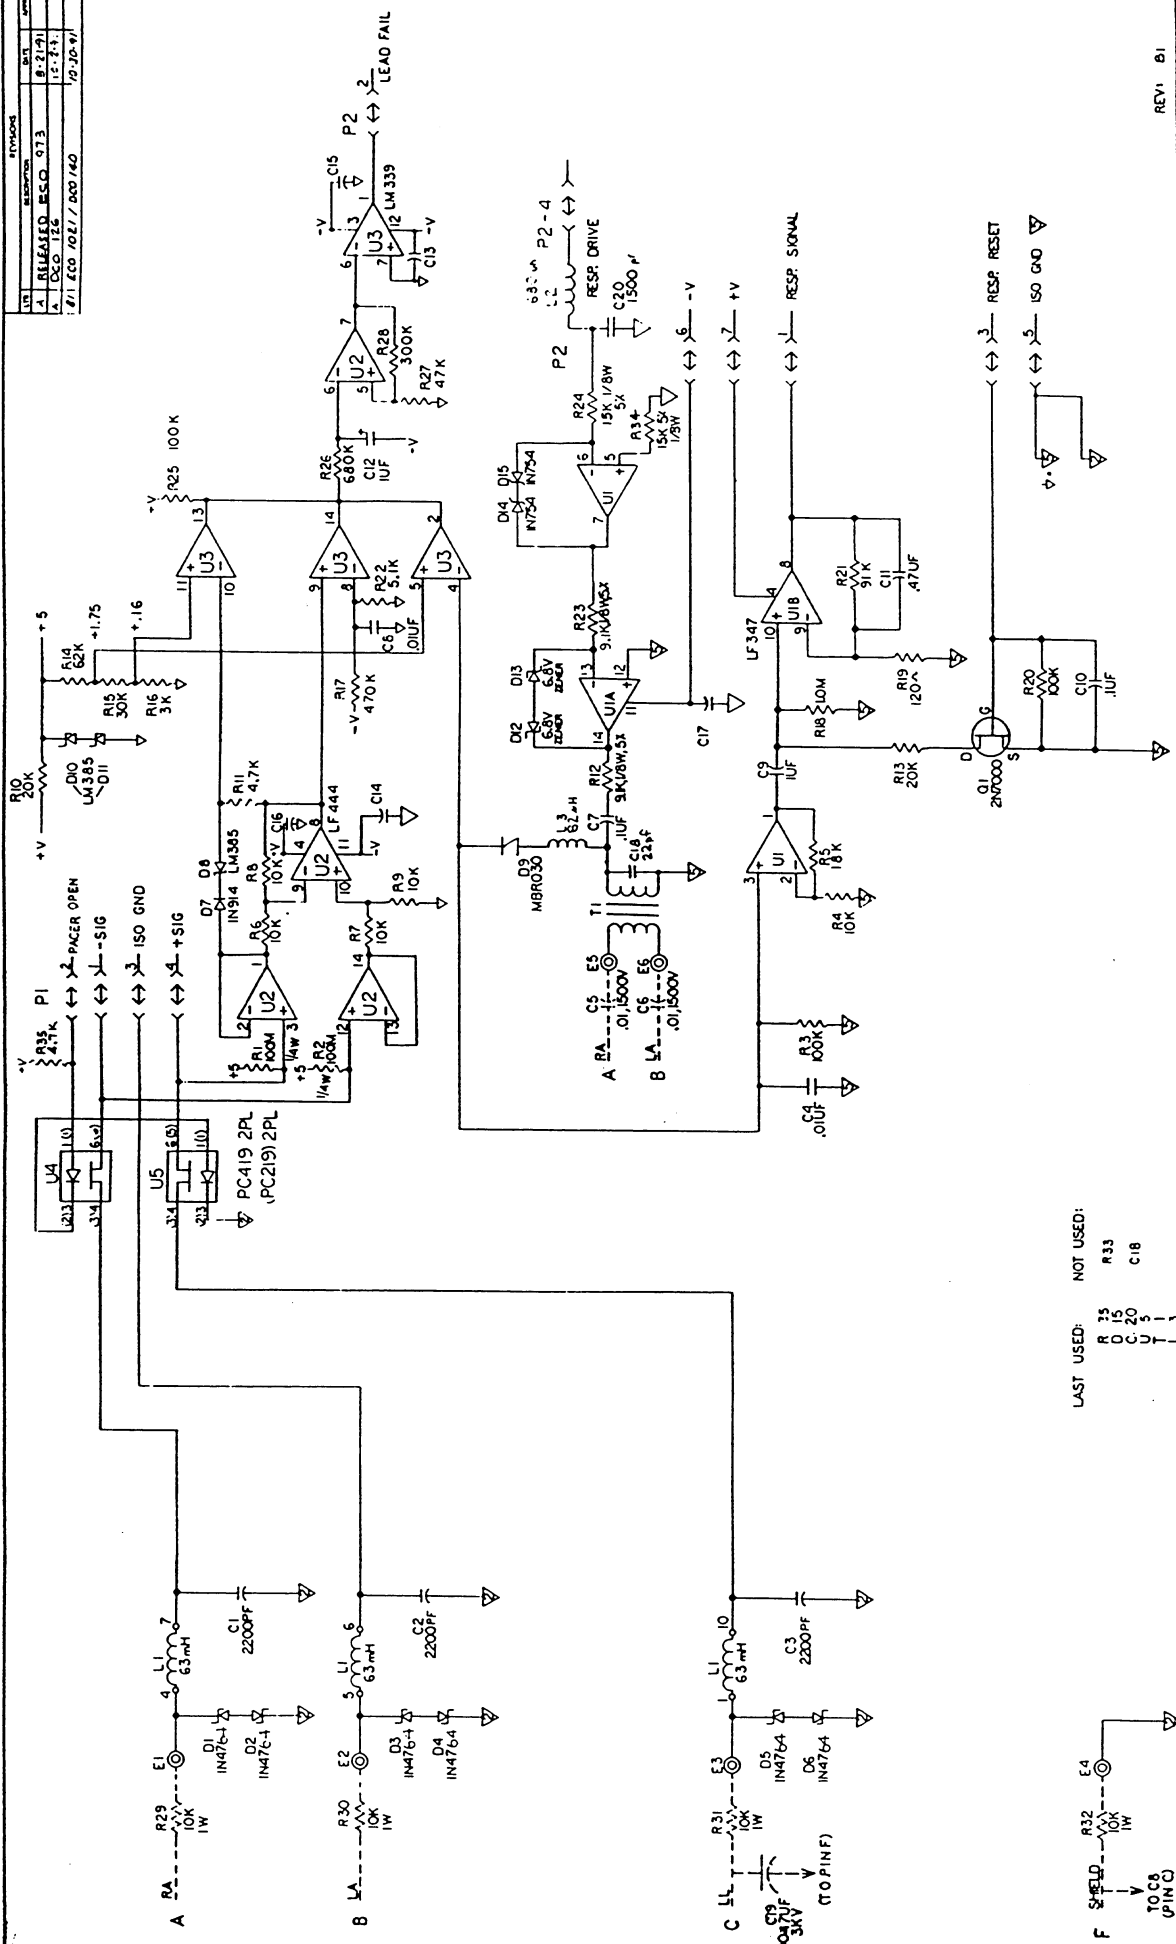


REV	1
DESCRIPTION	ECG W/RESP & Q2 SAT DAUGHTER 80
DATE	10-20-91
BY	...
REV	1
DESCRIPTION	ECG W/RESP & Q2 SAT DAUGHTER 80
DATE	10-20-91
BY	...

LAST USED: NOT USED:
 R 15 R 33
 Q 15 Q 18
 U 1 U 2
 U 3 U 4
 U 5 U 6
 U 7 U 8
 U 9 U 10

ALL RESISTORS 1/8 W UNLESS NOTED
 © FEED THROUGH SOLDER PADS
 - () - HEADER PIN CONN. 17/025



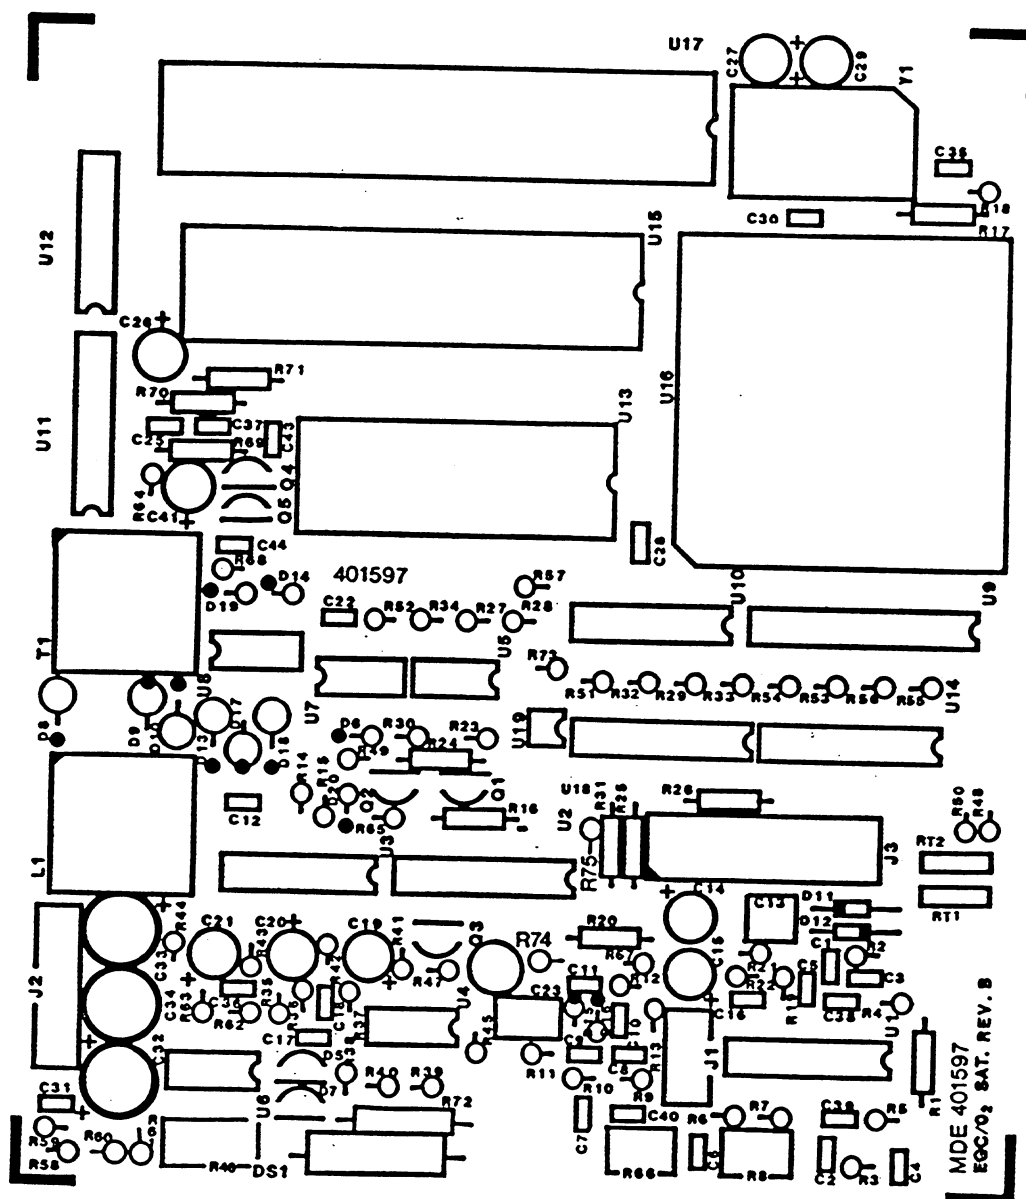

SLOT1 Sa0₂

Assembly Description
401598-0000 PCBA, ECG 3LD Sa02 MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
D 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
401597-0000	*1	1	PCB, ECG 3LD Sa02 MOTHER REV. B (E1044)	B	R	22	1.000	EA		Yes		
352100-0003A	*1	2	CAP, 3.3PF,50V,+/- .5PF,RA D,NPO EDPT		R	11	1.000	EA	C16	Yes		
100000	*1	3	NOTES & SPEC. INSTRUCTION S		P	0	0.000	EA	FOR ASSEMBLY	Yes		
352100-0220A	*1	5	CAP, 22PF,50V,10%,RAD,NPO EDPT		R	22	4.000	EA	C1,2,38,39	Yes		
352100-0223A	*1	6	CAP, .022UF,50V,10%,RAD,X7R		R	22	1.000	EA	C7	Yes		
352100-0331A	*1	7	CAP, 330PF,25V,10%,RAD,X7R		R	22	1.000	EA	C44	Yes		
352100-0471A	*1	8	CAP, 470PF,25V,10%,RAD,X7R		R	22	1.000	EA	C11	Yes		
352300-0007A	*1	9	CAP, .001UF,10%, MYLAR		R	66	3.000	EA	C25,37,43	Yes		
352300-0008A	*1	10	CAP, .01UF,5%,MYLAR		R	66	2.000	EA	C8,9	Yes		
352300-0015A	*1	11	CAP, .22UF,10%,MYLAR		R	66	1.000	EA	C12	Yes		
352300-0018A	*1	12	CAP, .47UF,10%,MYLAR		R	66	1.000	EA	C13	Yes		
352300-0102A	*1	13	CAP, 1000PF,50V,20%,RAD,MYLAR		R	66	1.000	EA	C18	Yes		
352300-0103A	*1	14	CAP, .01UF,50V,20%,RAD,MYLAR		R	22	2.000	EA	C17,22	Yes		
352300-0104A	*1	15	CAP, .1UF,50V,20%,RAD,MYLAR		R	22	5.000	EA	C5,6,28,30,31	Yes		
352300-0104A	*1	16	CAP, .1UF,50V,20%,RAD,MYLAR		R	22	2.000	EA	C35,36	Yes		
352300-0222A	*1	17	CAP, 2200PF,50V OR 100V,1%,MYLAR,.15L.S.		R	77	1.000	EA	C40	Yes		
352301-0103A	*1	18	CAP, .01UF,100V,20%,POLYCARB,.2 L.S.		R	66	1.000	EA	C23	Yes		
352301-0104A	*1	19	CAP, .1UF,5%,MYLAR		R	66	1.000	EA	C10	Yes		
352400-0105A	*1	20	CAP, 1UF,50V,20%,RAD,TANT, MAX: HT. .28; O.D. .16		R	11	1.000	EA	C26	Yes		
352203-0227A	*1	21	CAP, 220uF,16V,20%.RAD,ELCT,8mm x 12mm		R	77	1.000	EA	C32	Yes		
352200-0157A	*1	22	CAP, 150uF,25V,20%,RAD,ELCT,8mm x 12mm		R	22	2.000	EA	C33,34	Yes		
352401-0106A	*1	23	CAP, 10UF,35V,20%,RAD,TANT		R	11	6.000	EA	C19,20,21,27,29,41	Yes		
352401-0476A	*1	24	CAP, 47UF,10V,20%,RAD,TANT (10V ONLY)		R	11	2.000	EA	C14,15	Yes		
354000-0196A	*1	25	CONN, SGL ROW,STRT PIN,SNAP-AWAY (ENTER PER PIN)		R	22	4.000	PIN	1 PC. OF 4 PINS	Yes		

Assembly Description
401598-0000 PCBA, ECG 3LD Sa02 MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
0 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY U/M	REFERENCE	MLT	BEGIN	END
354000-0196A	*1	26	CONN, SGL ROW, STRT PIN, SN AP-AWAY (ENTER PER PIN)	R		22	7.000	PIN 1 PC. OF 7 PINS	Yes		
354000-0106A	*1	27	CONN, DBL ROW, STRT, SGL PI N, SNAP-AWAY	R		11	14.000	PIN J3 (14-PIN)	Yes		
356000-0008A	*1	28	REF OSCILLATOR, 4.0MHZ, CM OS HIGH SPEED	R		22	1.000	EA Y1	Yes		
360500-0048A	*1	29	SPCR, 1/4 X 1/4, SWAGE TYP E	R		11	1.000	EA DO NOT ISSUE	Yes		
364000-0008A	*1	30	IC, DG212CJ	R		11	1.000	EA U2	Yes		
364000-0010A	*1	31	IC, LM339	R		11	1.000	EA U3	Yes		
364000-0011A	*1	32	IC, LM358	R		11	1.000	EA U6	Yes		
364000-0025A	*1	33	IC, 74HC04	R		11	1.000	EA U10	Yes		
364000-0027A	*1	34	IC, 74HC32	R		11	1.000	EA U12	Yes		
364000-0038A	*1	35	IC, 27C256, CMOS, EPROM, 200 NS	R		11	1.000	EA U13	Yes		
364000-0080A	*1	36	IC, TMPZ84C00P (Z80A, CM OS VERSION)	R		11	1.000	EA U15	Yes		
364000-0091A	*1	37	IC, SG 3525	R		44	1.000	EA U11	Yes		
364000-0093A	*1	38	IC, ILQ5 QUAD OPTO ISOLAT OR	R		22	2.000	EA U14,18	Yes		
364000-0094A	*1	39	IC, HP2630, OPTO ISOLATOR	R		11	1.000	EA U7	Yes		
364000-0095A	*1	40	IC, MS6132, DUAL PORT RAM, 8 X 2K, 48-PIN (OR MS7132)	R		11	1.000	EA U17	Yes		
364000-0096A	*1	41	IC, 74HC240	R		11	1.000	EA U9	Yes		
364000-0131A	*1	42	IC, Z84C9008VSC ZILOG	R		11	1.000	EA U16 - ISSUE TO TEST	Yes		
364000-0132A	*1	43	IC, LF444 NATIONAL ONLY	R		22	1.000	EA U1	Yes		
364000-0133A	*1	44	IC, TL062ACP	R		11	1.000	EA U4	Yes		
364000-0134A	*1	45	IC, ILD5 DUAL OPTO	R		11	2.000	EA U5,8	Yes		
365000-0148A	*1	46	SOCKET, 48 PIN DIP	R		22	1.000	EA U17	Yes		
365000-0028A	*1	47	SKT, 28-POS, DIP, TIN PLATE , L.P.	R		11	1.000	EA U13X	Yes		
365000-0040A	*1	48	SKT, 40-POS, DIP, TIN PLATE , L.P.	R		11	1.000	EA U15X	Yes		
365000-0084A	*1	49	SKT, 84-PIN, PLCC	R		22	1.000	EA U4X,16X	Yes		

Assembly Description
401598-0000 PCBA, ECG 3LD Sa02 MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
D 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
370100-0101A	*1	50	RES, 100,1/4W,5%,CF	R		11	1.000	EA	R47	Yes		
370100-0102A	*1	51	RES, 1K,1/4W,5%,CF	R		11	5.000	EA	R27,28,29,32,51	Yes		
370100-0103A	*1	52	RES, 10K,1/4W,5%,CF	R		11	5.000	EA	R20,35,48,64,71	Yes		
370100-0104A	*1	53	RES, 100K,1/4W,5%,CF	R		11	5.000	EA	R34,17,23,24,62	Yes		
370100-0121A	*1	54	RES, 120,1/4W,5%,CF	R		11	2.000	EA	R9,10	Yes		
370100-0204A	*1	57	RES, 200K,1/4W,5%,CF	R		11	1.000	EA	R19	Yes		
370100-0222A	*1	58	RES, 2.2K,1/4W,5%,CF	R		11	2.000	EA	R45,16	Yes		
370100-0243A	*1	60	RES, 24K,1/4W,5%,CF	R		11	1.000	EA	R15	Yes		
370100-0332A	*1	61	RES, 3.3K,1/4W,5%,CF	R		11	2.000	EA	R13,49	Yes		
370100-0333A	*1	62	RES, 33K,1/4W,5%,CF	R		11	1.000	EA	R12	Yes		
370100-0392A	*1	63	RES, 3.9K,1/4W,5%,CF	R		11	1.000	EA	R52	Yes		
370100-0470A	*1	64	RES, 47,1/4W,5%,CF	R		11	1.000	EA	R69	Yes		
370100-0471A	*1	65	RES, 470,1/4W,5%,CF	R		11	5.000	EA	R53,54,55,56,67	Yes		
370100-0472A	*1	66	RES, 4.7K,1/4W,5%,CF	R		11	3.000	EA	R18,50,57	Yes		
370100-0473A	*1	67	RES, 47K,1/4W,5%,CF	R		11	3.000	EA	R25,31,74	Yes		
370100-0511A	*1	68	RES, 510,1/4W,5%,CF	R		11	2.000	EA	R33,68	Yes		
370100-0620A	*1	69	RES, 62,1/4W,5%,CF	R		11	1.000	EA	R11	Yes		
370100-0622A	*1	70	RES, 6.2K,1/4W,5%,CF	R		11	1.000	EA	R70	Yes		
370100-0153A	*1	72	RES, 15K,1/4W,5%,CF	R		11	2.000	EA	R26,40	Yes		
370100-0163A	*1	73	RES, 16K,1/4W,5%,CF	R		11	1.000	EA	R30	Yes		
370100-0202A	*1	74	RES, 2K,1/4W,5%,CF	R		11	4.000	EA	R58,61,63,65	Yes		
370200-1001A	*1	76	RES, 1K,1/4W,1%,MF	R		11	1.000	EA	R21	Yes		
370200-1183A	*1	77	RES, 118K,1/4W,1%,MF	R		11	1.000	EA	R36	Yes		
370200-1210A	*1	78	RES, 121,1/4W,1%,MF	R		11	1.000	EA	R44	Yes		

Assembly Description
401598-0000 PCBA, ECG 3LD Sa02 MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
D 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
370200-2001A	*1	79	RES, 2K,1/4W,1%,MF	R		11	2.000	EA	R59,60	Yes		
370200-2002A	*1	80	RES, 20K,1/4W,1%,MF	R		11	1.000	EA	R38	Yes		
370200-3011A	*1	81	RES, 3.01K,1/4W,1%,MF	R		11	1.000	EA	R1	Yes		
370200-3322A	*1	82	RES, 33.2K,1/4W,1%,MF	R		11	1.000	EA	R22	Yes		
370200-4990A	*1	83	RES, 499,1/4W,1%,MF	R		11	2.000	EA	R41,42	Yes		
370200-5492A	*1	84	RES, 54.9K,1/4W,1%,MF	R		11	1.000	EA	R14	Yes		
370200-6191A	*1	85	RES, 6.19K, 1/4W 1%, MF	R		11	1.000	EA	R37	Yes		
370200-6342A	*1	86	RES, 63.4K,1/4W,1%,MF	R		11	1.000	EA	R7	Yes		
370200-6812A	*1	87	RES, 68.1K,1/4W,1%,MF	R		11	5.000	EA	R2,3,4,5,6	Yes		
370200-8872A	*1	88	RES, 88.7K,1/4W,1%,MF	R		11	1.000	EA	R39	Yes		
370200-9761A	*1	89	RES, 9.76K,1/4W,1%,MF	R		11	1.000	EA	R43	Yes		
374300-0502A	*1	90	POT, 5K,TRIM,SIDE ADJ,CER MET,3/8 SQR,.15LS	R		11	1.000	EA	R46	Yes		
374401-0103A	*1	91	POT, 10K,TRIM,MULTI-TURN ,CERMET FILM (860X)	R		11	2.000	EA	R8,66	Yes		
376000-0019A	*1	92	XSTR, 2N7000,FET	R		11	1.000	EA	Q3	Yes		
376000-0020A	*1	93	XSTR, J201,FET	R		11	2.000	EA	Q1,2	Yes		
376000-0021A	*1	94	XSTR, 2N7010	R		44	2.000	EA	Q4,5	Yes		
378000-0005A	*1	95	DIO, 1N914,SIGNAL T&R	R		11	2.000	EA	D6,20	Yes		
378000-0011A	*1	96	DIO, 1N4741A,11V,ZENER T& R ***MOTOROLA ONLY***	R		11	2.000	EA	D15,16	Yes		
378000-0005A	*1	97	DIO, 1N914,SIGNAL T&R	R		11	2.000	EA	D11,12	Yes		
378000-0034A	*1	98	DIO, LM385,ZENER (XSTR NA TIONAL ONLY)	R		11	2.000	EA	D5,7	Yes		
900000	*1	99	ASSEMBLY LABOR & BURDEN	L		0	0.960	HR		Yes		
378000-0041A	*1	100	DIO, BYV27-150 (OR -200) T&R	R		22	6.000	EA	D8,9,10,13,17,18	Yes		
400988-0000	*1	101	ISO-TRANSFORMER, EP13 SWI TCHING SUPPLY	R		33	1.000	EA	T1	Yes		
400989-0000	*1	102	IDCTR, MULTI, EP13	R		22	1.000	EA	L1	Yes		

Assembly Description
401598-0000 PCBA, ECG 3LD Sa02 MOTHER REV. D (E1074)
Shrinkage Factor: 0.000

Group PFC Commodity Class Planner Buyer Drawing
A

Rev LT
D 22

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
384000-0061A	*1	103	GAS TUBE (SURGE ARRESTER)	R		33	1.000	EA	DS1	Yes		
370401-0108A	*1	104	RES, 1000M,1W,5%,2500V	R		66	1.000	EA	R72	Yes		
370200-1402A	*1	105	RES, 14K,1/4W,1%,MF	R		11	1.000	EA	R75	Yes		
100000	*1	106	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	FOR RESISTORS CHECK	Yes		
100000	*1	107	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	BIN - FILL IF REQUIRE	Yes		
100000	*1	108	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	CUT & JUMP PER	Yes		
100000	*1	109	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	ECO 950 & DCO 089	Yes		
364000-0176A	*1	110	IC, PC817,PHOTOCOUPLER,HI GH DENSITY MNTNG TYPE	R		22	1.000	EA	U19	Yes		
384000-0156A	*1	111	THERMISTOR, PTC RES DEV F OR CIRCUIT PROTECT	R		22	2.000	EA	RT1-2	Yes		
370100-0271A	*1	112	RES, 270,1/4W,5%,CF	R		11	1.000	EA	R73	Yes		
352101-0471A	*1	113	CAP, 470pF,10%,50V,RAD,HP 0	R		22	2.000	EA	C3,4	Yes		
378000-0040A	*1	120	DIO, 1N4756A,47V T&R	R		11	2.000	EA	D14,19	Yes		

Cumulative Lead Time for 401598-0000 = 99

Assembly	Description	Group	PFC	Commodity	Class	Planner	Buyer	Drawing	Rev	LT
401600-0000	PCBA, ECG W/RESP 3LD Sa02 DAUGHTER REV. B1 (D140)				A				B1	22

Shrinkage Factor: 0.000

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
401599-0000	*1	1	PCB, ECG 3LD Sa02 DAUGHTER REV. A (E973)	R		22	1.000	EA	-	Yes		
352100-0104A	*1	2	CAP, .1UF,50V,10%,RAD,X7R	R		11	5.000	EA	C13,14,15,16,17	Yes		
352100-0152A	*1	3	CAP, 1500PF,100V,20%,MONO CER,X7R	R		22	1.000	EA	C20	Yes		
352300-0103A	*1	4	CAP, .01UF,50V,20%,RAD,MYLAR	R		22	2.000	EA	C4,8	Yes		
352300-0104A	*1	5	CAP, .1UF,50V,20%,RAD,MYLAR	R		22	2.000	EA	C7,10	Yes		
352300-0222A	*1	6	CAP, 2200PF,50V OR 100V,1%,MYLAR,.15L.S.	R		77	2.000	EA	C1,3	Yes		
352300-0474A	*1	7	CAP, .47UF, 50V,20%,RAD,MYLAR(METALLIZED POLYESTER)	R		22	1.000	EA	C11	Yes		
352301-0105A	*1	8	CAP, 1UF,63V,20%,MYLAR	R		66	1.000	EA	C9	Yes		
352100-0220A	*1	9	CAP, 22PF,50V,10%,RAD,NPO EDPT	R		22	1.000	EA	C18	Yes		
352400-0105A	*1	10	CAP, 1UF,50V,20%,RAD,TANT, MAX: HT. .28; O.D. .16	R		11	1.000	EA	C12	Yes		
354000-0142A	*1	12	CONN, 7 SKT STRP,.1 SKT SP,.335 HT	R		22	1.000	EA		Yes		
354000-0143A	*1	13	CONN, 4 SKT STRP,.1 SKT SP,.335 HT.	R		22	1.000	EA		Yes		
364000-0010A	*1	14	IC, LM339	R		11	1.000	EA	U3	Yes		
352101-0472A	*1	15	CAP, 4700PF,20%,3KV, Z5U, CERAMIC DISC (5000PF OK)	R		22	1.000	EA	C19	Yes		
364000-0132A	*1	16	IC, LF444 NATIONAL ONLY	R		22	1.000	EA	U2	Yes		
365000-0014A	*1	17	SKT, 14-POS,DIP,TIN PLATE ,L.P.	R		11	1.000	EA	U1	Yes		
370101-0103A	*1	18	RES, 10K,1/8W,5%,CF	R		11	5.000	EA	R4,6,7,8,9	Yes		
370101-0203A	*1	19	RES, 20K,1/8W,5%,CF	R		11	2.000	EA	R10,13	Yes		
370402-0103A	*1	20	RES, 10K,1/2W,5%,CC (ALL N BRDLY ONLY)*BULK ONLY*	R		22	4.000	EA	R32,29,30,31	Yes		
370101-0153A	*1	22	RES, 15K,1/8W,5%,CF	R		11	2.000	EA	R24,34	Yes		
370101-0104A	*1	23	RES, 100K,1/8W,5%,CF	R		11	3.000	EA	R3,20,25	Yes		
370101-0105A	*1	24	RES, 1M,1/8W,5%,CF	R		11	1.000	EA	R18	Yes		
370101-0121A	*1	25	RES, 120,1/8W,5%,CF	R		11	1.000	EA	R19	Yes		
370101-0183A	*1	26	RES, 18K,1/8W,5%,CF	R		11	1.000	EA	R5	Yes		

Assembly	Description	Group	PFC	Commodity	Class	Planner	Buyer	Drawing	Rev	LT
401600-0000	PCBA, ECG W/RESP 3LD Sa02 DAUGHTER REV. B1 (D140)				A				81	22
Shrinkage Factor: 0.000										

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
370101-0302A	*1	27	RES, 3K,1/8W,5%,CF	R		11	1.000	EA	R16	Yes		
370101-0303A	*1	28	RES, 30K,1/8W,5%,CF	R		11	1.000	EA	R15	Yes		
370101-0304A	*1	29	RES, 300K,1/8W,5%,CF	R		11	1.000	EA	R28	Yes		
370101-0472A	*1	30	RES, 4.7K,1/8W,5%,CF	R		11	1.000	EA	R11	Yes		
370101-0473A	*1	31	RES, 47K,1/8W,5%,CF	R		11	1.000	EA	R27	Yes		
370101-0474A	*1	32	RES, 470K,1/8W,5%,CF	R		11	1.000	EA	R17	Yes		
370101-0512A	*1	33	RES, 5.1K,1/8W,5%,CF	R		11	1.000	EA	R22	Yes		
370101-0623A	*1	34	RES, 62K,1/8W,5%,CF	R		11	1.000	EA	R14	Yes		
370101-0684A	*1	35	RES, 680K,1/8W,5%,CF	R		11	1.000	EA	R26	Yes		
370101-0912A	*1	36	RES, 9.1K,1/8W,5%,CF	R		11	2.000	EA	R12,23	Yes		
370101-0913A	*1	37	RES, 91K,1/8W,5%,CF	R		22	1.000	EA	R21	Yes		
370500-0107A	*1	38	RES, 100M,1/4W,5%,M.O. (O R M.G.)	R		33	2.000	EA	R1,2	Yes		
376000-0019A	*1	39	XSTR, 2N7000,FET	R		11	1.000	EA	Q1	Yes		
378000-0005A	*1	40	DIO, 1N914,SIGNAL T&R	R		11	1.000	EA	D7	Yes		
378000-0009A	*1	41	DIO, 1N754A,6.8V,ZENER T& R ***NOT ONLY***	R		11	4.000	EA	D12,13,14,15	Yes		
378000-0054A	*1	42	DIO, 1N4764,100V,ZENER	R		22	6.000	EA	D1,2,3,4,5,6	Yes		
378000-0034A	*1	43	DIO, LM385,ZENER (XSTR NA TIONAL ONLY)	R		11	3.000	EA	D8,10,11	Yes		
378000-0037A	*1	44	DIO, MBR030,SCHOTTKY RCTF R	R		11	1.000	EA	D9	Yes		
382200-0030A	*1	45	INDCTR, 680uH SHIELDED	R		22	1.000	EA	L2	Yes		
352600-0019A	*1	46	CAP, .01UF,1000V,20%,Z5U, CER DISC,.4 L.S.	R		11	2.000	EA	C5,6	Yes		
400554-0000	*1	47	IDCTR, MULTI ESCORT II, R EV. 'B' **(FIFO)**	R		22	1.000	EA	L1	Yes		
364000-0135A	*1	48	IC, LF347, SCREENED TO +/- -1.5mV OFFSET & LOW NOISE	A		22	1.000	EA	U1	Yes		
382200-0027A	*1	49	IDCTR, 82uH,SHIELDED,ISOL ATED	R		22	1.000	EA	L3 IN SERIES WITH D9	Yes		
400553-0000	*1	50	XFMR, ESC. II RESP DRIVE REV. A **(FIFO)**	R		22	1.000	EA	T1	Yes		



Assembly	Description	Group	PFC	Commodity	Class	Planner	Buyer	Drawing	Rev	LT
401600-0000	PCBA, ECG W/RESP 3LD Sa02 DAUGHTER REV. B1 (D140)				A				B1	22

Shrinkage Factor: 0.000

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN	END
100000	*1	51	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	FOR ASSEMBLY	Yes		
100000	*1	52	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	FOR RESISTORS CHECK	Yes		
100000	*1	53	NOTES & SPEC. INSTRUCTION S	P		0	0.000	EA	BIN - FILL IF REQUIRE	Yes		
364000-0175A	*1	54	IC, PC219,PHOTOCOUPLER,MI NI-FLAT PKG.	R		22	2.000	EA	U4-5	Yes		
370100-0472A	*1	55	RES, 4.7K,1/4W,5%,CF	R		11	1.000	EA	R35	Yes		
399200-0001A	*1	56	24 GA BUSS WIRE, 1000 FT/ROLL	R		11	0.100	FT.	C2 - 1 PC = 1/2 IN.	Yes		
900000	*1	99	ASSEMBLY LABOR & BURDEN	L		0	0.190	HR	-	Yes		

Cumulative Lead Time for 401600-0000 = 99

0	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22	23	24	25	26	27	28	29	30	31	32	33	34	35	36	37	38	39	40	41	42	43	44	45	46	47	48	49	50	51	52	53	54	55	56	57	58	59	60	61	62	63	64	65	66	67	68	69	70	71	72	73	74	75	76	77	78	79	80	81	82	83	84	85	86	87	88	89	90	91	92	93	94	95	96	97	98	99	100	101	102	103	104	105	106	107	108	109	110	111	112	113	114	115	116	117	118	119	120	121	122	123	124	125	126	127	128	129	130	131	132	133	134	135	136	137	138	139	140	141	142	143	144	145	146	147	148	149	150	151	152	153	154	155	156	157	158	159	160	161	162	163	164	165	166	167	168	169	170	171	172	173	174	175	176	177	178	179	180	181	182	183	184	185	186	187	188	189	190	191	192	193	194	195	196	197	198	199	200	201	202	203	204	205	206	207	208	209	210	211	212	213	214	215	216	217	218	219	220	221	222	223	224	225	226	227	228	229	230	231	232	233	234	235	236	237	238	239	240	241	242	243	244	245	246	247	248	249	250	251	252	253	254	255	256	257	258	259	260	261	262	263	264	265	266	267	268	269	270	271	272	273	274	275	276	277	278	279	280	281	282	283	284	285	286	287	288	289	290	291	292	293	294	295	296	297	298	299	300	301	302	303	304	305	306	307	308	309	310	311	312	313	314	315	316	317	318	319	320	321	322	323	324	325	326	327	328	329	330	331	332	333	334	335	336	337	338	339	340	341	342	343	344	345	346	347	348	349	350	351	352	353	354	355	356	357	358	359	360	361	362	363	364	365	366	367	368	369	370	371	372	373	374	375	376	377	378	379	380	381	382	383	384	385	386	387	388	389	390	391	392	393	394	395	396	397	398	399	400	401	402	403	404	405	406	407	408	409	410	411	412	413	414	415	416	417	418	419	420	421	422	423	424	425	426	427	428	429	430	431	432	433	434	435	436	437	438	439	440	441	442	443	444	445	446	447	448	449	450	451	452	453	454	455	456	457	458	459	460	461	462	463	464	465	4
---	---	---	---	---	---	---	---	---	---	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	-----	---

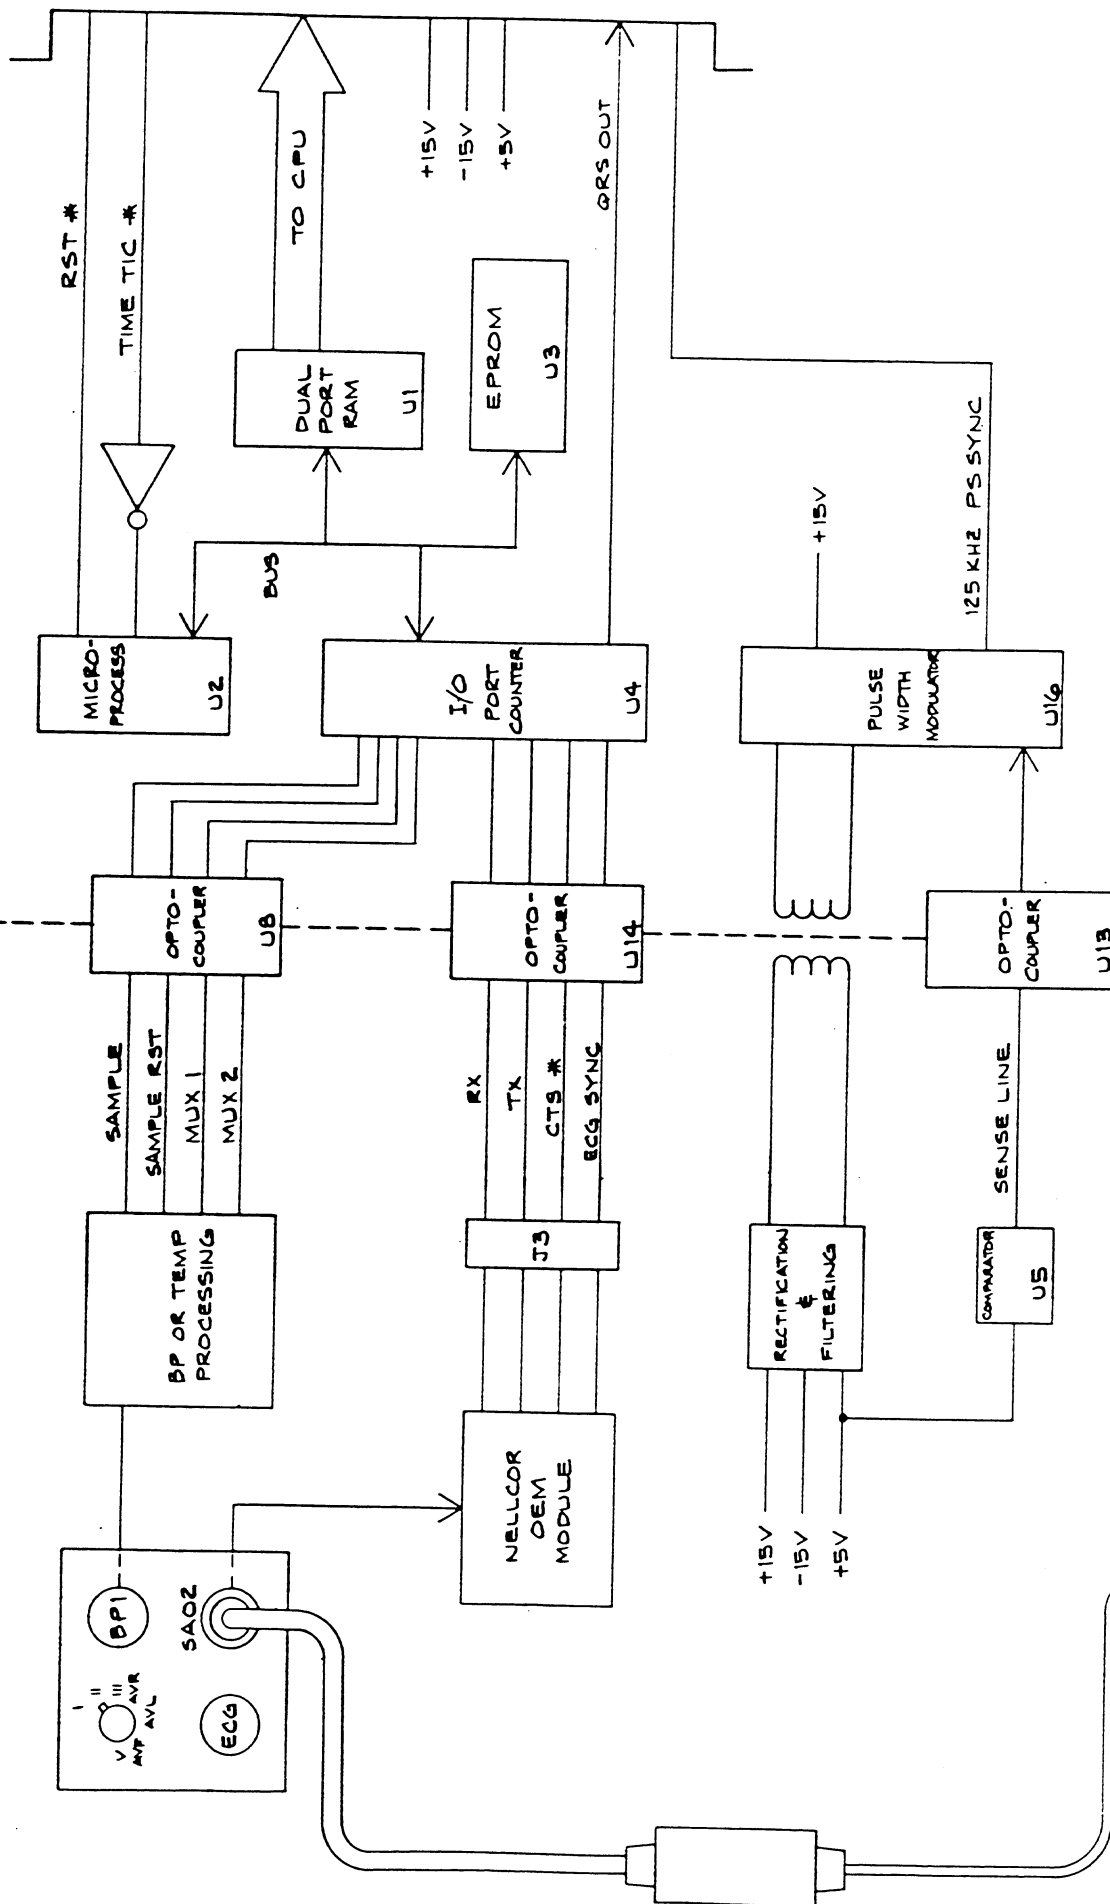

TOLERANCES UNLESS OTHERWISE SPECIFIED	1	2	3	4
FRACTIONS DEC ANGLES	1	2	3	4
APPROVALS	DATE			
DRAWN ATM	12-1-09			
CHECKED				


41 MEDICAL DATA ELECTRONICS


S LEAD-SAO2 (SLOT 2)
DIAGRAM

SCALE	SIZE	DRAWING NO
-------	------	------------

DO NOT SCALE DRAWING


University of Chicago

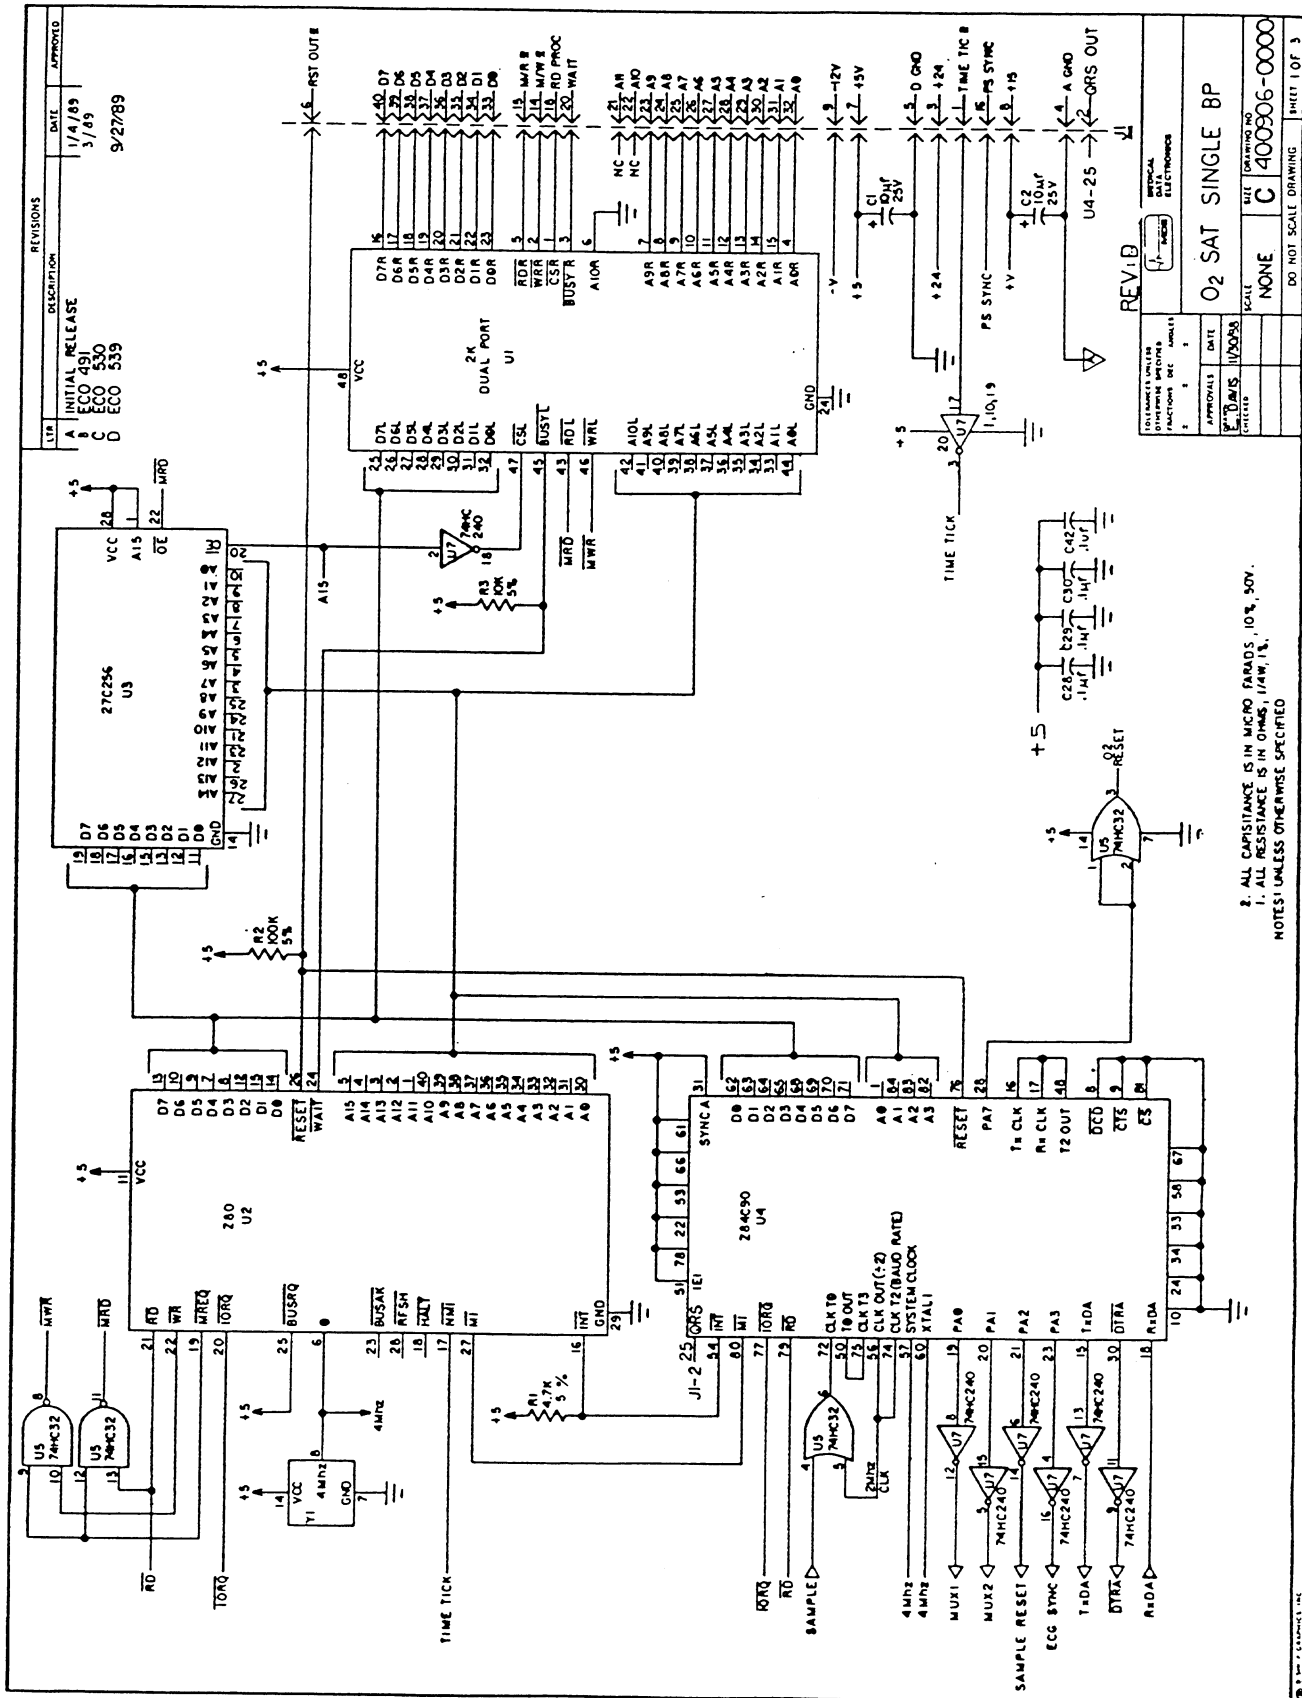

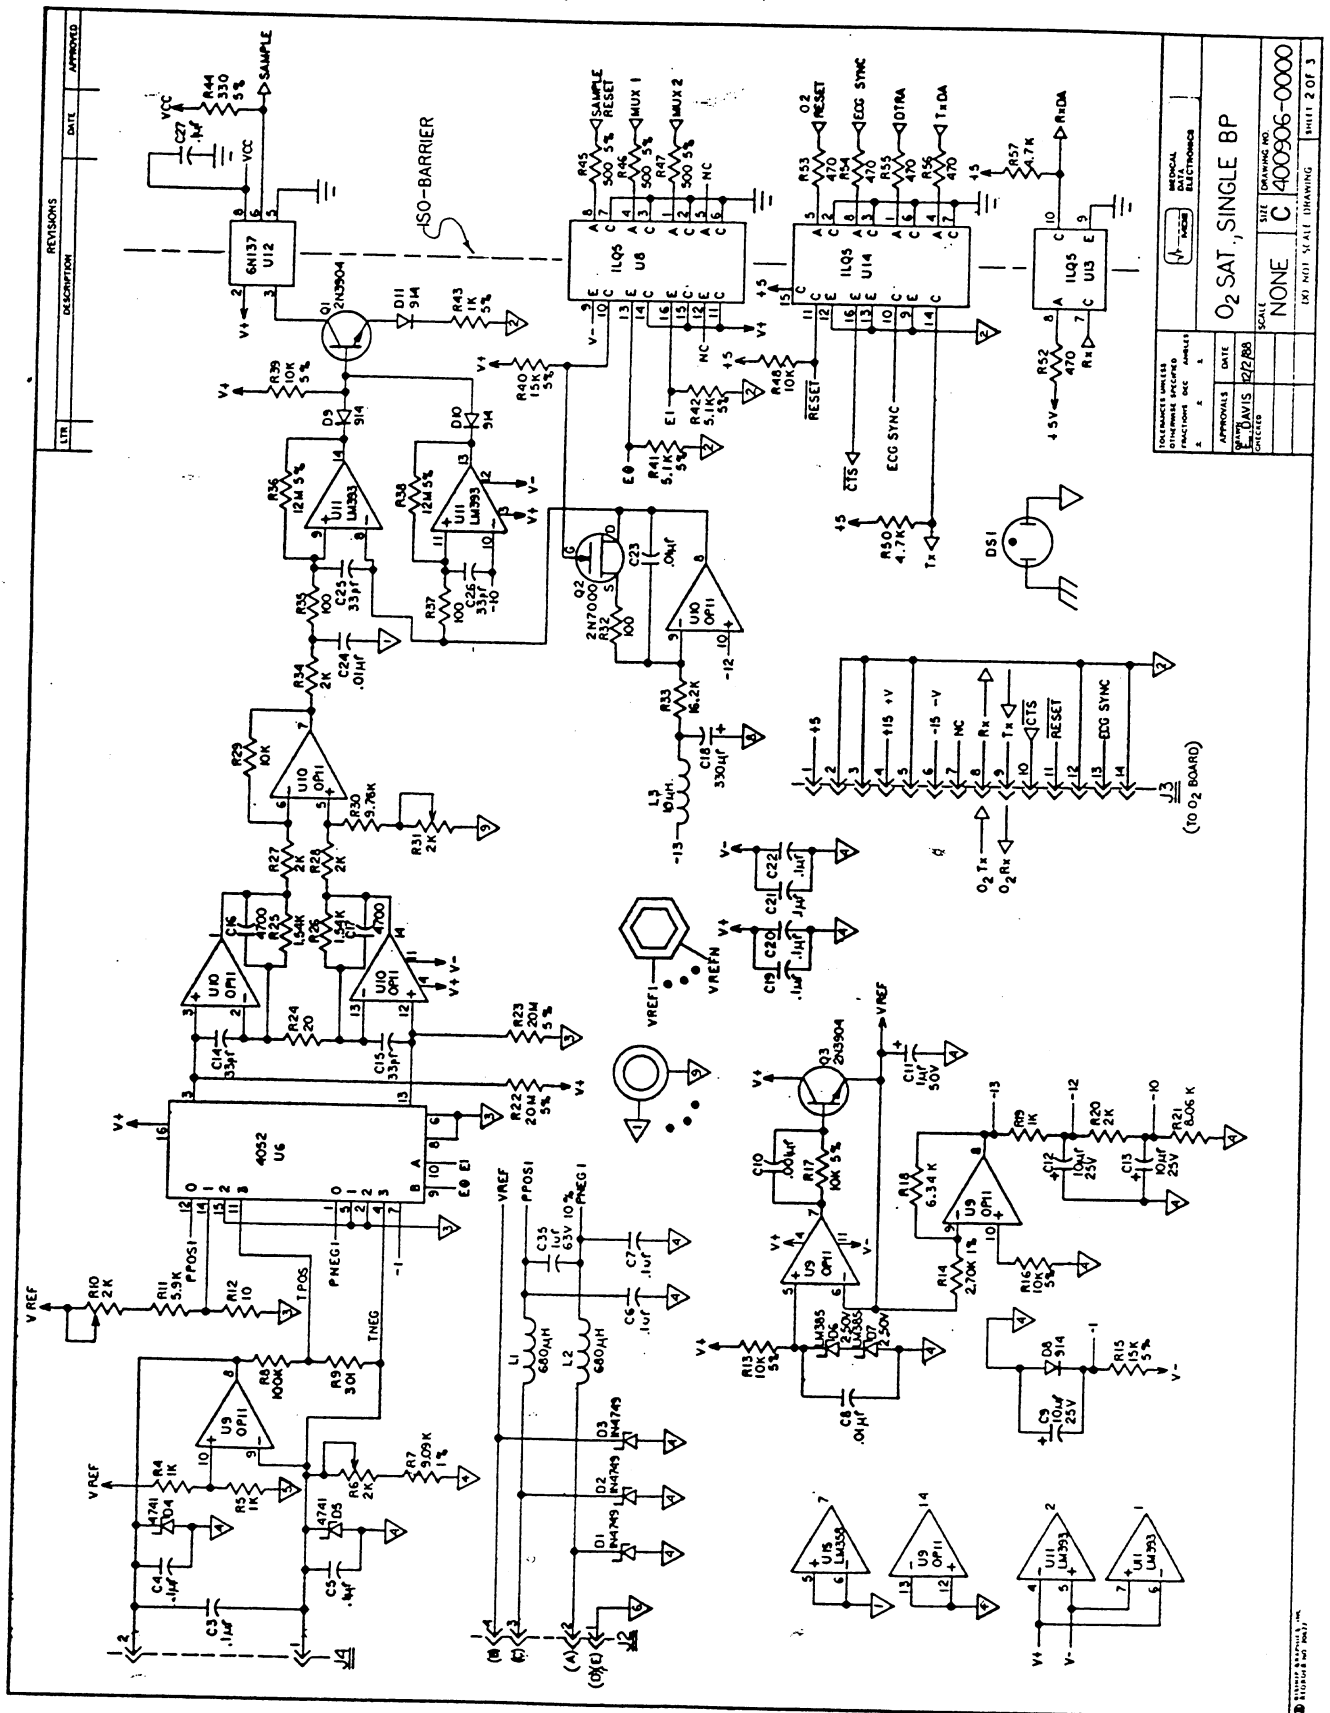


REVISIONS		DATE	APPROVED
1	DESCRIPTION		

LAST USED	NOT USED
C43 D81	R31
D20 J4	
L4 Q5	
R66 T1	
U16 Y1	

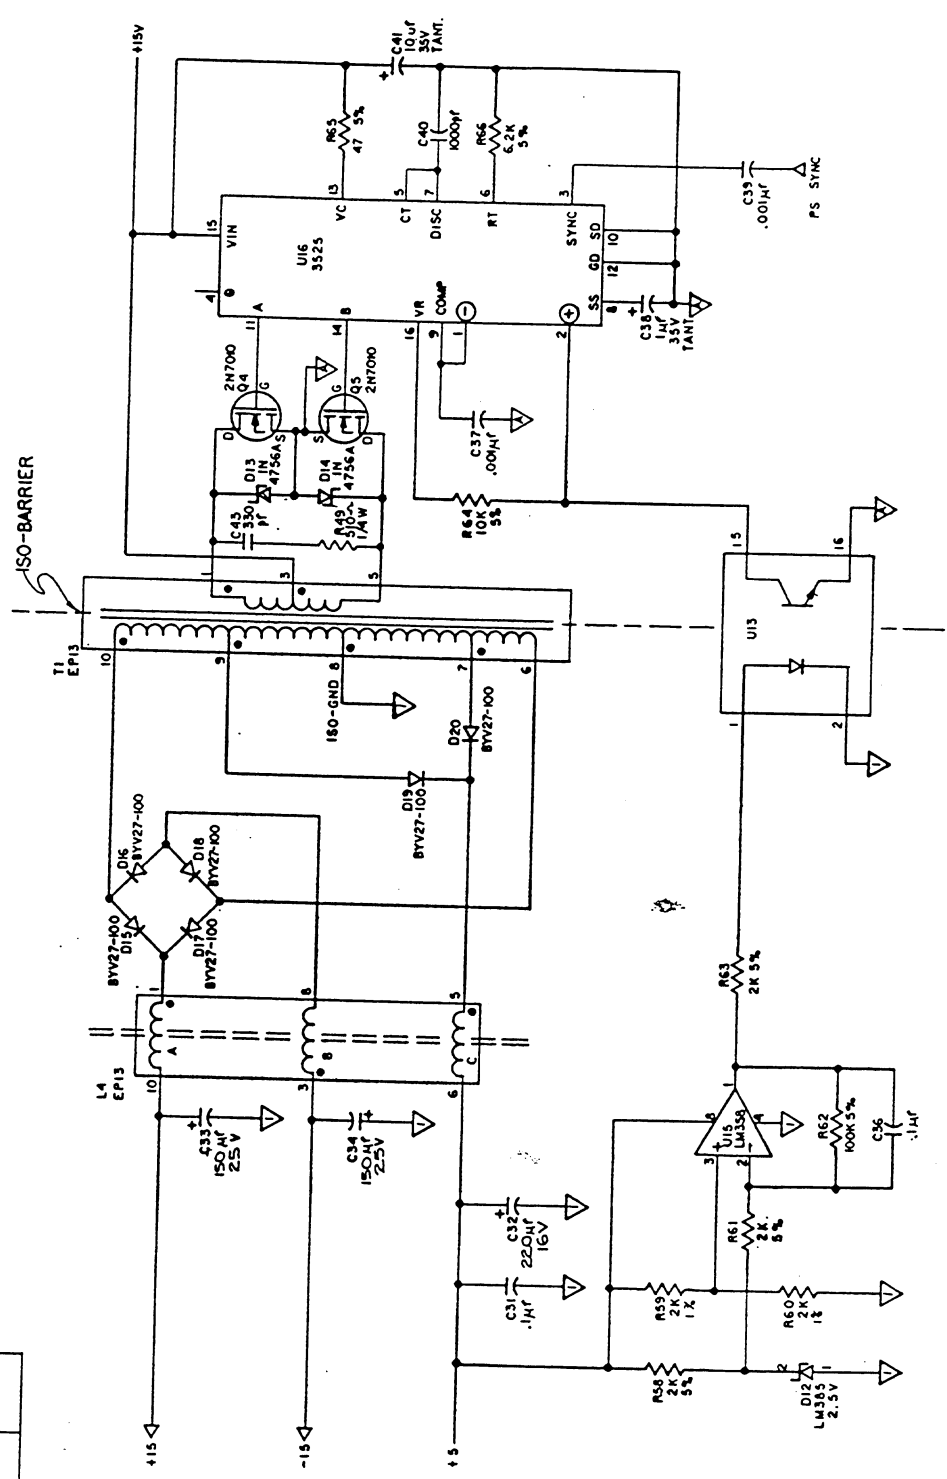

TOLERANCES UNLESS OTHERWISE SPECIFIED		FUNCTIONS SEE ANALYST	2
APPROVALS	DATE	BY	DATE
J. J. JONES	12/5/88		
O2 SAT, SINGLE BP		SCALE	NONE
C 400906-0000		REV	3 OF 3

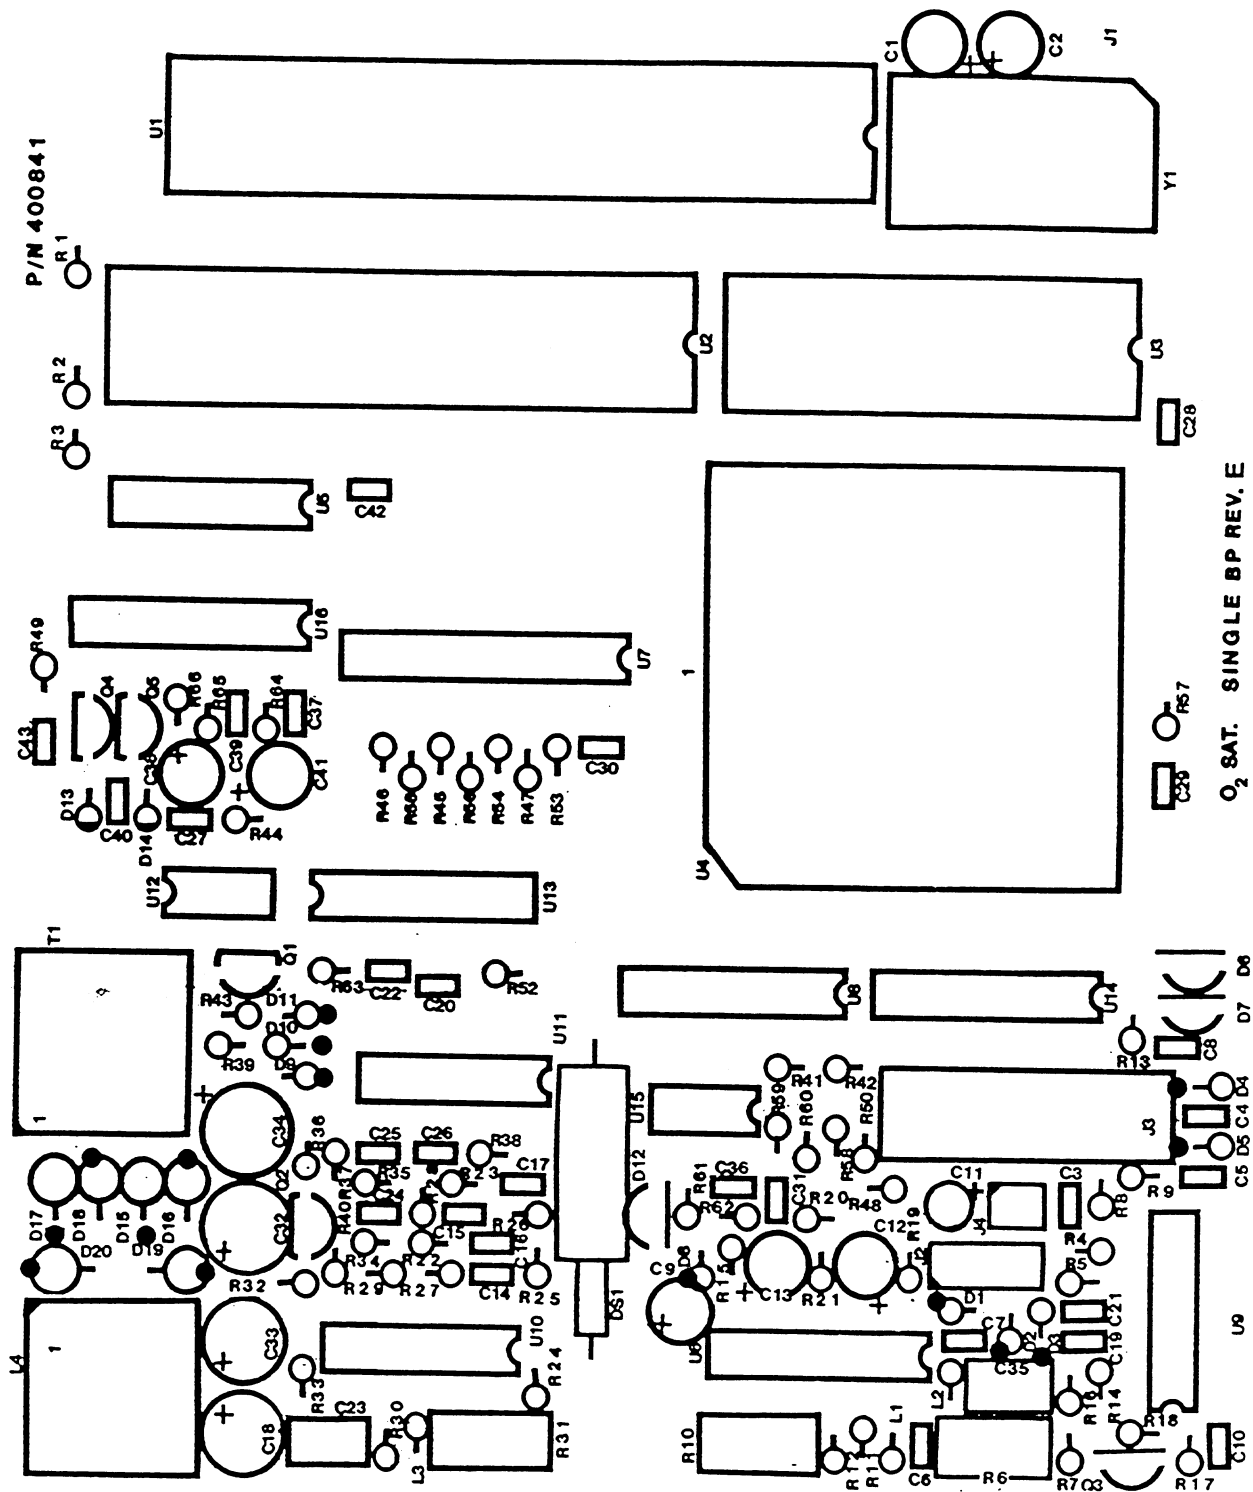

SLOT2 Sao²

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400906-0000 PCBA, 02 SAT. SINGLE BP, REVISION "G" (E787) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
400841-0000	*1	1	PCB, 02 SAT, SNGL. BP, RAW BD, REVISION 'E'	R		33	1.0	EA	-	Yes	
352100-0102A	*1	2	CAP, 1000PF, 50V, 10%, RAD, X 7R	R		11	1.0	EA	C37	Yes	
352300-0104A	*1	3	CAP, .1UF, 50V, 20%, RAD, MYL AR	R		22	7.0	EA	C19, 20, 21, 22, 27, 28, 29	Yes	
352300-0104A	*1	4	CAP, .1UF, 50V, 20%, RAD, MYL AR	R		22	4.0	EA	C30, 31, 36, 42	Yes	
352101-0330A	*1	6	CAP, 33PF, 100V, 5%, RAD, NPO	R		22	4.0	EA	C14, 15, 25, 26	Yes	
352201-0337A	*1	7	CAP, 330UF, 16V, ELEC, RAD	R		22	1.0	EA	C18	Yes	
352300-0007A	*1	8	CAP, .001UF, 10%, MYLAR	R		66	3.0	EA	C10, 39, 40	Yes	
352300-0012A	*1	9	CAP, .01UF, 10%, MYLAR	R		77	2.0	EA	C8, 24	Yes	
352300-0017A	*1	10	CAP, .0047UF, 10%, MYLAR	R		77	2.0	EA	C16, 17	Yes	
352301-0103A	*1	11	CAP, .01UF, 100V, 20%, POLYC ARB, .2 L.S.	R		66	1.0	EA	C23	Yes	
352301-0104A	*1	12	CAP, .1UF, 5%, MYLAR	R		66	4.0	EA	C3, 4, 5, 7	Yes	
352400-0105A	*1	13	CAP, 1UF, 50V, 20%, RAD, TANT , MAX: HT. .28; O.D. .16	R		11	2.0	EA	C11, 38	Yes	
352401-0106A	*1	14	CAP, 10UF, 35V, 20%, RAD, TAN T	R		11	6.0	EA	C1, 2, 9, 12, 13, 41	Yes	
352203-0227A	*1	15	CAP, 220uF, 16V, 20%, RAD, EL ECT, 8mm x 12mm	R		22	1.0	EA	C32	Yes	
352200-0157A	*1	16	CAP, 150uF, 25V, 20%, RAD, EL ECT, 8mm x 12mm	R		22	2.0	EA	C33, 34	Yes	
354000-0103A	*1	17	CONN, SGL ROW, STRT, SGL PI NS, SNAP-AWAY	R		11	4.0	PIN	J2 (4-PIN)	Yes	
354000-0103A	*1	18	CONN, SGL ROW, STRT, SGL PI NS, SNAP-AWAY	R		11	2.0	PIN	J4 (2-PIN)	Yes	
354000-0106A	*1	19	CONN, DBL ROW, STRT, SGL PI NS, SNAP-AWAY	R		11	14.0	PIN	J3 (14-PIN)	Yes	
356000-0008A	*1	20	REF OSCILLATOR, CMOS 4.0M HZ, HIGH SPEED	R		22	1.0	EA	Y1	Yes	
364000-0010A	*1	21	IC, LM339	R		11	1.0	EA	U11	Yes	
364000-0011A	*1	22	IC, LM358	R		11	1.0	EA	U15	Yes	
364000-0027A	*1	23	IC, 74HC32	R		11	1.0	EA	U5	Yes	
364000-0038A	*1	24	IC, 27C256, CMOS, EPROM, 200 NS	R		11	1.0	EA	U3	Yes	
364000-0055A	*1	25	IC, CD4052	R		11	1.0	EA	U6	Yes	
364000-0065A	*1	26	IC, OP11FP, OP AMP	R		11	2.0	EA	U9, 10	Yes	

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400906-0000 PCBA, 02 SAT. SINGLE BP, REVISION "G" (E787) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
364000-0080A	*1	27	IC, TMPZ84C00P (Z80A, CMOS VERSION)	R		11	1.0	EA	U2	Yes	
364000-0091A	*1	28	IC, SG 3525	R		44	1.0	EA	U16	Yes	
364000-0093A	*1	29	IC, ILQ5 QUAD OPTO ISOLAT OR	R		11	3.0	EA	U8,13,14	Yes	
364000-0095A	*1	30	IC, MS6132,DUAL PORT RAM, 8 X 2K,48-PIN (OR MS7132)	R		11	1.0	EA	U1	Yes	
364000-0096A	*1	31	IC, 74HC240	R		11	1.0	EA	U7	Yes	
364000-0099A	*1	32	IC, 6N137	R		11	1.0	EA	U12	Yes	
364000-0131A	*1	33	IC, Z84C9008VSC ZILOG	R		11	1.0	EA	U4 - ISSUE TO TEST	Yes	
365000-0084A	*1	34	SKT, 84-PIN,PLCC	R		22	1.0	EA	U4X	Yes	
370100-0101A	*1	35	RES, 100,1/4W,5%,CF	R		11	3.0	EA	R32,35,37	Yes	
370100-0102A	*1	36	RES, 1K,1/4W,5%,CF	R		11	1.0	EA	R43	Yes	
370100-0103A	*1	37	RES, 10K,1/4W,5%,CF	R		11	7.0	EA	R3,13,16,17,39,48,64	Yes	
370100-0104A	*1	38	RES, 100K,1/4W,5%,CF	R		11	2.0	EA	R2,62	Yes	
370100-0126A	*1	39	RES, 12M,1/4W,5%,CF	R		11	2.0	EA	R36,38	Yes	
370100-0153A	*1	40	RES, 15K,1/4W,5%,CF	R		11	2.0	EA	R15,40	Yes	
370100-0202A	*1	41	RES, 2K,1/4W,5%,CF	R		11	3.0	EA	R58,61,63	Yes	
370100-0206A	*1	42	RES, 20M,1/4W,10%,CF	R		11	2.0	EA	R22,23	Yes	
370100-0331A	*1	44	RES, 330,1/4W,5%,CF	R		11	1.0	EA	R44	Yes	
370100-0470A	*1	45	RES, 47,1/4W,5%,CF	R		11	1.0	EA	R65	Yes	
370100-0471A	*1	46	RES, 470,1/4W,5%,CF	R		11	5.0	EA	R52,53,54,55,56	Yes	
370100-0472A	*1	47	RES, 4.7K,1/4W,5%,CF	R		11	3.0	EA	R1,50,57	Yes	
370100-0511A	*1	48	RES, 510,1/4W,5%,CF	R		11	4.0	EA	R45,46,47,49	Yes	
370100-0512A	*1	49	RES, 5.1K,1/4W,5%,CF	R		11	2.0	EA	R41,42	Yes	
370100-0622A	*1	50	RES, 6.2K,1/4W,5%,CF	R		11	1.0	EA	R66	Yes	
370200-0100A	*1	51	RES, 10,1/4W,1%,MF	R		11	1.0	EA	R12	Yes	
370200-0200A	*1	52	RES, 20,1/4W,1%,MF	R		11	1.0	EA	R24	Yes	

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400906-0000 PCBA, 02 SAT. SINGLE BP, REVISION "G" (E787) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
370200-1001A	*1	53	RES, 1K,1/4W,1%,MF	R		11	3.0	EA	R4,5,19	Yes	
370200-1002A	*1	54	RES, 10K,1/4W,1%,MF	R		11	1.0	EA	R29	Yes	
370200-1003A	*1	55	RES, 100K,1/4W,1%,MF	R		11	1.0	EA	R8	Yes	
370200-1541A	*1	56	RES, 1.54K,1/4W,1%,MF	R		11	2.0	EA	R25,26	Yes	
370200-1622A	*1	57	RES, 16.2K,1/4W,1%,MF	R		11	1.0	EA	R33	Yes	
370200-2001A	*1	58	RES, 2K,1/4W,1%,MF	R		11	6.0	EA	R20,27,28,34,59,60	Yes	
370200-2701A	*1	59	RES, 2.7K,1/4W,1%,MF	R		11	1.0	EA	R14	Yes	
370200-3010A	*1	60	RES, 301,1/4W,1%,MF	R		11	1.0	EA	R9	Yes	
370200-5901A	*1	61	RES, 5.9K,1/4W,1%,MF	R		11	1.0	EA	R11	Yes	
370200-6341A	*1	62	RES, 6.34K,1/4W,1%,MF	R		11	1.0	EA	R18	Yes	
370200-8061A	*1	63	RES, 8.06K,1/4W,1%,MF (8 .05K N/A :OK PER KR)	R		11	1.0	EA	R21	Yes	
370200-9091A	*1	64	RES, 9.09K,1/4W,1%,MF	R		11	1.0	EA	R7	Yes	
370200-9761A	*1	65	RES, 9.76K,1/4W,1%,MF	R		11	1.0	EA	R30	Yes	
374300-0202A	*1	66	POT, 2K,TRIM,SIDE ADJ,CER MET,3/8 SQR,.15LS	R		11	3.0	EA	R6,10,31	Yes	
376000-0003A	*1	67	XSTR, 2N3904	R		11	2.0	EA	Q1,3	Yes	
376000-0019A	*1	68	XSTR, 2N7000,FET	R		11	1.0	EA	Q2	Yes	
376000-0021A	*1	69	XSTR, 2N7010	R		11	2.0	EA	Q4,5	Yes	
378000-0005A	*1	70	DIO, 1N914,SIGNAL	R		11	4.0	EA	D8,9,10,11	Yes	
378000-0011A	*1	71	DIO, 1N4741A,11V,ZENER ** *MOTOROLA ONLY***	R		11	2.0	EA	D4,5	Yes	
378000-0012A	*1	72	DIO, 1N4749A,24V,ZENER ** *MOT ONLY***	R		11	3.0	EA	D1,2,3	Yes	
378000-0034A	*1	73	DIO, LM385,ZENER (XSTR NA TIONAL ONLY)	R		11	3.0	EA	D6,7,12	Yes	
378000-0040A	*1	74	DIO, 1N4756A,47V	R		11	2.0	EA	D13,14	Yes	
378000-0041A	*1	75	DIO, BYV27-150 (OR -100)	R		22	6.0	EA	D15,16,17,18,19,20	Yes	
400988-0000	*1	76	ISO-TRANSFORMER, EP13 SWI TCHING SUPPLY	R		33	1.0	EA	T1	Yes	
382200-0005A	*1	77	CHOKE, 10UH,MOLDED	R		11	1.0	EA	L3	Yes	

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
400906-0000 PCBA, 02 SAT. SINGLE BP, REVISION "G" (E787) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
382200-0015A	*1	78	CHOKE, 680 UH	R		11	2.0	EA	L1,2	Yes	
400989-0000	*1	79	MULTI-INDCTR, EP13	R		22	1.0	EA	L4	Yes	
384000-0061A	*1	80	GAS TUBE (SURGE ARRESTER)	R		33	1.0	EA	DS1	Yes	
365000-0040A	*1	81	SKT, 40-POS,DIP,TIN PLATE ,L.P.	R		11	1.0	EA	U2	Yes	
365000-0148A	*1	82	SOCKET, 48 PIN DIP	R		22	1.0	EA	U1	Yes	
365000-0028A	*1	83	SKT, 28-POS,DIP,TIN PLATE ,L.P.	R		11	1.0	EA	U3	Yes	
352100-0331A	*1	84	CAP, 330PF,25V,10%,RAD,X7 R	R		22	1.0	EA	C43	Yes	
352301-0105A	*1	85	CAP, 1UF,63V,20%,MYLAR	R		22	1.0	EA	C35	Yes	
352100-0104A	*1	86	CAP, .1UF,50V,10%,RAD,X7R	R		11	1.0	EA	C6	Yes	

Cumulative Lead Time for 400906-0000 = 77

SWITCHING POWER SUPPLY BOARD

CHAPTER 8

8.0.0 SWITCHING POWER SUPPLY BOARD WITH BATTERY CHARGER

8.1.0 OVERVIEW

The Switching Power Supply Board provides the flexibility to operate the ESCORT via two separate input circuits, along with producing DC operating voltages used throughout the monitor. The DC voltages are regulated by a sense line on the +15V output. Battery level indication originates on this board and the battery charging circuitry is incorporated into the design.

8.2.0 INPUT CIRCUITS

The ESCORT monitor can be powered by two different input modes. The monitor can be:

1. Plugged into an AC outlet, or
2. Powered by internal battery packs

When the ESCORT is plugged into an AC outlet, AC power passes through the power transformer. This steps down the line voltage to approximately 17 VAC and provides line power isolation. Full wave rectification is completed by the Bridge Rectifier CR1. The capacitors C13, C14, C15, C17, C30, and C31 filter the DC voltage.

The ON/STBY switch interrupts V_{in} to the pulse width modulator, U2. Local oscillation comes from R14, R15, and C7, which provide a free running frequency to the regulator. Pin 3 of U2 is a 250 KHz synchronizing input signal from the CPU, which will preempt the local oscillation. This signal assists in reducing beat frequency noise on ECG and other circuits. It also keeps all output voltages in phase with each other. C11 and R13 compensate for and stabilize the frequency. A soft start occurs when C8 slowly charges to capacity. The switching outputs of U2 pins 11 and 14 go to the high power MOSFET transistors Q3 and Q4. They, in turn, drive the transformer T1. Clamping diodes, D2 and D3, provide spike protection for Q3 and Q4. The voltages derived from T1 are +24V, +15V, +7.5V, -15V, and -17V.

8.2.1 VOLTAGE SENSE

Because the +15V output has the largest demand for power consumption, it is used by U2 for voltage regulation. A voltage feedback signal for a closed loop operation provides a sense line to U2 pin 1. U2 will vary the duty cycle of its switching output pins 11 and 14 to maintain the regulated output of +15V. Mutual inductance from windings in T1 keep all of the other voltages at a constant. Each of the voltages have their own rectifying and L.C. circuits to provide AC ripple filtering.

8.2.2 INDICATORS AND SIGNALS

Also contained on the Power Supply Board are battery level and AC detect signals (BATT LEVEL and AC DETECT). BATT LEVEL, found at J5 pin 11, is sent to the CPU for evaluation to determine the charge level of the batteries. If AC is supplying the ESCORT with power then AC DETECT at J5 pin 5 will be high. The AC LED will be enabled at J2 pin 2 and controlled by the AC LIGHT signal. When being powered by the battery packs, the signal will be pulled low by circuitry on the Battery Charger Section.

8.3.0 BATTERY CHARGING CIRCUITRY

8.3.1 OVERVIEW

After AC voltage enters the charging circuit, it is full wave rectified and filtered. A current sensing circuit checks battery level for fully charged or not-fully charged condition.

If the batteries are not fully charged, voltage regulators will charge them at 150 mA. Current limiting is internal to the regulators. To prevent excessive power consumption, the signal BATT CHG CTRL from the CPU will not allow charging when the recorder is in use. When charging current is active, it passes through blocking diodes and on to the batteries. The two diodes provide discharge protection for the PCBA.

8.3.2 CURRENT SENSING

Current sensing (for charging status) is done by U3, a comparator that measures the difference at pin 2 and 3. If pin 3 is higher than pin 2, the output at pin 1 is low. This provides a path for the voltage regulators. By redirecting in this way, the batteries cease to be charged.

If 85 mA or more is sensed, the batteries are in the charging mode and the charging voltage is +15V. The CHG LED will be "ON". If less than 85 mA is sensed, the batteries are fully charged and the voltage drops to approximately 13.8V. The CHG LED will be "OFF".

8.3.3 TEMPERATURE COMPENSATION


A temperature compensating circuit composed of D11 and D13 adjusts charging voltage by increasing or decreasing load as temperature rises or falls within the unit.

8.3.4 VOLTAGE REGULATING


Voltage regulation for the charge circuitry is done by U4 and U5. These regulators offer internal current limiting (constant with temperature), thermal overload protection and safe area protection. This will prevent damage to the batteries by providing proper voltage levels. Optimal charging voltages are achieved at the factory by adjusting R41 and R48.

8.3.5 DISCHARGE PROTECTION


The diodes D12 and D15 provide discharge protection to the circuit by blocking the path from the batteries.

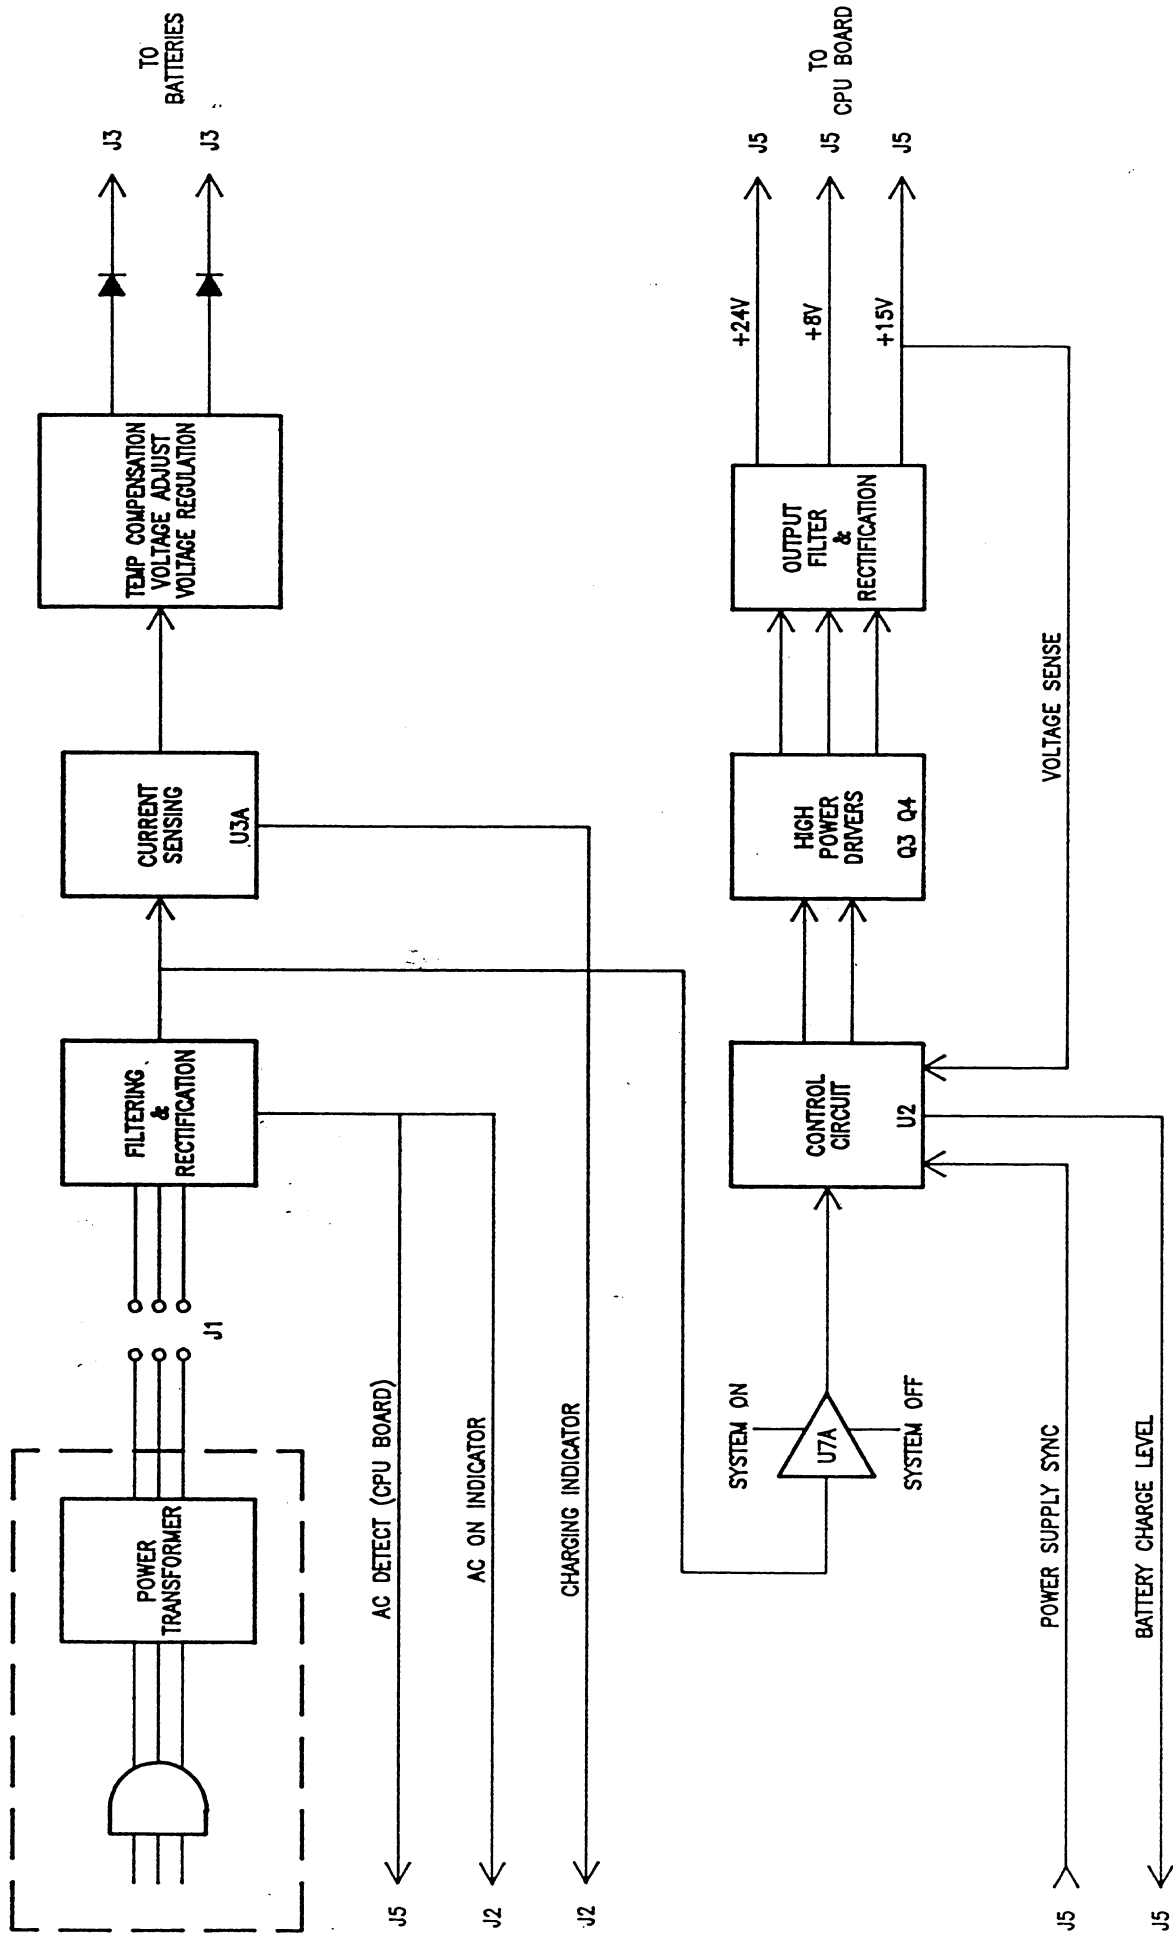

ESCORT III SWITCHING POWER SUPPLY BOARD
BLOCK DIAGRAM

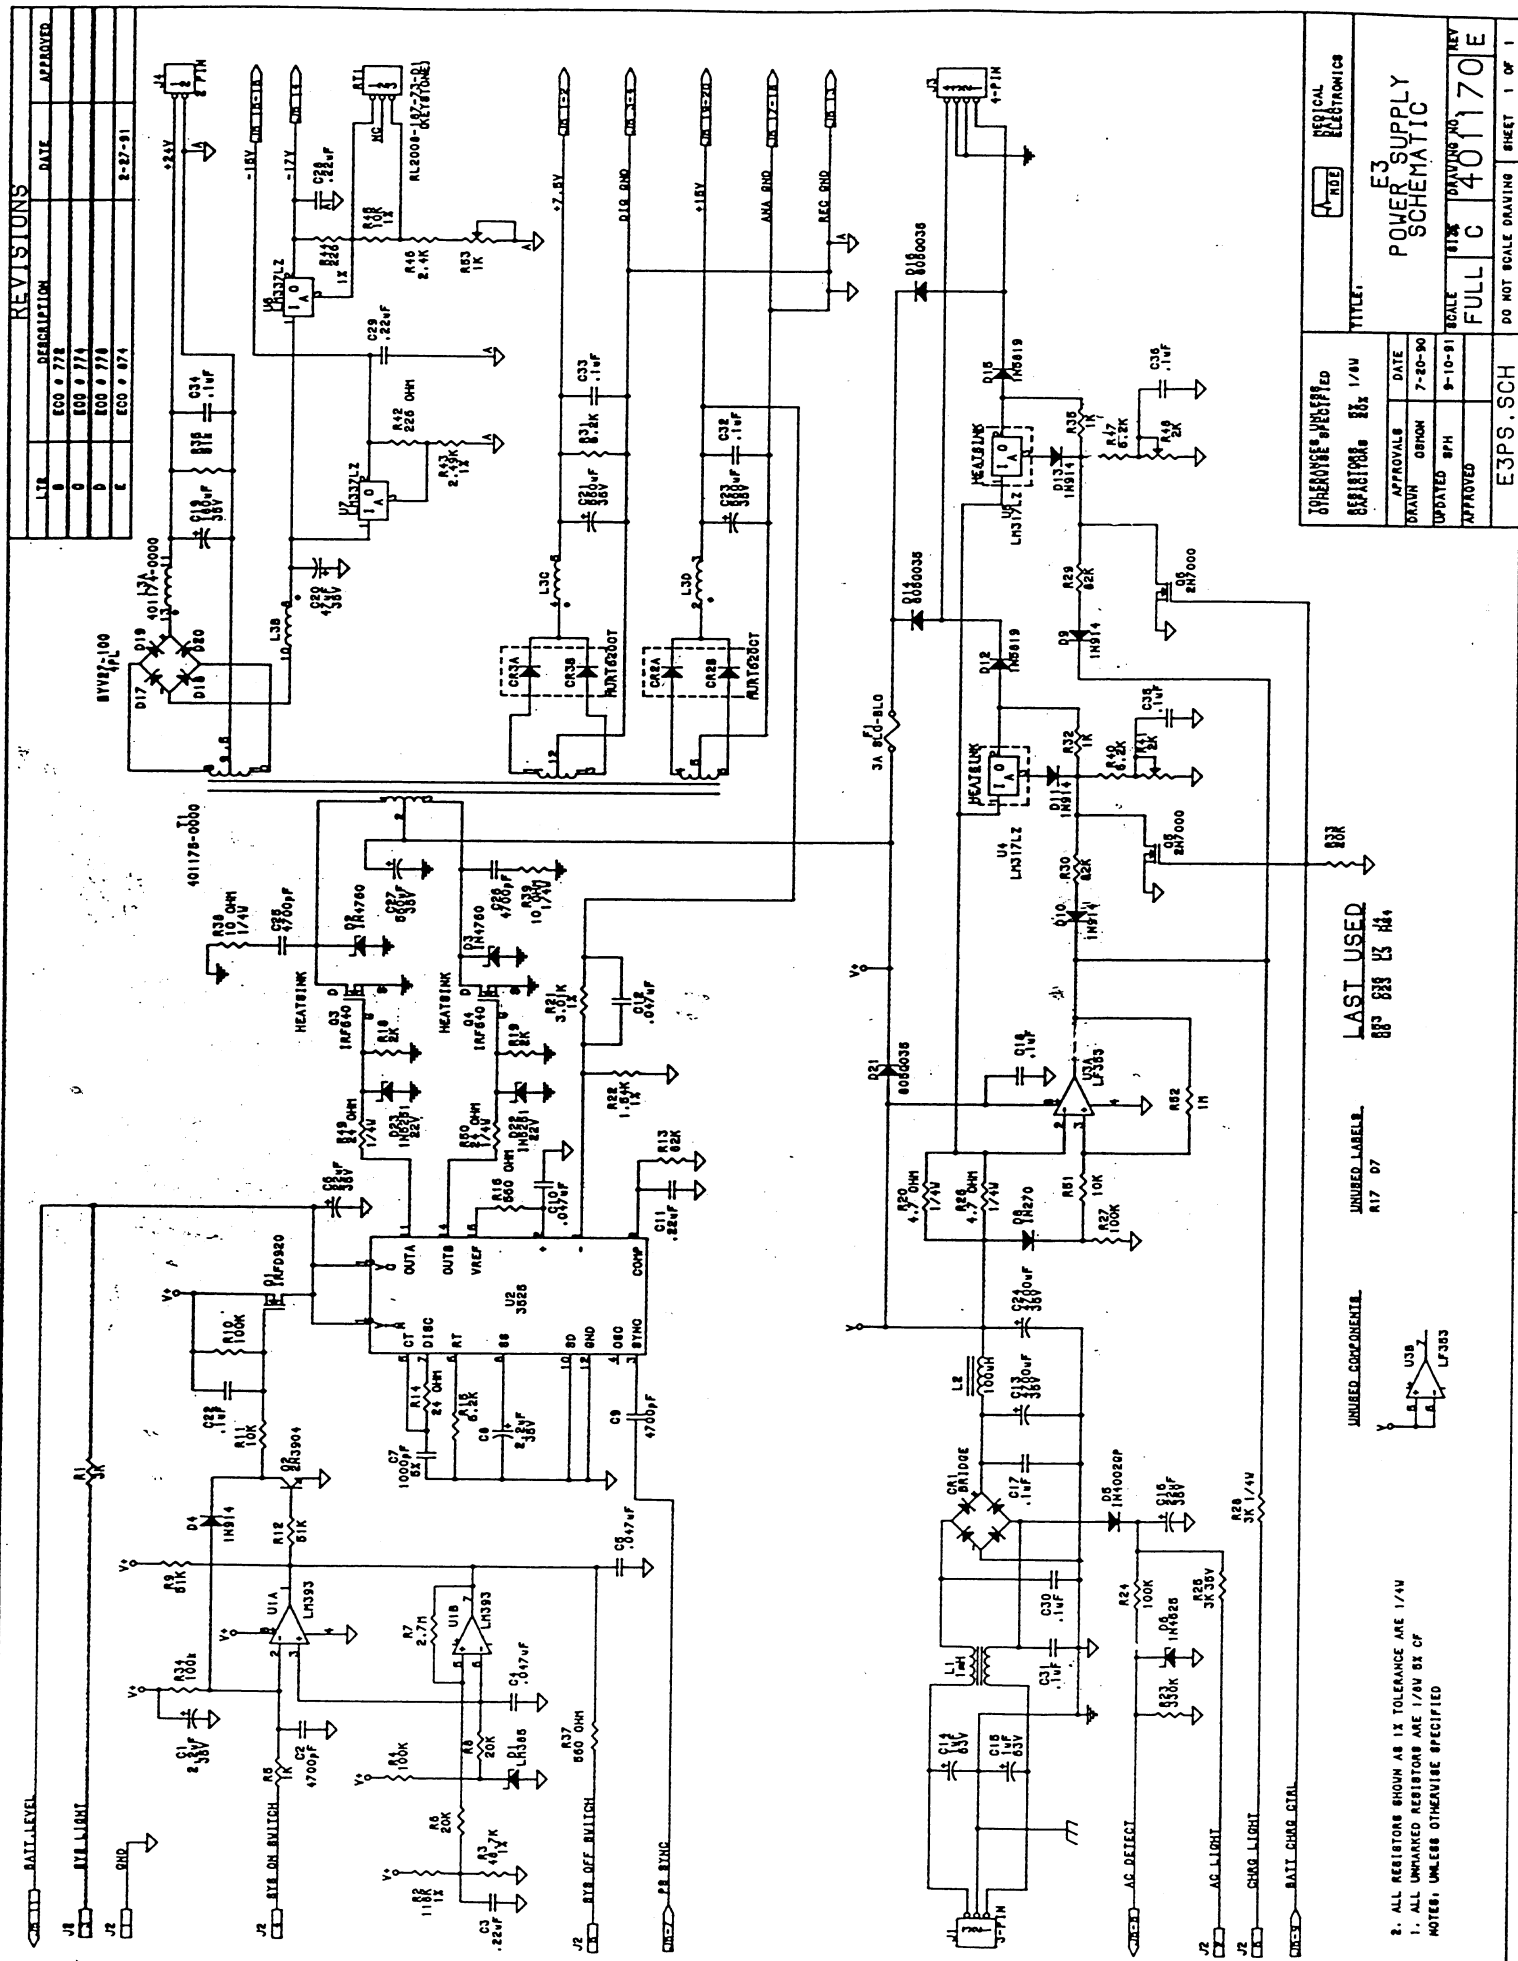

2. ALL RESISTORS SHOWN AS 1% TOLERANCE ARE 1/4W
1. ALL UNMARKED RESISTORS ARE 1/8W 5% CF
NOTES: UNLESS OTHERWISE SPECIFIED

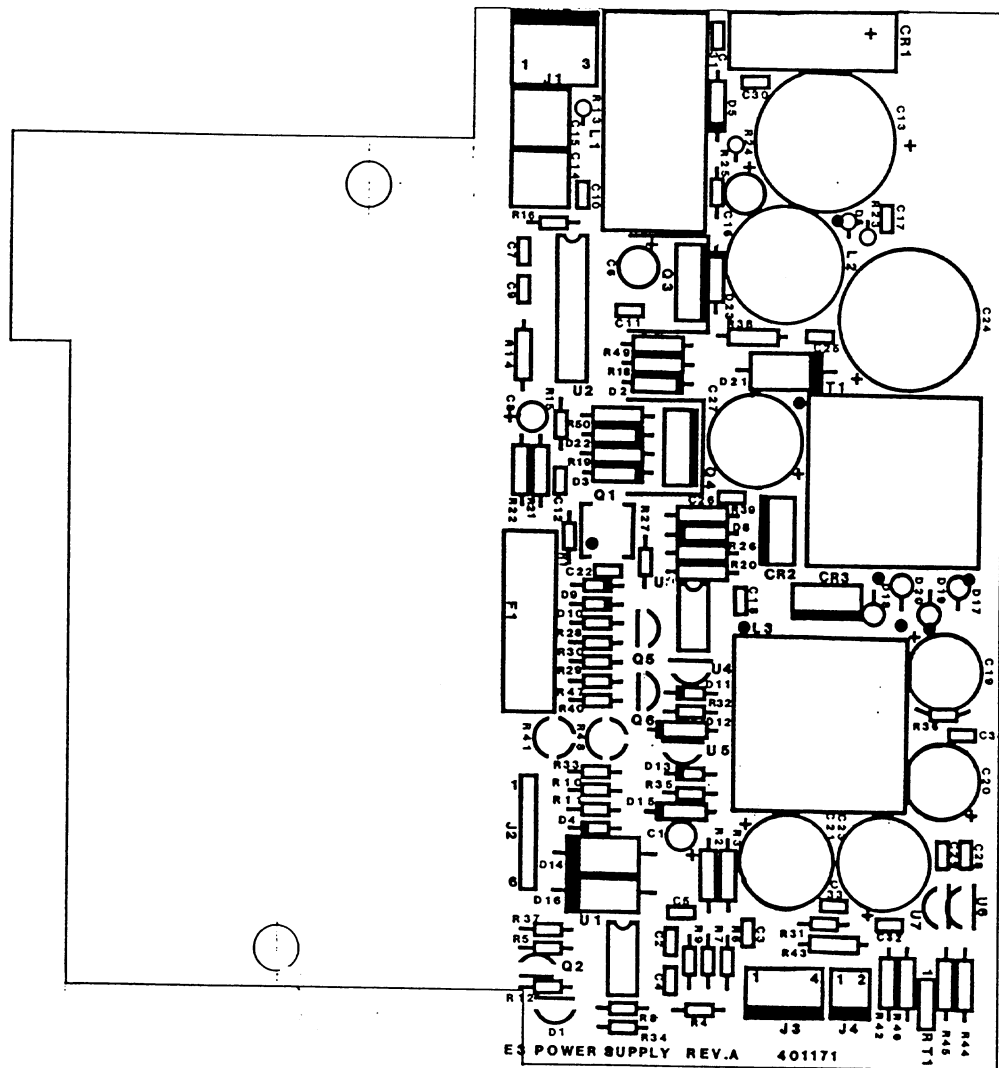

POWER SUPPLY

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
401170-0000 PCBA, E3 POWER SUPPLY REV. D1 (D007) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
401171-0000	*1	1	PCB, E3 POWER SUPPLY REV. B	R		33	1.0	EA	-	Yes	
352300-0104A	*1	2	CAP, .1UF,50V,20%,RAD,MYLAR	R		22	5.0	EA	C17,18,30,31,32	Yes	
352300-0104A	*1	3	CAP, .1UF,50V,20%,RAD,MYLAR	R		22	3.0	EA	C33,34,22	Yes	
352201-0476A	*1	4	CAP, 47UF,35V,RAD,ELECT,S	R		22	1.0	EA	C20	Yes	
352300-0010A	*1	5	WTCH SP TYPE,10X16MM								
352300-0010A	*1	5	CAP., .001UF,5%,MYLAR SOR	R		66	1.0	EA	C7	Yes	
352300-0224A	*1	6	T FROM 352300-0007A								
352300-0224A	*1	6	CAP, .22UF,50V,20%,MYLAR	R		22	2.0	EA	C3,11	Yes	
352200-0226A	*1	7	CAP, 22UF,35V,RAD,ELECT	R		22	2.0	EA	C6,16	Yes	
352301-0105A	*1	8	CAP, 1UF,63V,20%,MYLAR	R		22	2.0	EA	C14, C15	Yes	
352300-0472A	*1	9	CAP, .0047UF,50V,20%,MYLAR	R		22	5.0	EA	C2,9,12,25,26	Yes	
352300-0473A	*1	10	CAP, .047UF,50V,20%,MYLAR	R		22	3.0	EA	C4,5,10	Yes	
352200-0567A	*1	11	CAP, 560uF,35V,LOW ESR,EL	R		33	3.0	EA	C21,23,27	Yes	
352401-0225A	*1	12	ECT (12.5 x 20mm)								
352401-0225A	*1	12	CAP, 2.2UF,35V,20%,TANT	R		11	4.0	EA	C1,8,28,29	Yes	
354000-0148A	*1	13	CONN, 4-P,M,STRT,.1 CTR,L	R		11	1.0	EA	J3	Yes	
354000-0085A	*1	14	OCKING RAMP								
354000-0085A	*1	14	CONN, 3-PIN,M,STRT LCK,.1	R		11	1.0	EA	J1	Yes	
354000-0103A	*1	15	56 CTR								
354000-0103A	*1	15	CONN, SGL ROW,STRT,SGL PI	R		11	1.0	PIN	J2	Yes	
354000-0222A	*1	16	NS,SNAP-AWAY								
354000-0222A	*1	16	CONN, 2-PIN,LOCKING	R		22	1.0	EA	J4	Yes	
360300-0007A	*1	17	FUSE, HLDR	R		11	2.0	EA	F1	Yes	
360300-0023A	*1	18	FUSE, 3A SLOW-BLOW (5X20M	R		22	1.0	EA	F1	Yes	
364000-0064A	*1	19	M)								
364000-0064A	*1	19	IC, LM317LZ,VOLT. REGULAT	R		11	2.0	EA	U4, U5	Yes	
364000-0091A	*1	20	OR								
364000-0091A	*1	20	IC, SG 3525	R		44	1.0	EA	U2	Yes	
364000-0144A	*1	21	IC, LM393N,DUAL COMP	R		33	1.0	EA	U1	Yes	
364000-0145A	*1	22	IC, LF353N,DUAL OPAMP	R		33	1.0	EA	U3	Yes	
370200-1183A	*1	23	RES, 118K,1/4W,1%,MF	R		11	1.0	EA	R2	Yes	
370100-0103A	*1	24	RES, 10K,1/4W,5%,CF	R		11	1.0	EA	R45	Yes	
370100-0302A	*1	25	RES, 3K,1/4W,5%,CF	R		11	3.0	EA	R1, R25, R28	Yes	

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
401170-0000 PCBA, E3 POWER SUPPLY REV. D1 (D007) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
370200-4872A	*1	26	RES, 48.7K,1/4W,1%,MF	R		11	1.0	EA	R3		Yes
370101-0102A	*1	27	RES, 1K,1/8W,5%,CF	R		11	3.0	EA	R5,32,35		Yes
370101-0103A	*1	28	RES, 10K,1/8W,5%,CF	R		11	1.0	EA	R11		Yes
370101-0104A	*1	29	RES, 100K,1/8W,5%,CF	R		11	4.0	EA	R4,10,24,34		Yes
370200-2260A	*1	30	RES, 226 OHM, 1/4W, 1%	R		22	2.0	EA	R42,44		Yes
370101-0275A	*1	31	RES, 2.7K,1/8W,5%,CF	R		11	1.0	EA	R7		Yes
370100-0100A	*1	32	RES, 10,1/4W,5%,CF	R		11	2.0	EA	R38,39		Yes
370101-0202A	*1	33	RES, 2K,1/8W,5%,CF	R		11	2.0	EA	R18,19		Yes
370101-0203A	*1	34	RES, 20K,1/8W,5%,CF	R		11	3.0	EA	R6,8,33		Yes
370100-0240A	*1	35	RES, 24,1/4W,5%,CF	R		11	3.0	EA	R14,49,50		Yes
370101-0513A	*1	36	RES, 51K,1/8W,5%,CF	R		11	2.0	EA	R12,36		Yes
370101-0334A	*1	37	RES, 330K,1/8W,5%,CF	R		11	1.0	EA	R23		Yes
370101-0561A	*1	38	RES, 560,1/8W,5%,CF	R		11	2.0	EA	R16,37		Yes
370101-0622A	*1	39	RES, 6.2K,1/8W,5%,CF	R		11	4.0	EA	R15,31,40,47		Yes
370101-0823A	*1	40	RES, 82K,1/8W,5%,CF	R		11	1.0	EA	R13		Yes
370100-0047A	*1	41	RES, 4.7,1/4W,5%,CF	R		11	2.0	EA	R20,26		Yes
370200-2491A	*1	42	RES, 2.49K,1/4W,1%,MF	R		11	1.0	EA	R43		Yes
370200-1541A	*1	43	RES, 1.54K,1/4W,1%,MF	R		11	1.0	EA	R22		Yes
370200-3011A	*1	44	RES,3.01K, 1/4W 1%, MF	R		11	1.0	EA	R21		Yes
374100-0202A	*1	45	POT, 2K,TRIM,TOP ADJ,CTRD LEADS,CERNET	R		11	2.0	EA	R41,48		Yes
376000-0003A	*1	46	XSTR, 2N3904	R		11	1.0	EA	Q2		Yes
376000-0017A	*1	47	XSTR,BUK456-100A,100V,24A ,PWR (T0-220)MOSFET ONLY	R		11	2.0	EA	Q3, Q4		Yes
376000-0019A	*1	48	XSTR, 2N7000,PET	R		11	2.0	EA	Q5, Q6		Yes
376000-0022A	*1	49	XSTR, IRFD9020,PWR MOSFET	R		33	1.0	EA	Q1		Yes
378000-0001A	*1	50	DIO, 1N270	R		11	1.0	EA	D8		Yes

Assembly Description Group PFC Commodity Class Planner Buyer Drawing
401170-0000 PCBA, E3 POWER SUPPLY REV. D1 (D007) A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
378000-0002A	*1	51	DIO, 1N4002GP, RECTFR, (MOT ONLY)	R		11	1.0	EA	D5		Yes
378000-0005A	*1	52	DIO, 1N914, SIGNAL	R		11	5.0	EA	D4, 9, 10, 11, 13		Yes
378000-0021A	*1	53	DIO, 1N4760, 68V, 10%, ZENER ***MOT ONLY***	R		11	2.0	EA	D2, D3		Yes
378000-0023A	*1	54	DIO, 80SQ035 8A RECTIFIER (OR 040 OR 045)	R		44	3.0	EA	D14, 16, 21		Yes
378000-0026A	*1	55	DIO, 1N4625 (OR 1N4628)	R		11	1.0	EA	D6		Yes
378000-0033A	*1	57	DIO, MUR1620CT, 200V, 16A, R CTFR, ULTRAFAST, COM ANOD	R		11	2.0	EA	CR2, 3		Yes
378000-0034A	*1	58	DIO, LM385, ZENER (XSTR NA TIONAL ONLY)	R		11	1.0	EA	D1		Yes
378000-0036A	*1	59	DIO, 1N5819, 1AMP, SCHOTTKY	R		11	2.0	EA	D12, D15		Yes
378000-0041A	*1	60	DIO, BYV27-150 (OR -100)	R		22	4.0	EA	D17, 18, 19, 20		Yes
378000-0051A	*1	62	DIODE, 1N5251, 12V, ZENER	R		33	2.0	EA	D22, 23		Yes
360600-0046A	*1	63	HEATSINK, T0-202 & T0-220	R		22	2.0	EA	HS1, 2		Yes
360600-0024A	*1	64	HTSNK, IERC RUC671B	R		22	2.0	EA	HS3, 4		Yes
382200-0025A	*1	65	CHOKE, 1mH, 6 AMP, COMMON M ODE	R		33	1.0	EA	L1		Yes
401174-0000	*1	66	INDUCTOR, MULTI, E3 PWR SUP PLY, 4 ELEMENT REV. "A"	R		33	1.0	EA	L3		Yes
401175-0000	*1	67	XFMR, SWITCHING, E3 PWR SU PPLY REV. "A"	R		33	1.0	EA	T1		Yes
384000-0118A	*1	68	THERMISTOR, NTC R=300 OHM	R		22	1.0	EA	RT1		Yes
352201-0478A	*1	69	CAP, 4700 UF, 35V, ELECT. (18X40MM)	R		22	2.0	EA	C13, 24		Yes
352200-0187A	*1	70	CAP., 180 UF, 35V, ELECT. LOW ESR	R		22	1.0	EA	C19		Yes
378000-0052A	*1	71	RECTIFIER, 8AMP BRIDGE 20 0V	R		22	1.0	EA	CR1		Yes
364000-0116A	*1	72	IC, LM337LZ, VOLT. REGULAT OR, T0-92 CASE	R		22	2.0	EA	U6, 7		Yes
382200-0026A	*1	73	CHOKE, 100uH, 6 AMP, POWER	R		33	1.0	EA	L2		Yes
358100-0013A	*1	74	SCR, 4-40 X 3/8, PH PNHD, C AD1	R		11	2.0	EA	FOR MOUNTING HS		Yes
358200-0001A	*1	75	WSHR, SHLDR	R		11	2.0	EA	FOR MOUNTING HS		Yes
360500-0022A	*1	76	NUT, #4 HEX, LRG PTFRN	R		11	2.0	EA	FOR MOUNTING HS		Yes
358200-0009A	*1	77	WSHR, #4 SPLIT LOCK	R		11	2.0	EA	FOR MOUNTING HS		Yes

Medical Data Electronics
MANUFACTURING BOM WITH LABOR AND PROCESS

Description
PCBA, E3 POWER SUPPLY REV. D1 (D007)

Group PFC Commodity Class Planner Buyer Drawing
A

ITEM	LEVEL	SEQ.	DESCRIPTION	REV	CL	LT	QUANTITY	U/M	REFERENCE	MLT	BEGIN
358200-0004A	*1	78	WSHR, #4 FLAT STL CAD1, (.125ID,9/32OD,.025THK)	R		11	2.0	EA	FOR MOUNTING HS	Yes	
360500-0040A	*1	79	HARDWARE, ISO-THERM PAD, T0-220	R		11	2.0	EA	FOR T0-220	Yes	
365000-0008A	*1	80	SKT, 8-POS,DIP,TIN PLATE, L.P.	R		11	2.0	EA	XU1,XU3	Yes	
365000-0016A	*1	81	SKT, 16-POS,DIP,TIN PLATE ,L.P.	R		11	1.0	EA	XU2	Yes	
370101-0913A	*1	82	RES, 91K,1/8W,5%,CF	R		11	2.0	EA	R29,30	Yes	
370101-0203A	*1	83	RES, 20K,1/8W,5%,CF	R		11	1.0	EA	R27	Yes	
370101-0103A	*1	84	RES, 10K,1/8W,5%,CF	R		11	1.0	EA	R51	Yes	
370101-0105A	*1	85	RES, 1M,1/8W,5%,CF	R		11	1.0	EA	R52	Yes	
370101-0683A	*1	86	RES, 68K,1/8W,5%,CF	R		22	1.0	EA	R9	Yes	
370200-2701A	*1	87	RES, 2.7K,1/4W,1%,MF	R		11	1.0	EA	R46	Yes	
352100-0104A	*1	88	CAP, .1UF,50V,10%,RAD,X7R	R		11	2.0	EA	C35,36	Yes	
360500-0085A	*1	89	STANPOFF SWAGE 4-40X1/8" LG	R		22	2.0	EA		Yes	

Ma. 2000

PERFORMANCE CHECK

CHAPTER 9

9.0.0 PERFORMANCE CHECK

9.1.0 OVERVIEW

MDE recommends a yearly performance check to verify all functions on the ESCORT 300A. A calibrated patient simulator, such as the MDE DATASIM Model 2000 or 6000, will be necessary to complete the performance check.

Begin with a thorough visual inspection of the unit, paying particular attention to the power cord.

9.2.0 BATTERIES

Note: Medical Data Electronics suggests battery replacement every two (2) years regardless of test results. Batteries used beyond life expectancy may fail without notice and could disrupt power to the ESCORT monitor.

All lead-acid battery packs should be fully charged prior to performance check; refer to Chapter 6 for charging procedures. If in doubt, charge the batteries.

Connect the ESCORT monitor to a 120 VAC, 60Hz power source. Set the AC switch located on the rear panel of the ESCORT to the "I" position. The yellow *battery charging* LED located on the front of the ESCORT should be off and the green *AC ON* LED should be on. If the yellow charging LED is on, allow the batteries to fully charge until the time when the LED turns off.

Turn the AC switch to the "0" position; observe if the monitor operates under battery power. Access the soft key TEST page to view battery status (i.e., HIGH, MID, LOW). Battery status should read: **MONTR BAT HI 12.8V** (voltage will vary)

Turn the ON/STBY switch to STBY, turn the AC switch on the rear panel to the "0" position. Remove the two lead-acid battery packs and measure the voltage with an open load, the voltage should measure approximately 13.0 to 13.5 volts.

Next, cycle the lead-acid battery packs individually as follows:

- i. Insure that ON/STBY switch is in STBY position
- ii. Insure that AC switch is in "0" position
- iii. Insert one battery pack into one of the battery slots
- iv. Turn the ON/STBY switch to the ON position
- v. Confirm that the ESCORT monitor operates and Battery Level indicates HIGH
- vi. Turn the ON/STBY switch to STBY position
- vii. Remove battery pack and install into adjacent slot
- viii. Repeat steps "iii" through "vii" for both battery slots

Reinstall both batteries upon successful completion of individual tests.

9.3.0 LEAKAGE TESTING

Note: All leakage tests are usually done with a meter specifically designed for making this measurement on medical equipment. For safety reasons, do not attempt these measurements unless this type of instrument is available.

9.3.1 CHASSIS LEAKAGE

To test the chassis to ground leakage, use a safety leakage tester. There should be less than 100uA read on the meter between chassis and earth ground, with the ground of the monitor open. Reverse the polarity on the AC input and check again.

9.3.2 PATIENT INPUT LEAKAGE

Using the patient lead cable, short all of the leads together. With a meter between the leads and earth ground, less than 20uA should be read. If you do not use a cable, short lead inputs at connector. Meter should read less than 10uA when at the connector.

As described above, with the leads shorted, put a meter between leads and 120V AC. The leakage current should be less than 20uA when using leads, or 10uA when at the connector.

9.4.0 GROUND CHECK

Test for ground continuity between AC plug ground and chassis ground at unpainted metal screw head on the rear panel. Power cord ground should be less than .15 ohms.

9.5.0 RAM, ROM SELF TEST

Using soft keys, call up the TEST page. Do a RAM self test by pressing soft key TEST RAM. The screen will say RAM TEST IN PROGRESS. Some screen glitches may be observed at this time. When test is completed screen will note PASSED RAM TEST or RAM BAD CALL SERVICE. Repeat the above procedure for ROM testing.

9.6.0 KEYPAD

Test hard key function by pressing all the hard keys, verifying that the key initiates function. Verify audio key click. softkeys require testing only one function.

FUNCTIONAL TESTS

Note: When using patient simulator, the tolerance factor of the simulator must be factored in determining if the monitor is within tolerance.

9.7.0 ECG

Using a calibrated patient simulator, confirm heart rate count at low, mid and high ranges, such as 20 BPM, 100 BPM, and 250 BPM. Input signal should be 1mV R-wave. Heart rate should be $\pm 2\%$, not including simulator accuracy. Check asystole, 00 count.

Verify a normal heart rate count at a low amplitude such as .2mV and a high amplitude such as 3mV. Adjust soft key sizing as necessary.

Verify alarms by turning alarm function on using soft keys. Factory default setting is 140 BPM high and 50 BPM low for adult mode, 200 BPM high and 100 BPM low for neonatal mode. Using patient simulator violate alarm limits, both high and low, returning to NSR in between to reset alarm.

Check pacer flag operation by inserting a pacer spike at 4mV to 200mV typical amplitude, for 200uS to 2mS typical in width. Be sure to have the soft key PACE in the ON mode. Cardiotach should not be affected by pacer spike.


9.8.0 PRESSURE

Zero simulator using manufacturers directions. Confirm pressure readings at a low, mid and high ranges such as 10mmHg, 100mmHg and 250mmHg. Pressure reading accuracy should be $\pm 1\%$ or 1mm (whichever is greater) not including simulator tolerance.

If ESCORT is configured for 2 Blood Pressures, repeat the above procedure on BP2.

9.9.0 TEMPERATURE

For temperature testing a small resistor circuit with a high degree of accuracy is necessary. For best results, use 1 % resistors along with a potentiometer to adjust the resistance to the exact value required for testing.

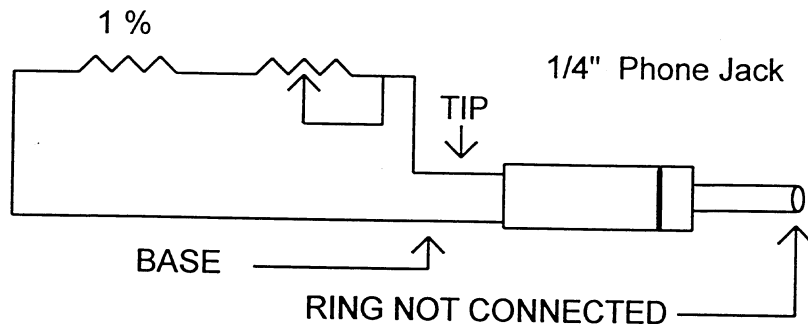

A 1/4" stereo phone jack is used to input the resistance that is simulating the temperature. Wire this jack and circuit as in the diagram above with the resistor circuit placed between the tip and the base of the jack. The ring is not connected.

Start with the 1 degree testing circuit. A resistor circuit equaling $18,597 \text{ ohms} \pm 40 \text{ ohms}$ should be assembled and placed between the tip and the base of the temperature jack. The monitor should read $1 \text{ degree C} \pm .2 \text{ degrees C}$. Using a circuit equaling $5,998 \text{ ohms} \pm 13 \text{ ohms}$, the temperature should read $25 \text{ degrees C} \pm .2 \text{ degrees C}$, and for a reading of $40 \text{ degrees C} \pm .2 \text{ degrees C}$, use a $3,203 \text{ ohm} \pm 6 \text{ ohm}$ reference. Testing low, mid and high ranges is recommended.

9.10.0 RESPIRATION

Using a patient simulator with an output of 1 ohm impedance change, check respiration at a low, mid and high level, such as 10 BPM, 40 BPM and 80 BPM. Accuracy should be $\pm 2\%$ or 2 BPM not including simulator tolerance. Verify a normal respiration count at a low impedance change such as .25 ohm and a high impedance change such as 3 ohms. Adjust soft key sizing as necessary. Verify 00 count by simulator apnea function. Also check apnea alarm function.

9.11.0 RECORDER

Verify recorder operation by using hard keys RECORD 1 and RECORD 2. Terminate recording with the RECORD STOP key.

9.12.0 NIBP

Connect manometer to bottom lumen. Go to test page and put the monitor in *TEST CHK* mode. Return to NIBP page, and pump up manometer to 100mmHg $\pm 2\%$. Next, vent or disconnect manometer. Monitor should read 0mmHg. Go to test page and toggle test key to *TEST LEAK*. Connect cuff and hose assembly and wrap cuff on itself. Return to NIBP page and push start. Do not touch cuff while test is in progress.

9.13.0 SAO₂

Check patient cable input pins. Verify they are straight and not bent. Connect patient module cable to monitor. Verify sensor LED is lit. Put sensor on valid sensor sight. Look for normal waveform and reading. Remove any ECG input from the monitor. Assure a NO C-LOCK message appears. If you have a Nellcor Simulator or Pocket Tester you can check SAO₂ accuracy. Use simulator according to manufacturers instructions. Tolerance should be: Adult 70 - 100% ± 2 digits, Adult 50 - 69% ± 3 digits. Neonatal 70 - 94% ± 3 digits. If using the Nellcor Pocket Tester it is important not to have any ECG signal input to the monitor. Readout should be 81% SAO₂.

9.14.0 PERFORMANCE CHECK LIST

NEO	_____	ADULT	_____	MODEL	_____
PORT 1	_____	PORT 2	_____	SERIAL NUMBER	_____
DEG C	_____	DEG F	_____	DATE	_____
				TECHNICIAN	_____

BATTERY OPERATION

Batteries charged	OK	_____
Battery #1 operation	OK	_____
Battery #2 operation	OK	_____

LEAKAGE

Chassis leakage	100uA or less	_____
Patient input leakage at ground	20uA or less	_____
without cable	10uA or less	_____
at 120V AC	20uA or less	_____
without cable	10uA or less	_____
Ground check	.15 ohms or less	_____
RAM Self Test	RAM OK	_____
ROM Self Test	ROM OK	_____
Keypad	OK	_____
audio click	OK	_____

ECG TESTS

Heart rate at 1mV low	OK	_____
mid	OK	_____
high	OK	_____
asytole	OK	_____
Normal heart rate at low amplitude	OK	_____
Normal heart rate at high amplitude	OK	_____
Alarm violation high	OK	_____
Alarm violation low	OK	_____
Pacer rejection operation	OK	_____

BLOOD PRESSURE

BP1 reading low	OK	_____
mid	OK	_____
high	OK	_____
BP2 reading low	OK	_____
mid	OK	_____
high	OK	_____

TEMPERATURE

T1 - 1 degree reading	OK	_____
25 degrees reading	OK	_____
40 degrees reading	OK	_____
T2 - 1 degree reading	OK	_____
25 degree reading	OK	_____
40 degrees reading	OK	_____

RESPIRATION

Resp rate at 1 ohm: low	OK	_____
mid	OK	_____
high	OK	_____
Normal resp rate at low impedance change	OK	_____
Normal resp rate at high impedance change	OK	_____
Apnea alarm violation	OK	_____

RECORDER OPERATION	OK	_____
--------------------------	----	-------

NIBP

Static 100mmHg input reads within $\pm 2\%$	OK	_____
Static 0mmHg input reads 0	OK	_____
Leak test	OK	_____

SAO₂

Patient module cable operation check	OK	_____
NO C-LOCK check	OK	_____

MECHANICAL DISASSEMBLY

CHAPTER 10

10.0.0 MECHANICAL DISASSEMBLY

CAUTION!!!

Only qualified technicians should attempt to perform repairs or removal of any parts in the **ESCORT 300A**. Opening the **ESCORT 300A** could violate warranty.

READ ALL DISASSEMBLY INSTRUCTIONS PRIOR TO PERFORMING ANY REMOVAL OF PARTS!!!

REFER TO THE CONNECTOR PLACEMENT DRAWING WHEN REPLACING CONNECTORS.

10.1.0 SAFETY

High voltage is exposed when the covers are removed from the monitor. Disconnect the AC power cord **AND** remove the batteries to insure that current is removed from the unit. Always observe safe working techniques when troubleshooting or removing components. Work surface's should be free of any stray metal parts.

THE COMPONENTS IN THE ESCORT MONITOR ARE STATIC SENSITIVE. USE AN ELECTRO-STATIC DISCHARGE KIT WHENEVER HANDLING PRINTED CIRCUIT BOARDS.

10.2.0 FUSE REPLACEMENT

There are two .5 AMP Slow Blow fuses located in the power module at the rear panel. The module can be removed by prying the tab at the low-center area of the module with a flat-bladed screwdriver. Pull out the fuse holder and replace any damaged fuses. To replace the module, push it back into place until a click is heard and the module is secure. For 220V, use .25 amp slow blow.

10.3.0 DISASSEMBLY

This chapter includes removal instructions only; the reinstallation of assemblies is the opposite of removal.

10.3.1 TOP COVER

Remove the three screws on each side of the monitor. Lift the top cover straight up.

10.3.2 BOTTOM COVER

Remove the three screws on each side of the monitor. Lift the chassis out of the bottom cover.

CAUTION: When re-assembling the unit, make sure all top and bottom screws are replaced. Failure to do so could cause the unit to come apart in transport!

10.3.3 RECORDER REMOVAL

- * Remove Top and Bottom covers.

Disconnect the gray ribbon cable at the rear of the recorder. Open the paper door and remove the roll of paper. Inside the paper housing, at the rear of the recorder, there are two screws that must be detached from the recorder mounting bracket. Use a flat bladed screwdriver to do this. After loosening these two screws, lift the recorder out of the chassis. The screws are part of the recorder assembly and will not fall out.

10.3.4 PROCESSOR UNIT (This consists of all Main Parameter PCBA's and their Daughter Boards.)

- * Remove Top and Bottom covers.

Back off the long screw at the center of the processor unit until it is disengaged from the nut. Lift ECG and Temp/Pressure Boards (along with the connector plate) up and out of the sockets as a unit.

A. Temperature/Pressure Board removal:

Remove the four allen screws using a 5/64 allen wrench. Pull away from the connector plate slightly. Remove J5 (T1), J4 (T2), J3 (BP1), and J2 (BP2). Pull the PCBA away from the connector plate.

B. ECG Board removal:

Pull gray cap off the lead select knob (applies only to units with 5 lead select). Using "special tool", loosen screw and pull off the knob. Remove the two allen screws on the connector plate using a 5/64 allen wrench. Disconnect the "sync out" and pull the ECG Board away from the connector plate.

CAUTION!!!

Take great care in replacing the processor unit. Be sure that both boards are securely in the connector slots.

10.3.5 SWITCHING POWER SUPPLY/BATTERY CHARGER PCBA

- * Remove Top and Bottom covers.

Unplug J1 and J2 on the Switching Power Supply Board. Unscrew the two Phillips-head screws located nearest the center of the chassis side bar. Remove the insulator (FISH) paper. Gently lift out the PCBA about half-way, then remove J3 and J4. Then, lift the PCBA completely out of the chassis.

10.3.6 CPU REMOVAL

- * Remove Top and Bottom covers, Processor Unit and Switching Power Supply Board.

Remove J4, J6, and J8 on the CPU. Remove the seven Phillips-head screws securing the CPU Board to the chassis then gently lift the CPU out.

10.3.7 LCD REMOVAL

- * Remove Top and Bottom covers, Switching Power Supply Board, and Processor Unit.

Remove J9 and J6 on the CPU Board, noting which direction they must be replaced. Remove J4 from the Power Supply Board. Remove the four corner nuts (securing the LCD to the chassis) using a 5/16" nut driver. Remove the ground strap.

Remove the Backlight Driver PCBA by removing the screws that hold it in place and lift it off the securing bar. The Backlight Driver PCBA is part of the LCD and should be removed with it. The wires connecting the Backlight Driver board to the display are secured to the LCD brass backplate with two tie-wraps. These tie-wraps must be cut and removed in order to take the LCD out of the chassis.



NOTE: When replacing the PCBAs remember to reinstall the fish paper for each board.

10.3.8 EL DISPLAY REMOVAL

- * Remove Top and Bottom covers, Switching Power Supply Board, and Processor Unit.

Remove J9 and J6 on the CPU Board, noting which direction they must be replaced. Remove J2 from the Power Supply Board. Remove J1 from the EL Display Driver Board. Remove the four corner nuts (securing the EL Display to the chassis) using a 5/16" nut driver.

NOTE: When replacing the PCBAs remember to reinstall the fish paper for each board.

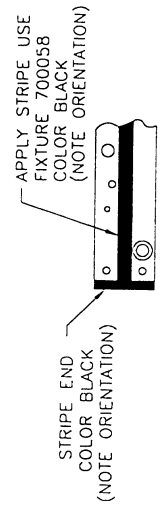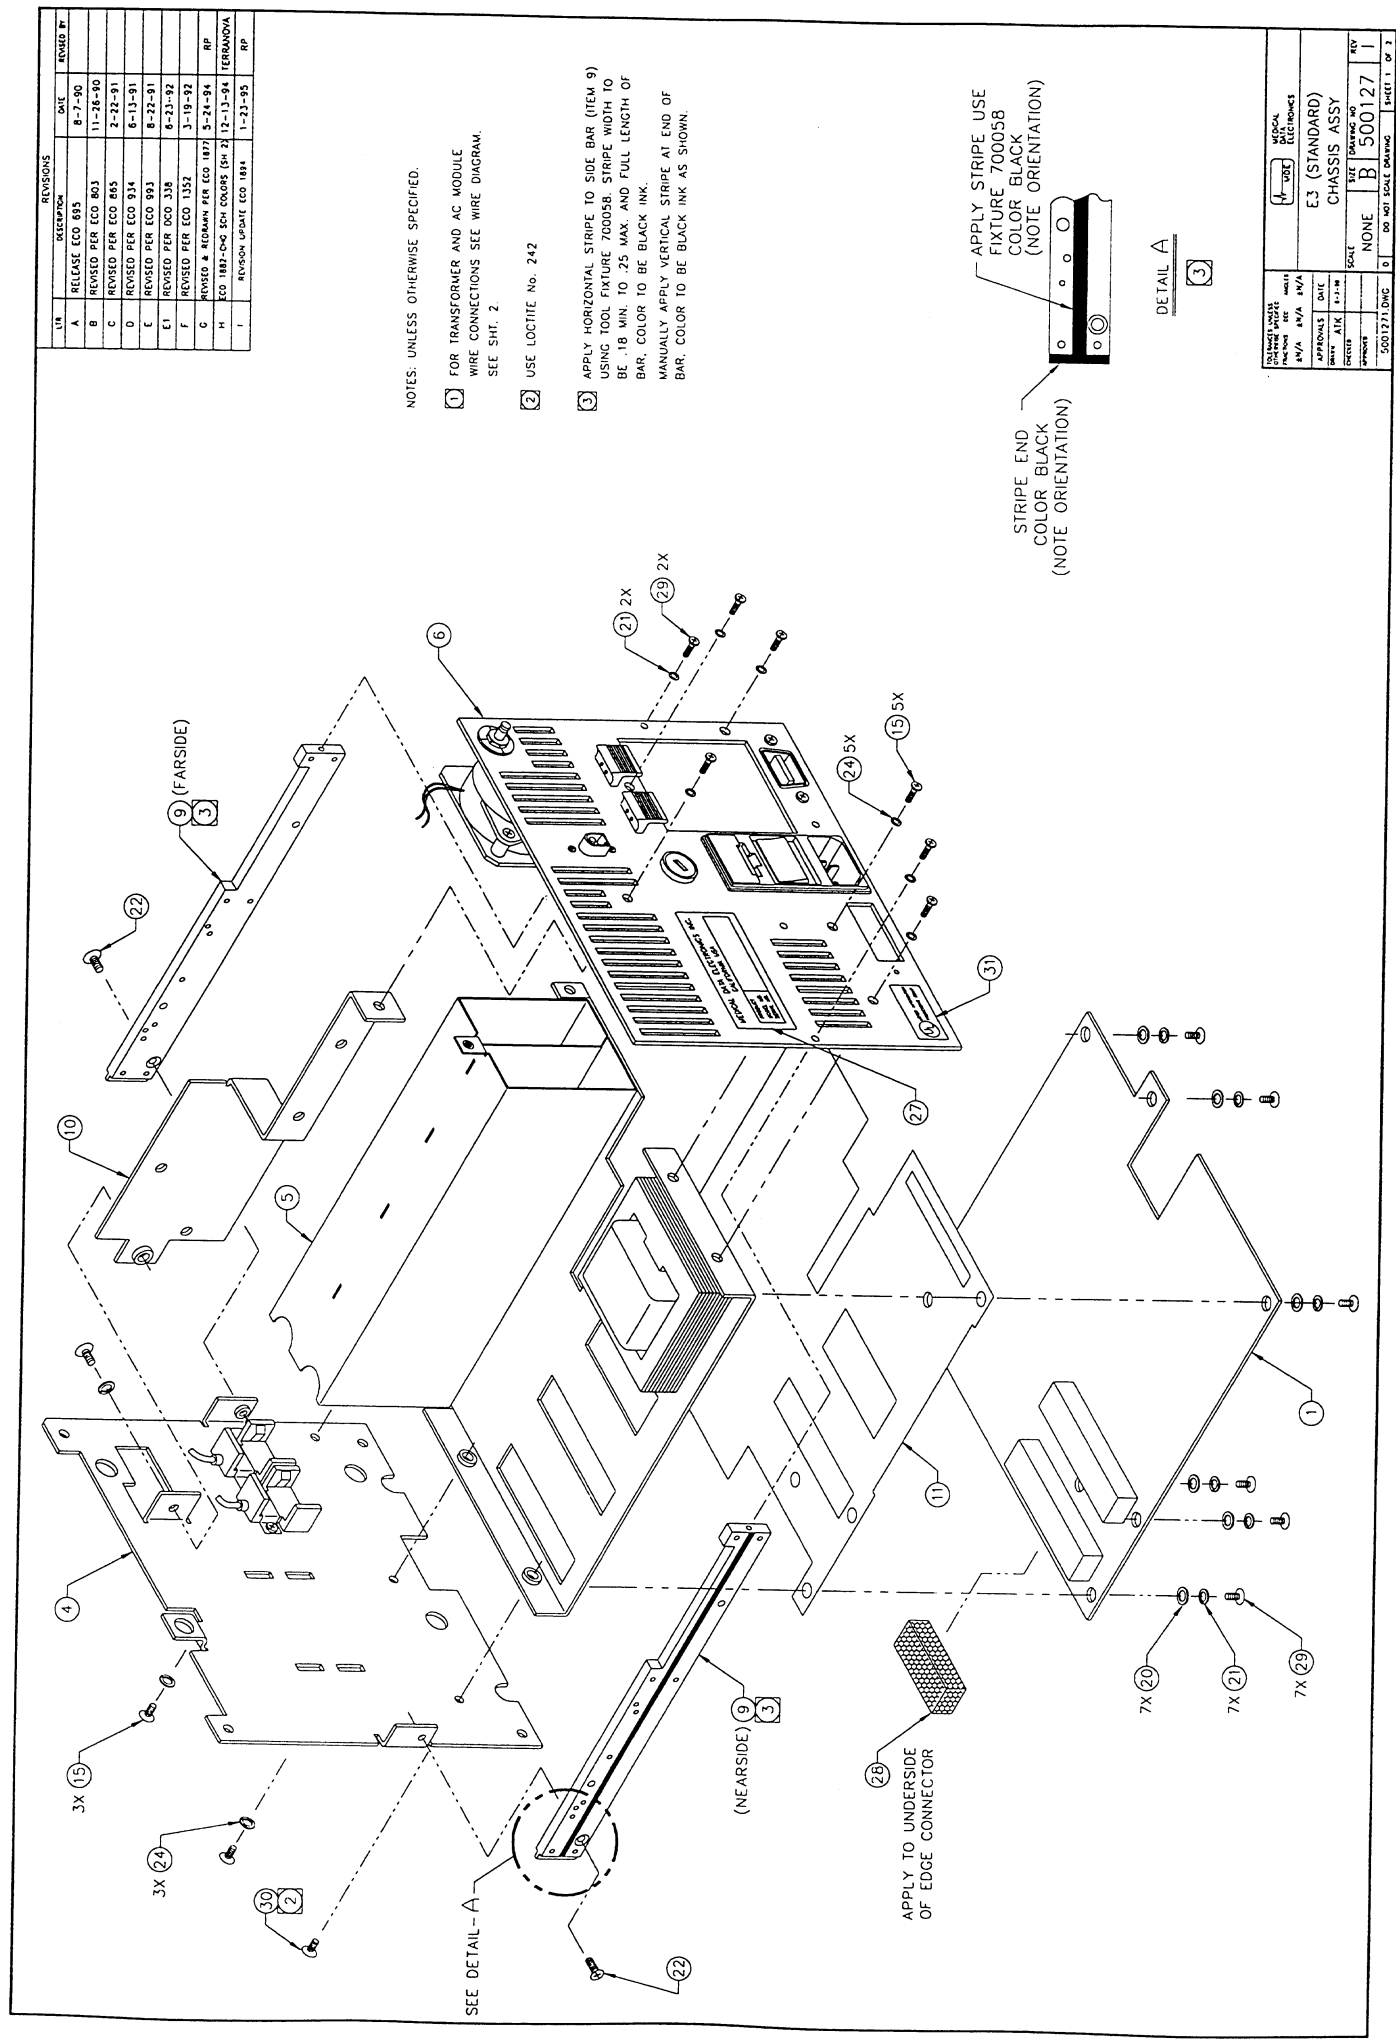

DETAIL A

- NOTES: UNLESS OTHERWISE SPECIFIED.
- FOR TRANSFORMER AND AC MODULE
WIRE CONNECTIONS SEE WIRE DIAGRAM.
SEE SHT. 2.
 - USE LOCITE No. 242
 - APPLY HORIZONTAL STRIPE TO SIDE BAR (ITEM 9)
USING TOOL FIXTURE 700058. STRIPE WIDTH TO
BE .18 MIN. TO .25 MAX. AND FULL LENGTH OF
BAR. COLOR TO BE BLACK INK.
MANUALLY APPLY VERTICAL STRIPE AT END OF
BAR. COLOR TO BE BLACK INK AS SHOWN.

REVISIONS		DATE	REVISED BY
A	RELEASE ECO 885	8-7-90	
B	REVISED PER ECO 803	11-26-90	
C	REVISED PER ECO 865	2-22-91	
D	REVISED PER ECO 934	6-13-91	
E	REVISED PER ECO 993	8-22-91	
F	REVISED PER ECO 1352	8-23-92	
G	REVISED PER ECO 1352	3-19-92	
H	REVISED PER ECO 1872	5-24-94	RP
I	ECO 1882-COG BGA COUPLER (SH 2)	12-13-94	TERAMONDA
J	REVISION UPDATE ECO 1884	1-23-95	RP

DESIGNER: JAVIERE		CHECKED: JAVIERE		DATE: 8/7/90	
DRAWN: JAVIERE		CHECKED: JAVIERE		DATE: 8/7/90	
APPROVED: JAVIERE		CHECKED: JAVIERE		DATE: 8/7/90	
SCALE: NONE		SIZE: B		DRAWING NO: 500127	
SHEET: 1 OF 2		DO NOT SCALE DRAWING		SHEET: 1 OF 2	

Figure 10-1

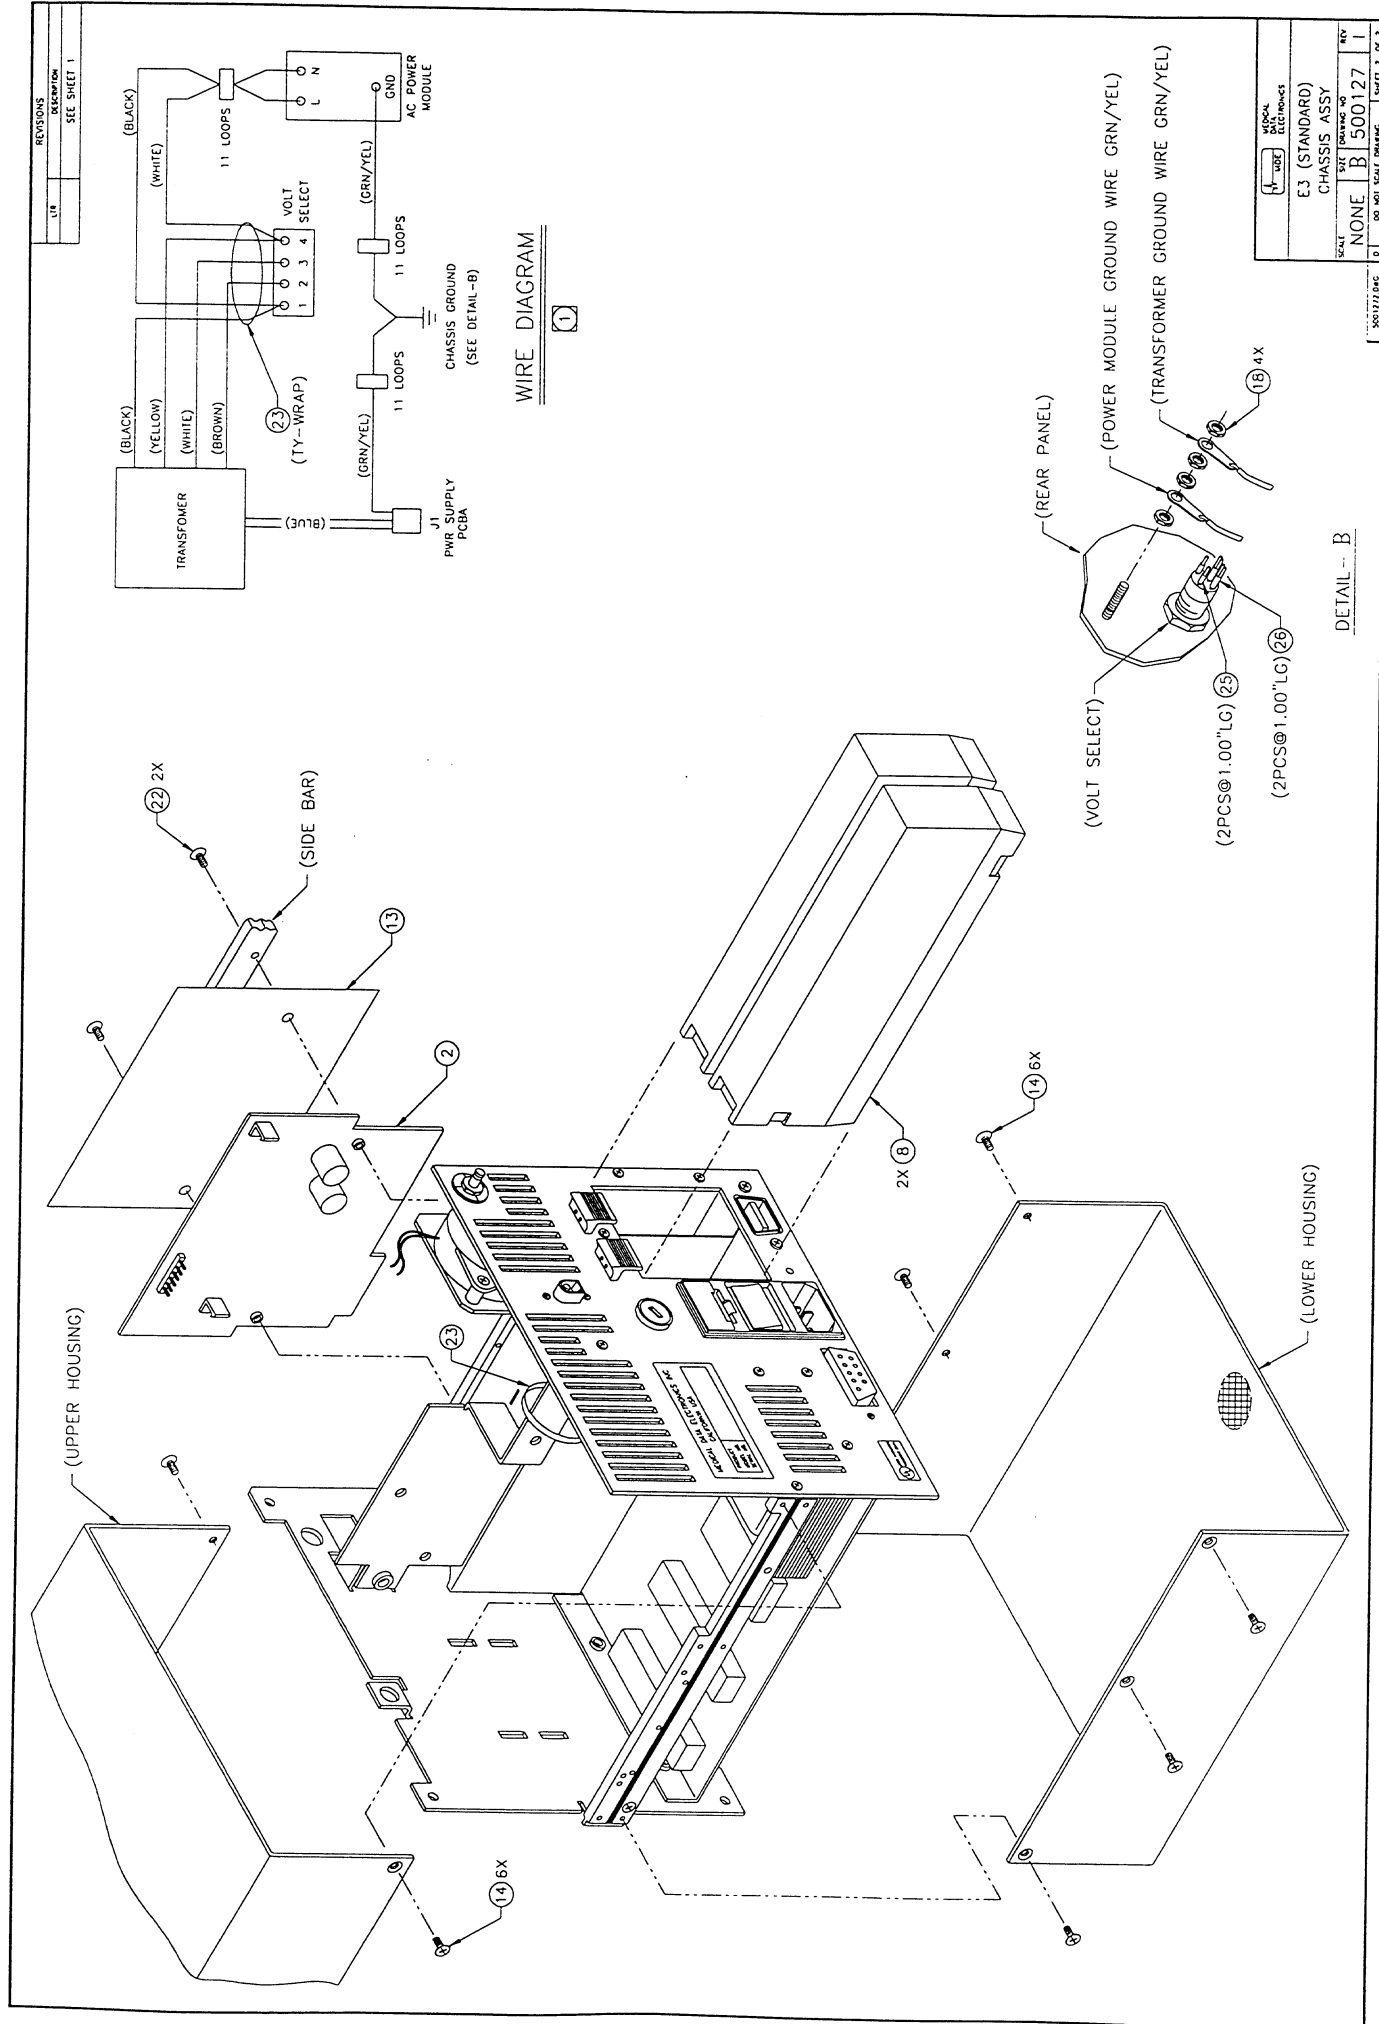


Figure 10-1 (continued)


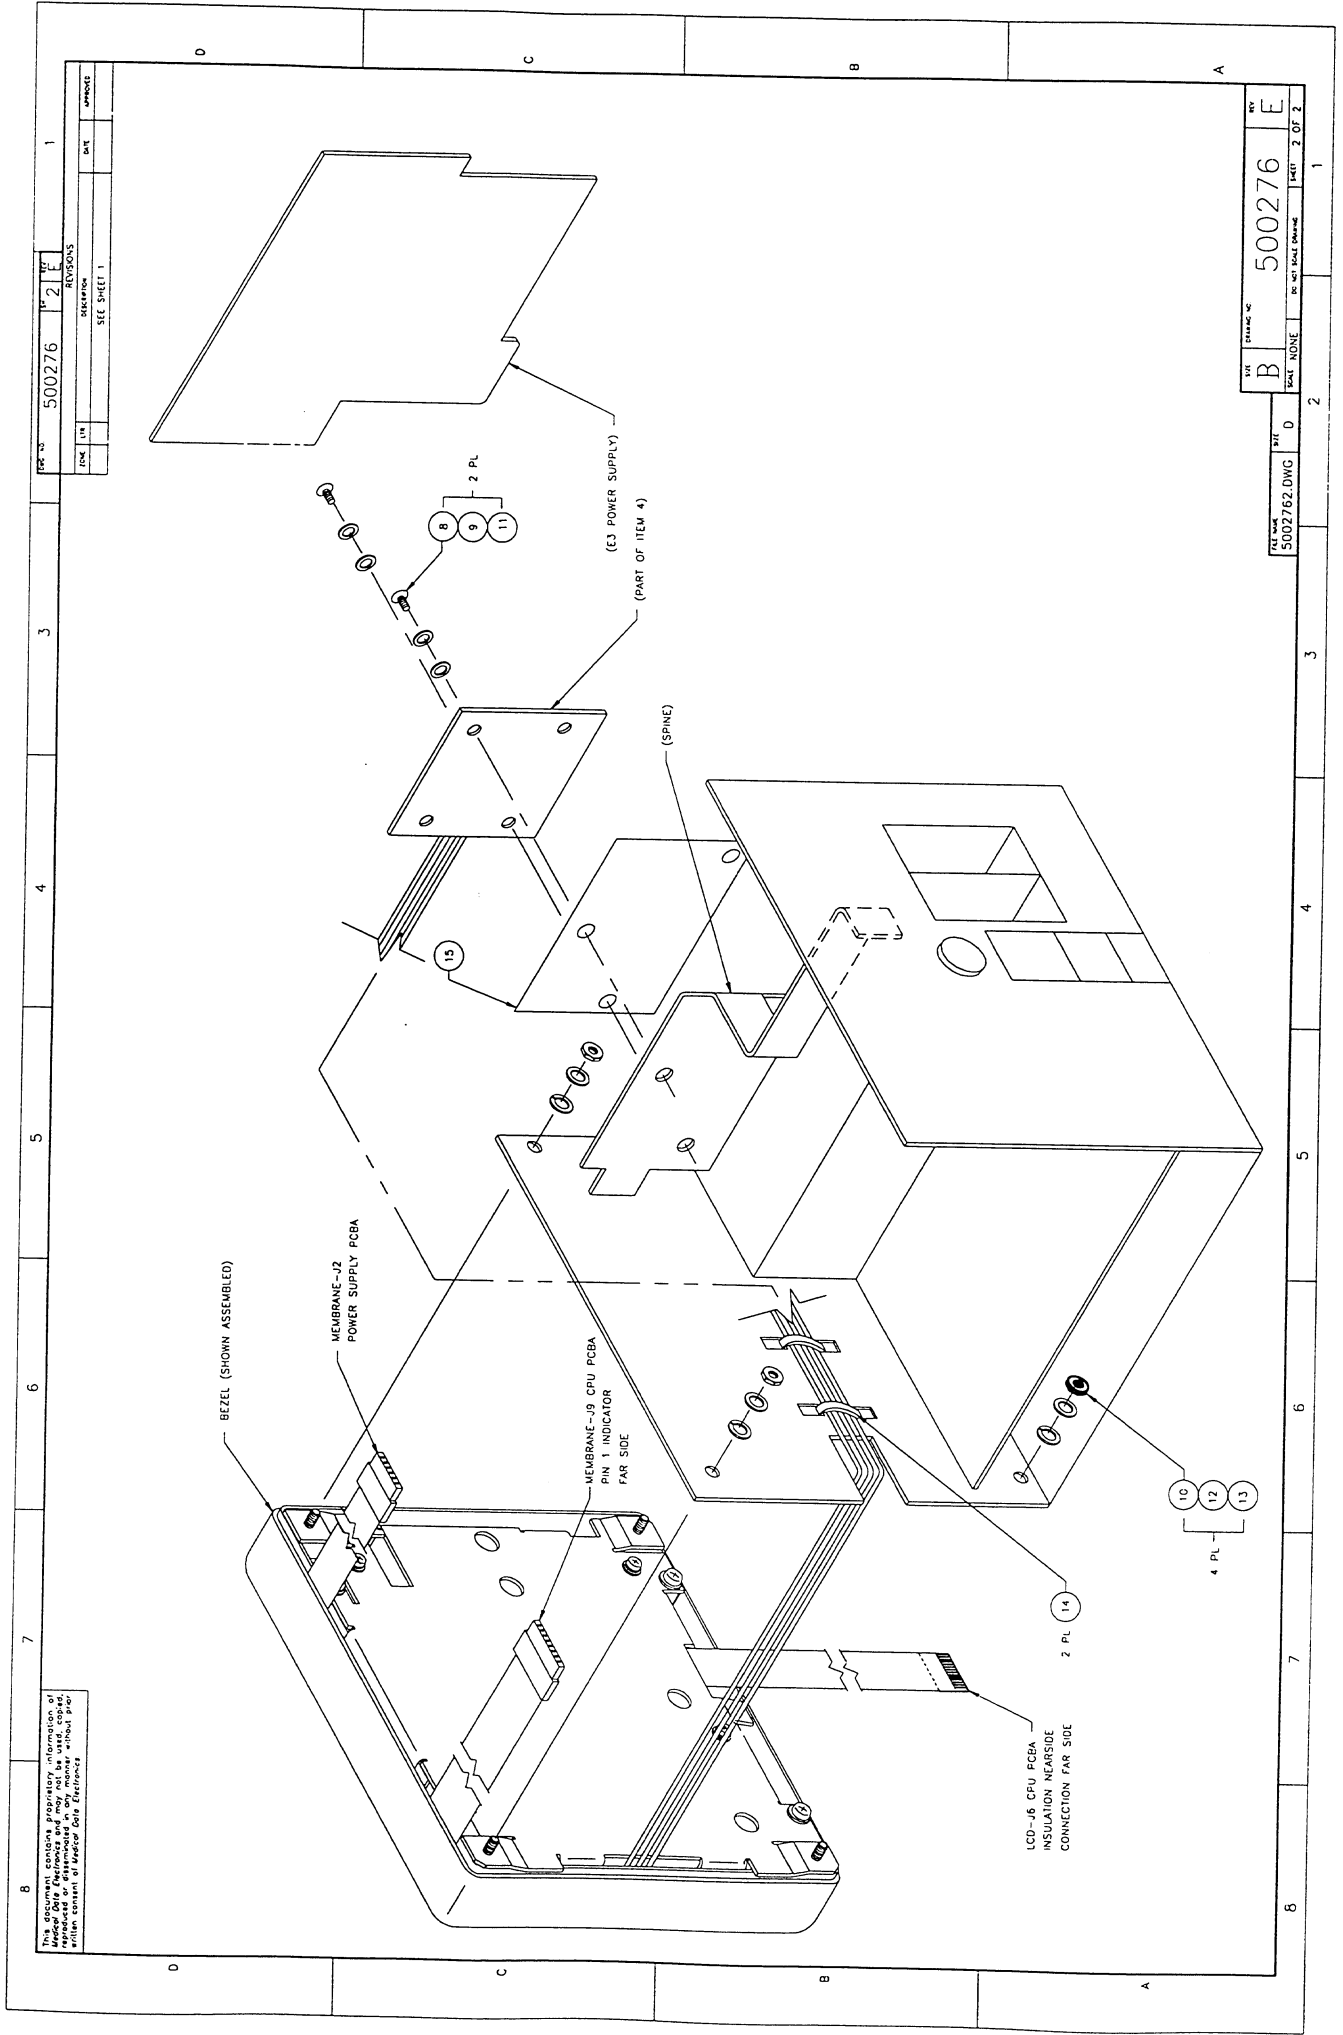


Figure 10-2 (continued)

REVISIONS			DATE	REMOVED BY
LT#	DESCRIPTION	DATE	REMOVED BY	
A	RELEASED PER ECO 1332	1-18-93	AJM	
B	ECO 1401	5-10-93	AJM	
C	ECO 1405	5-19-93	AJM	
D	REVISED PER ECO 1459	9-7-93	R.P.	
E	ECO 1671-CHG CBL (REF 22)	04-04-94	TERRANOVA	
F	ECO 1685-ADDED REF 23	05-11-94	TERRANOVA	
G	ECO 1746-BOM CHG (REF R21)	08-15-94	TERRANOVA	
H	REVISED BEZEL LABEL ECO 1894	1-23-95	RP	
I	REV UPDATE PER ECO 1904	2-2-95	RP	

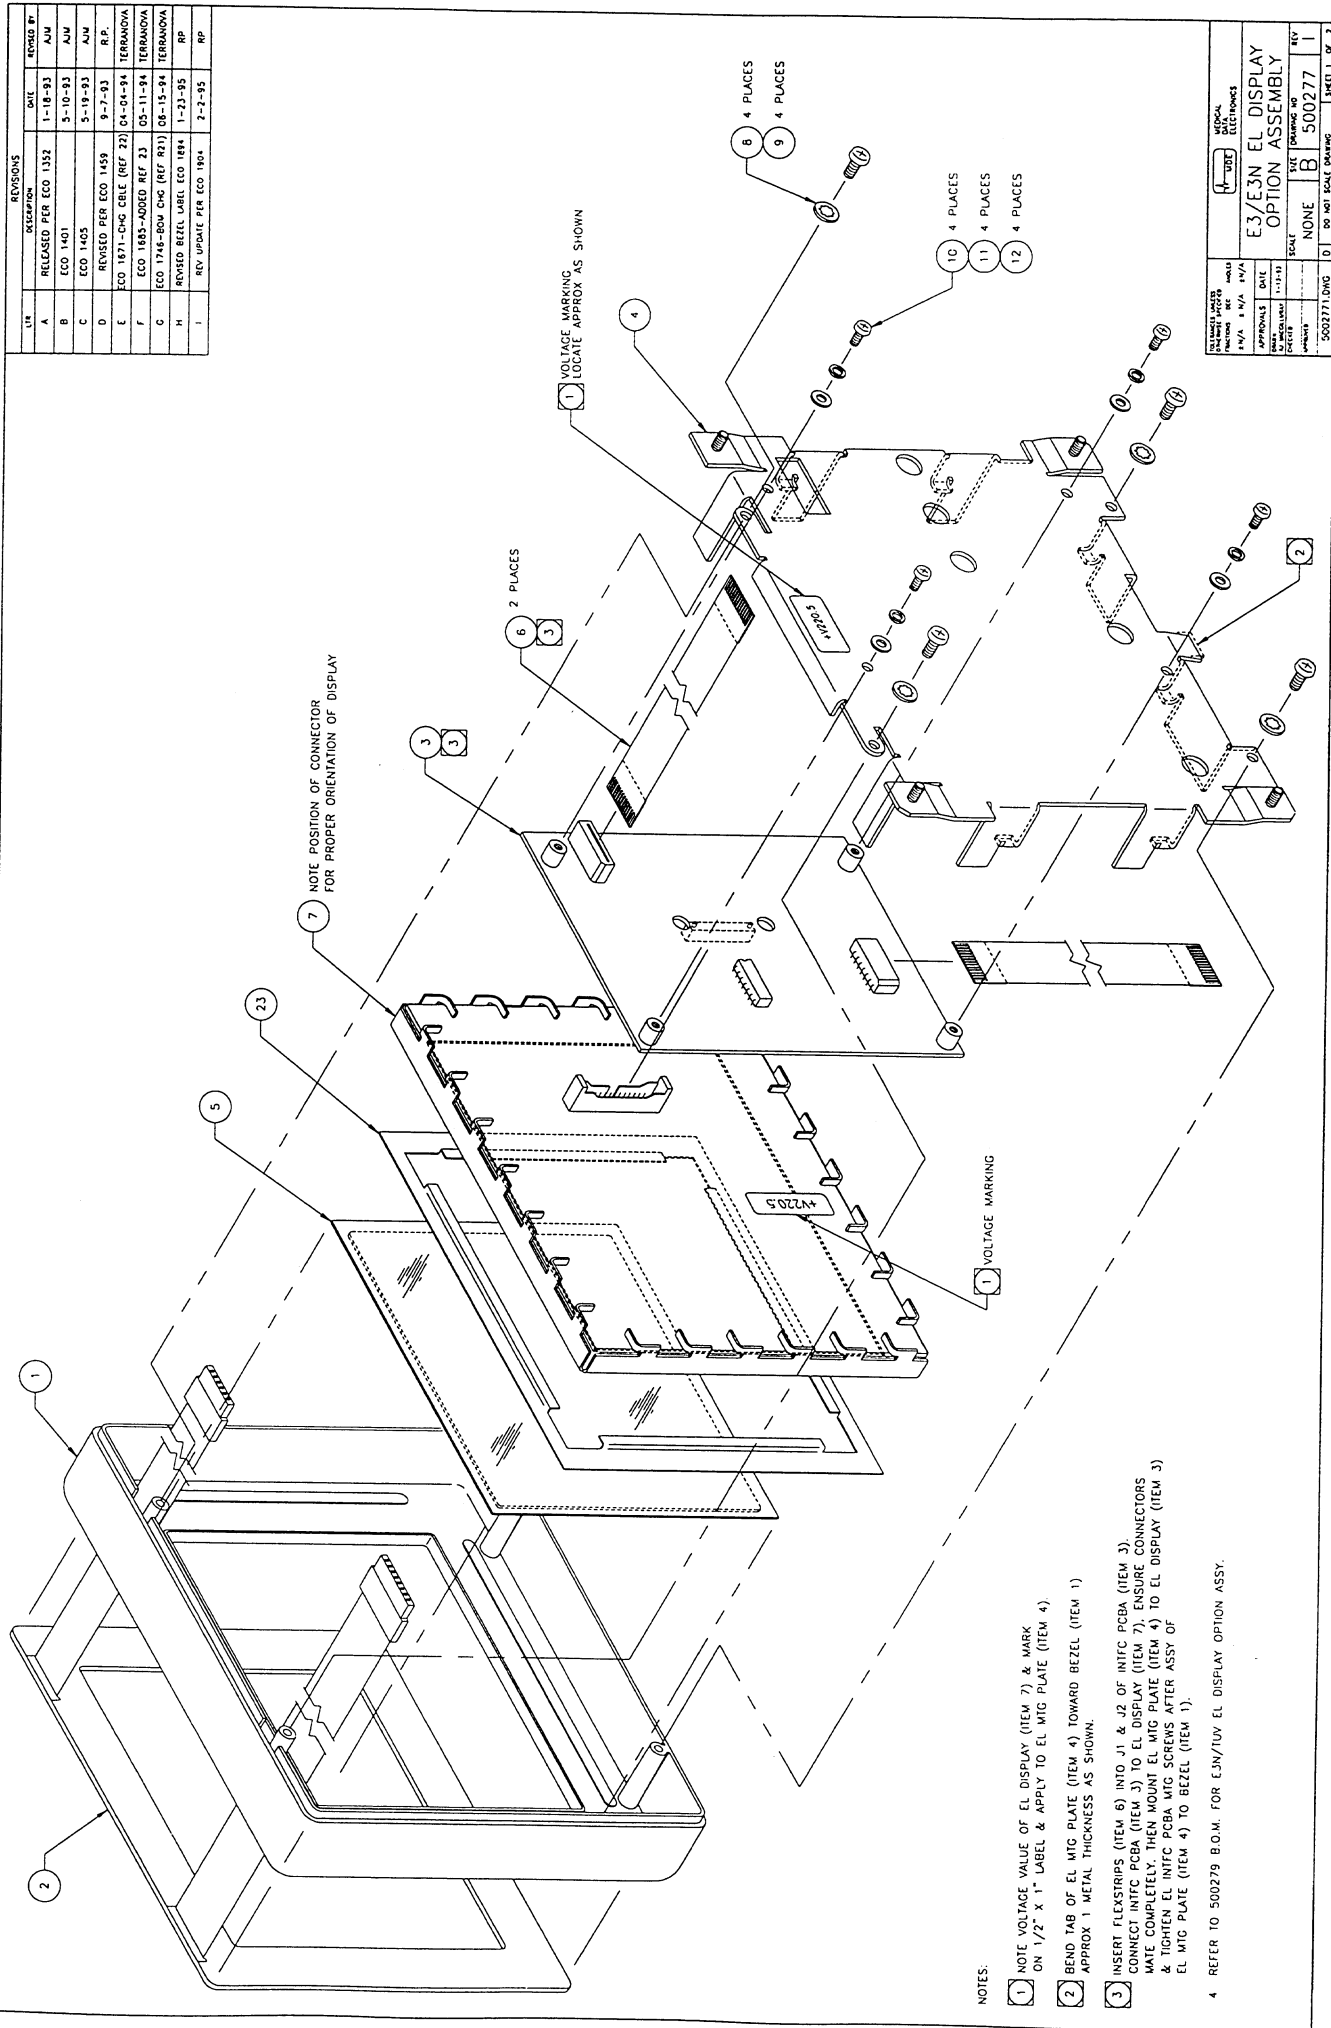

NOTES:

- 1 NOTE VOLTAGE VALUE OF EL DISPLAY (ITEM 7) & MARK ON 1/2" x 1" LABEL & APPLY TO EL MTG PLATE (ITEM 4).
- 2 BEND TAB OF EL MTG PLATE (ITEM 4) TOWARD BEZEL (ITEM 1). APPROX 1 METAL THICKNESS AS SHOWN.
- 3 INSERT FLEXSTRIPS (ITEM 6) INTO J1 & J2 OF INITFC PCB (ITEM 3). CONNECT INITFC PCB (ITEM 3) TO EL DISPLAY (ITEM 7). ENSURE CONNECTORS MATE COMPLETELY. THEN MOUNT EL MTG PLATE (ITEM 4) TO EL DISPLAY (ITEM 3) & TIGHTEN EL INITFC PCB SCREWS AFTER ASSY OF EL MTG PLATE (ITEM 4) TO BEZEL (ITEM 1).
- 4 REFER TO 500279 B.O.M. FOR E3N/TUV EL DISPLAY OPTION ASSY.

APPROVALS		DATE	SCALE	SIZE	REV
DESIGNED BY	DATE	1-13-93	NONE	B	500277
DRAWN BY	DATE				
CHECKED BY	DATE				
APPROVED BY	DATE				
TERRANOVA ELECTRONICS					
E3/E3N EL DISPLAY OPTION ASSEMBLY					
SHEET 1 OF 2					

Figure 10-3


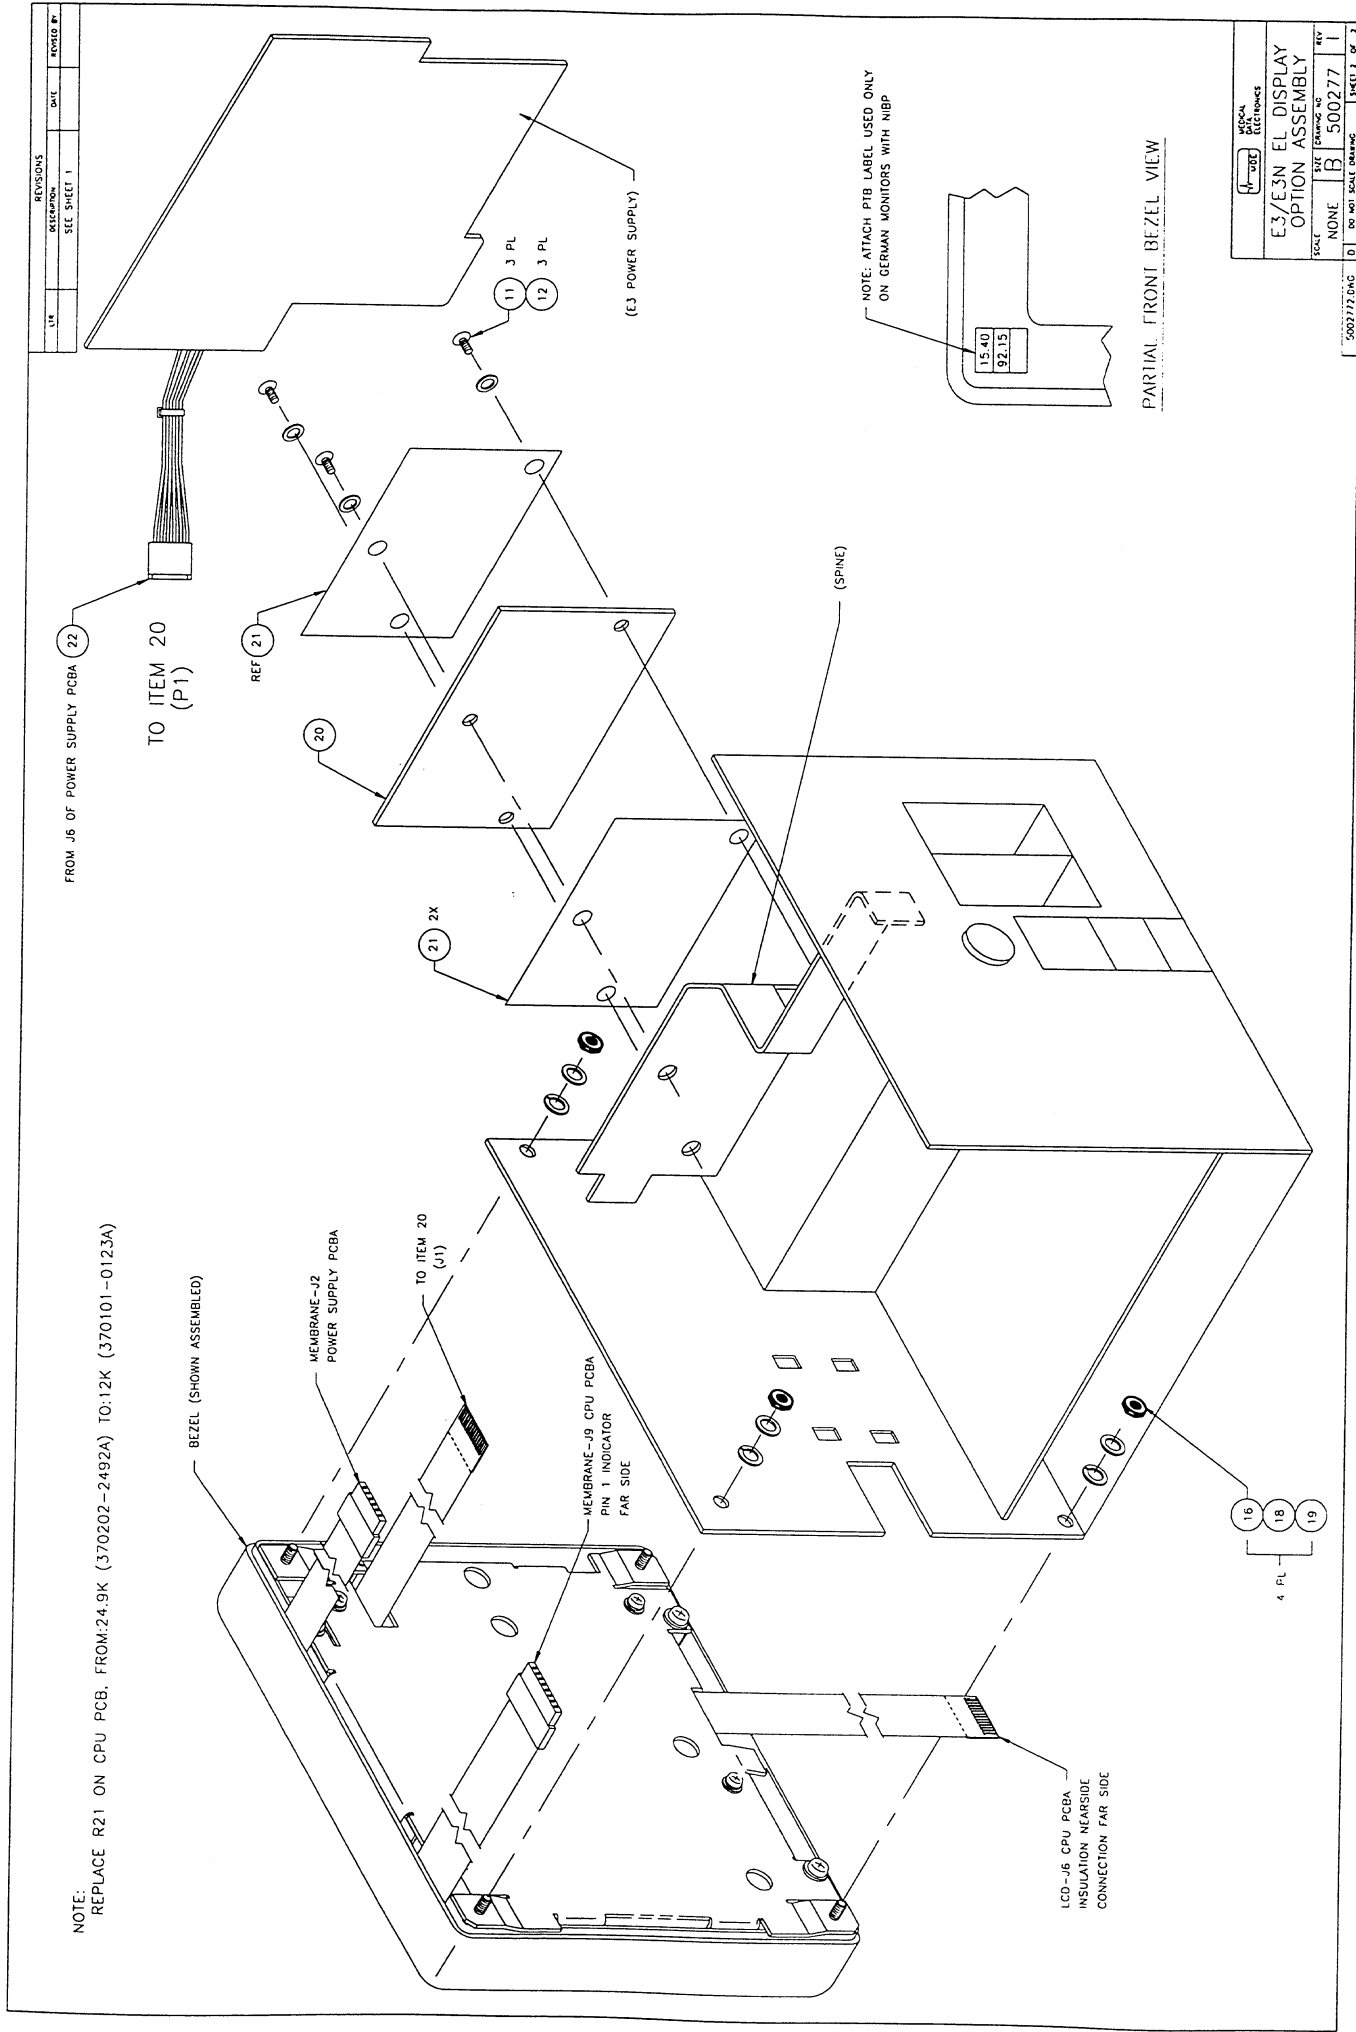


Figure 10-3 (continued)

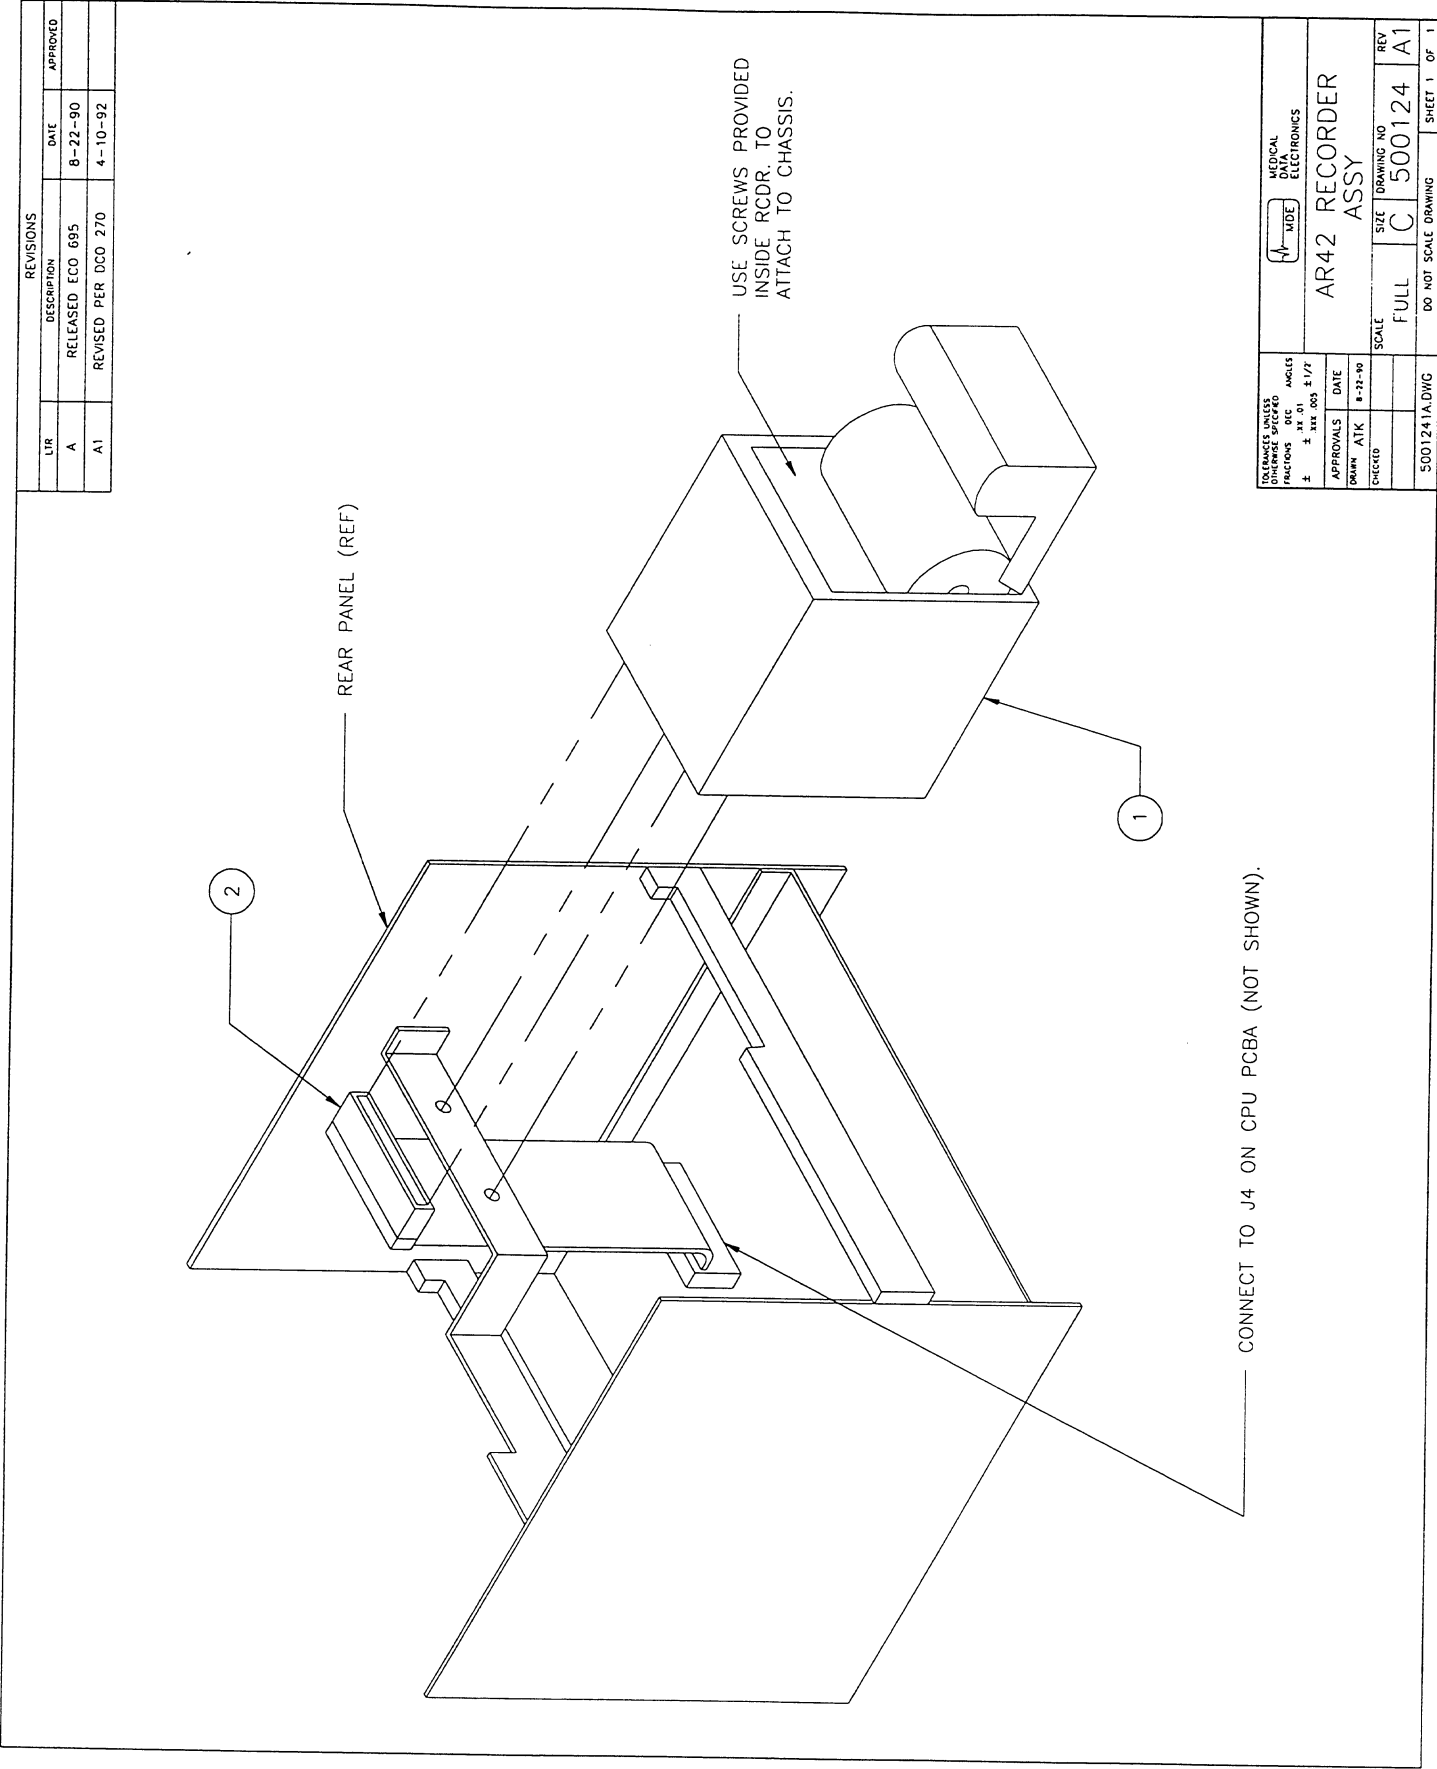

REVISIONS			
LTR	DESCRIPTION	DATE	APPROVED
A	RELEASED ECO 695	8-22-90	
A1	REVISED PER DCO 270	4-10-92	

TOLERANCES UNLESS OTHERWISE SPECIFIED		MEDICAL DATA ELECTRONICS	
INCHES	FRACTIONS	MM	DECIMALS
±	1/16 1/8 1/4 1/2	±	0.05 0.1 0.2 0.5
APPROVALS		DATE	
DESIGN	ATK	8-22-90	
CHECKED			
5001241A.DWG			
AR42 RECORDER ASSY		REV	
SCALE		DRAWING NO	
FULL		500124	
SIZE		A1	
DO NOT SCALE DRAWING		SHEET 1 OF 1	

Figure 10-4

358100-0004A	SCR, 4-40 X 3/8, PH FLTHD, SS, 100 DEG.	4	22
358100-0036A	SCR, 4-40 X 1/4, PH PNHD, ZINC OR ANY	9	29
358100-0041A	SCR, 6-32 X 1/4 PHL PNHD	8	15
358100-0102A	SCR, 6-32 x 1/8 IN LG PHPNHD, STL ANY PLT	1	30
358200-0004A	WSHR, #4 FLAT STL ZINC, (.125ID, 9/32OD, .025THK)	7	20
358200-0009A	WSHR, #4 SPLIT LOCK	11	21
358200-0018A	WSHR, #6 INT TOOTH STEEL	8	24
360500-0023A	NUT, #6 HEX, LRG PTRN	4	18
385000-0000A	TY-WRAPS, 3IN LENGTH (1000/BAG)	1	23
385000-0004A	SHRINK TUBING, 1/8in BLACK VW-1	2	25
385000-0005A	SHRINK TUBING, 1/4in BLACK VW-1	2	26
400404-0000	LABEL, ~UL LISTED MEDICAL EQUIP.~ 26T1 -E3/E4	1	31
400746-0000	DGHTR BD. 1/8 FOAM INSULATION, REV B (E1521)	1	28
401073-0000	SIDE BAR E3 MONITOR REV. D (E1677)	2	9
401093-0000	FISHPAPER E3 CPU REV. B (E827)	1	11
401168-0000	PCBA, E3 CPU MOTHER REV. S (E2003)	1	1
401170-0000	PCBA, E3 POWER SUPPLY REV. T (E1879)	1	2
401234-0000	FISH PAPER PWR SPLY PCBA E3 REV. B	1	13
401237-0000	FRONT PLATE ASSY E3 REV. D1 (D584)	1	4
401238-0000	SUB-CHASSIS ASSY E3 REV. C (E1732)	1	5
401244-0000	REAR PNL ASSY E3 REV. F (E1360)	1	6
401247-0000	E3/E2B/E2B BATTERY PACK W/ LABEL ASSY REV. A	2	8
401347-0000	LBL, SERIAL NUMBER E3/E4/LINK/DEFIB	1	27
402016-0000	SPINE - E3 REV. A (E1352)	1	10
402584-0000	FAB PAINT SCREW #4-40 x 3/16 REV. A (E1932)	12	14

358100-0036A	SCR, 4-40 X 1/4, PH PNHD, ZINC OR ANY	3	8
358100-0140A	SCR, PLASTITE, 6 x 1/4~LG, PNH PHL STL ZN PLATE	4	5
358200-0004A	WSHR, #4 FLAT STL ZINC, (.125ID, 9/32OD, .025THK)	3	9
358200-0006A	WSHR, #6 FLT STL ZINC	4	10
358200-0009A	WSHR, #4 SPLIT LOCK	3	11
358200-0010A	WSHR, #6 SPLT LCK	4	12
360500-0023A	NUT, #6 HEX, LRG PTRN	4	13
362000-0015A	LCD, 6 IN 320x200 DBL SUPERTWST FOR E3 **FIFO**	1	4
385000-0000A	TY-WRAPS, 3IN LENGTH (1000/BAG)	2	14
401071-0000	LCD PLATE E3 MONITOR REV. D (E1071)	1	2
401081-0000	MEMBRANE E3 MONITOR REV. F (E1982)	1	3
401315-0000	ROM, SINGLE CHANNEL E3 60HZ V7.66 (S035)	0	REFERENCE ONLY
401394-0000	LCD GROUNDING WIRE ASSEMBLY E3 REV. A (E780)	1	7
402019-0000	FISH PAPER EL/LCD PWR SUPPLY - E3 REV A (E1352)	1	15
402537-0000	BEZEL - E3A REV. A (E1894)	1	1

358100-0036A	SCR, 4-40 X 1/4, PH PNHD, ZINC OR ANY	7	12
358100-0140A	SCR, PLASTITE, 6 x 1/4~LG, PNH PHL STL ZN PLATE	4	8
358200-0004A	WSHR, #4 FLAT STL ZINC, (.125ID, 9/32OD, .025THK)	4	10
358200-0006A	WSHR, #6 FLT STL ZINC	4	16
358200-0009A	WSHR, #4 SPLIT LOCK	7	11
358200-0010A	WSHR, #6 SPLT LCK	4	18
360500-0023A	NUT, #6 HEX, LRG PTRN	4	19
362000-0032A	ELECTROLUMINESCENT DISPLAY	1	7
370101-0113A	RES, 11K, 1/8W, 5%, CF TAPE & REEL	1	R21
401081-0000	MEMBRANE E3 MONITOR REV. F (E1982)	1	2
401986-0000	PCBA, E3 ELECTROLUMIN DISPLAY DRVR REV D1 (D524)	1	20
401988-0000	PCBA, E3 ELECTROLUMINESCENT INTERFACE REV C (E1837)	1	3
402014-0000	MTG PLATE EL DISPLAY - E3 REV. A (E1352)	1	4
402017-0000	FILTER, POLARIZED EL DISPLAY - E3 REV D (E2094)	1	5
402018-0000	FLEXSTRIP, 14-POS, 1.25mm PITCH, 6.5IN LG REV C (E1947)	2	6
402019-0000	FISH PAPER EL/LCD PWR SUPPLY - E3 REV A (E1352)	2	21
402067-0000	ROM, E3EL CPU 60HZ 110V SINGLE CHANNEL 7.66 (S035)	0	REF ONLY
402336-0000	E3/E3N EL POWER SUPPLY ASSY REV A (E1671)	1	22
402360-0000	E3/E3B EL FLTR MTG FRAME REV C (E2032)	1	23
402537-0000	BEZEL - E3A REV. A (E1894)	1	1

ESCORT 300A

**AR42 RECORDER ASSEMBLY
PARTS LISTING**

P/N 500124

366000-0008A	THERM.RCDR.PAPER,50MM WIDE, NO GRID, KANZAKI C692	1	-
366000-0015A	RECORDER, MODEL AR42 **(FIFO)**	1	1
401314-0000	CBL, AR42 RECORDER REV. C (E1344)	1	2



Medical Data Electronics • 12720 Wentworth Street • Arleta, California 91331-4329
(800) 237-5243 • (818) 768-6411 • FAX (818) 768-0759